

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101620\
 Data File : FB025082.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2020 13:17
 Operator : DD/AJ
 Sample : L4218-02MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 17 00:16:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	452034	21.531 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	747433	24.854 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	743369	24.322 ng/ml
3) t n-Heptane	7.759	237394	7.803 ng/ml
4) t Benzene	7.893	362763	9.738 ng/ml
6) t Toluene	10.631	981400	28.113 ng/ml
7) t Ethylbenzene	13.070	292306	9.018 ng/ml
8) t m-Xylene	13.204	583052	18.355 ng/ml
9) t O-Xylene	13.931	574308	18.899 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	447052	17.626 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101620\
Data File : FB025082.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2020 13:17
Operator : DD/AJ
Sample : L4218-02MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 17 00:16:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

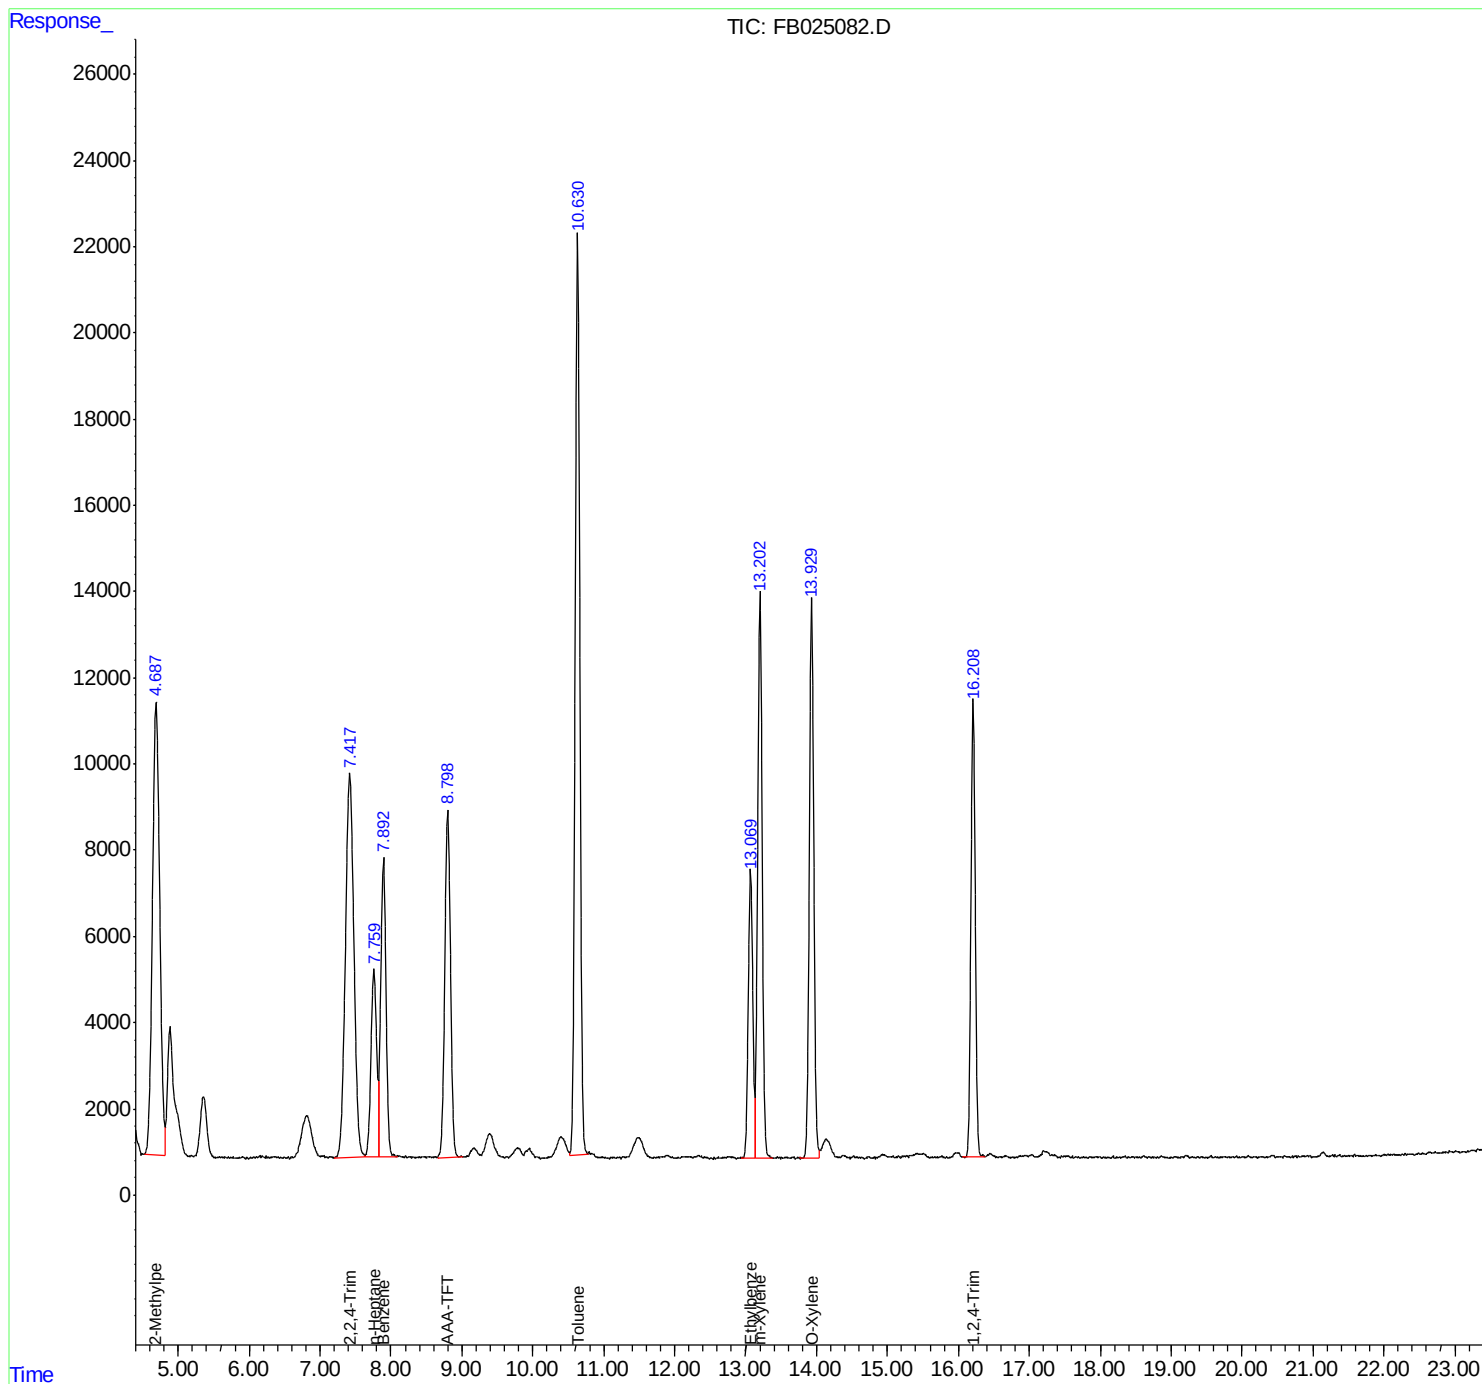

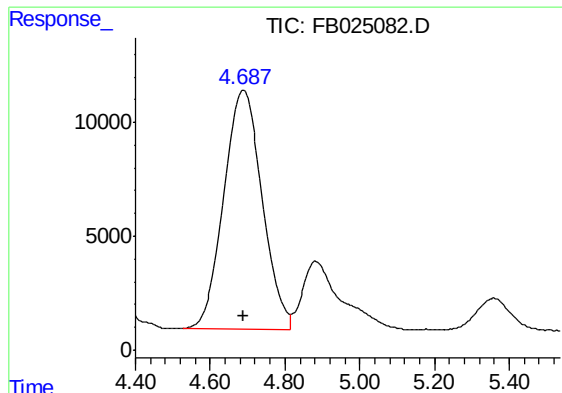


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 747433
Conc: 24.85 ng/ml

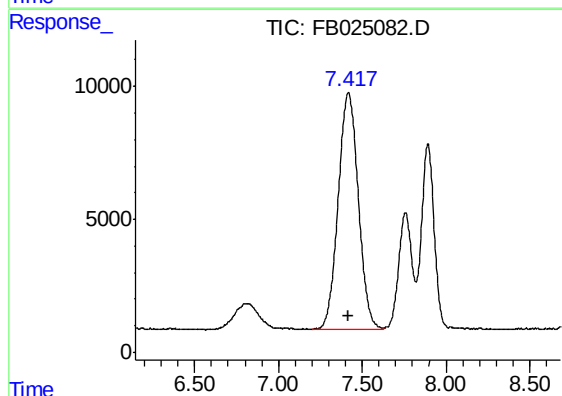


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 743369
Conc: 24.32 ng/ml

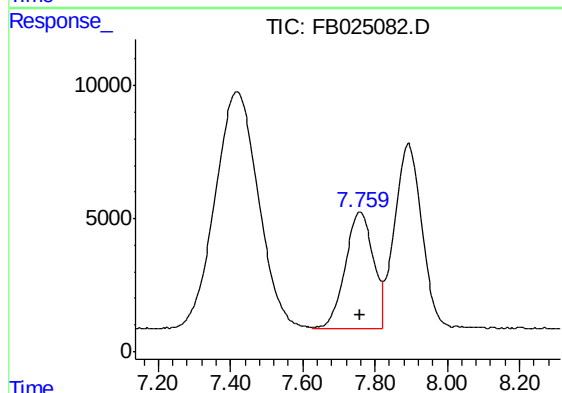


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 237394
Conc: 7.80 ng/ml

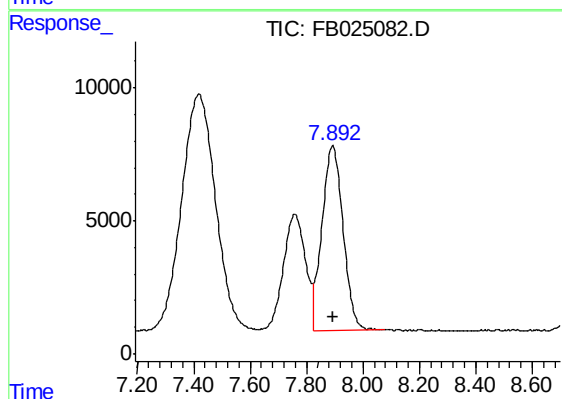


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 362763
Conc: 9.74 ng/ml

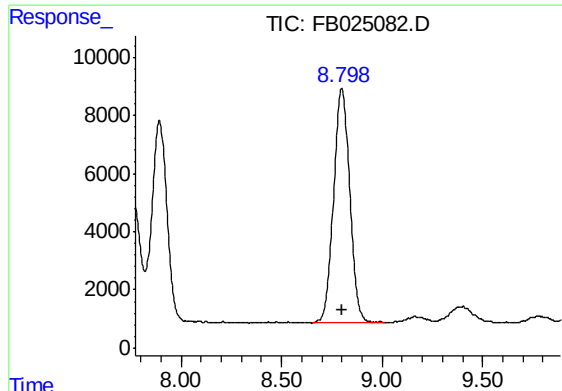


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 452034
Conc: 21.53 ng/ml

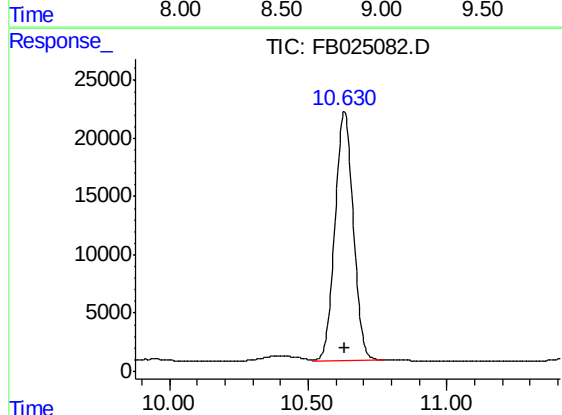


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 981400
Conc: 28.11 ng/ml

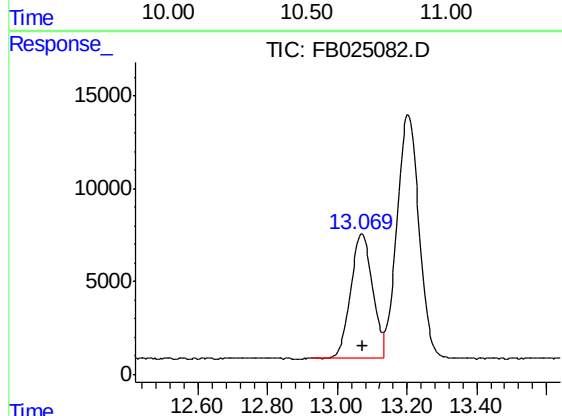


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 292306
Conc: 9.02 ng/ml

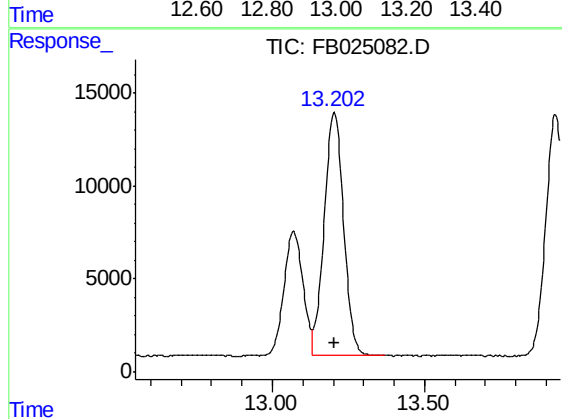


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 583052
Conc: 18.35 ng/ml

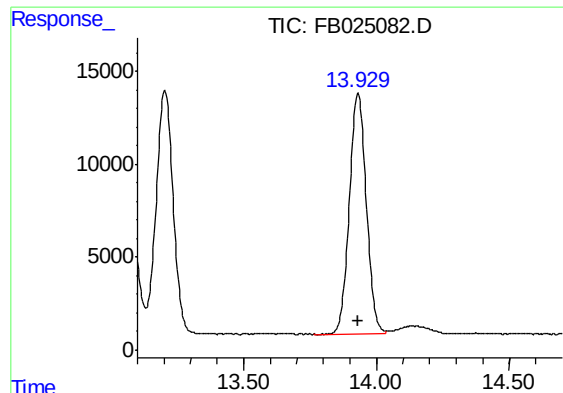

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.001 min
Response: 574308
Conc: 18.90 ng/ml

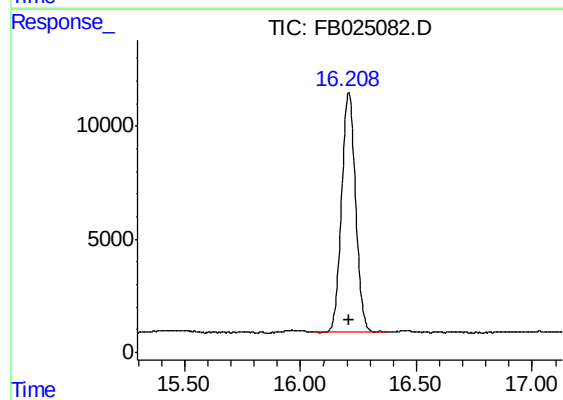

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 447052
Conc: 17.63 ng/ml