

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101620\
 Data File : FB025081.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2020 12:46
 Operator : DD/AJ
 Sample : L4218-02MS
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 17 00:16:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	446995	21.291 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	771855	25.666 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	789673	25.837 ng/ml
3) t n-Heptane	7.759	253097	8.320 ng/ml
4) t Benzene	7.894	364931	9.796 ng/ml
6) t Toluene	10.631	985125	28.219 ng/ml
7) t Ethylbenzene	13.071	291518	8.993 ng/ml
8) t m-Xylene	13.204	581979	18.321 ng/ml
9) t O-Xylene	13.931	563926	18.558 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	453713	17.889 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101620\
Data File : FB025081.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2020 12:46
Operator : DD/AJ
Sample : L4218-02MS
Misc : 5.03/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 17 00:16:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

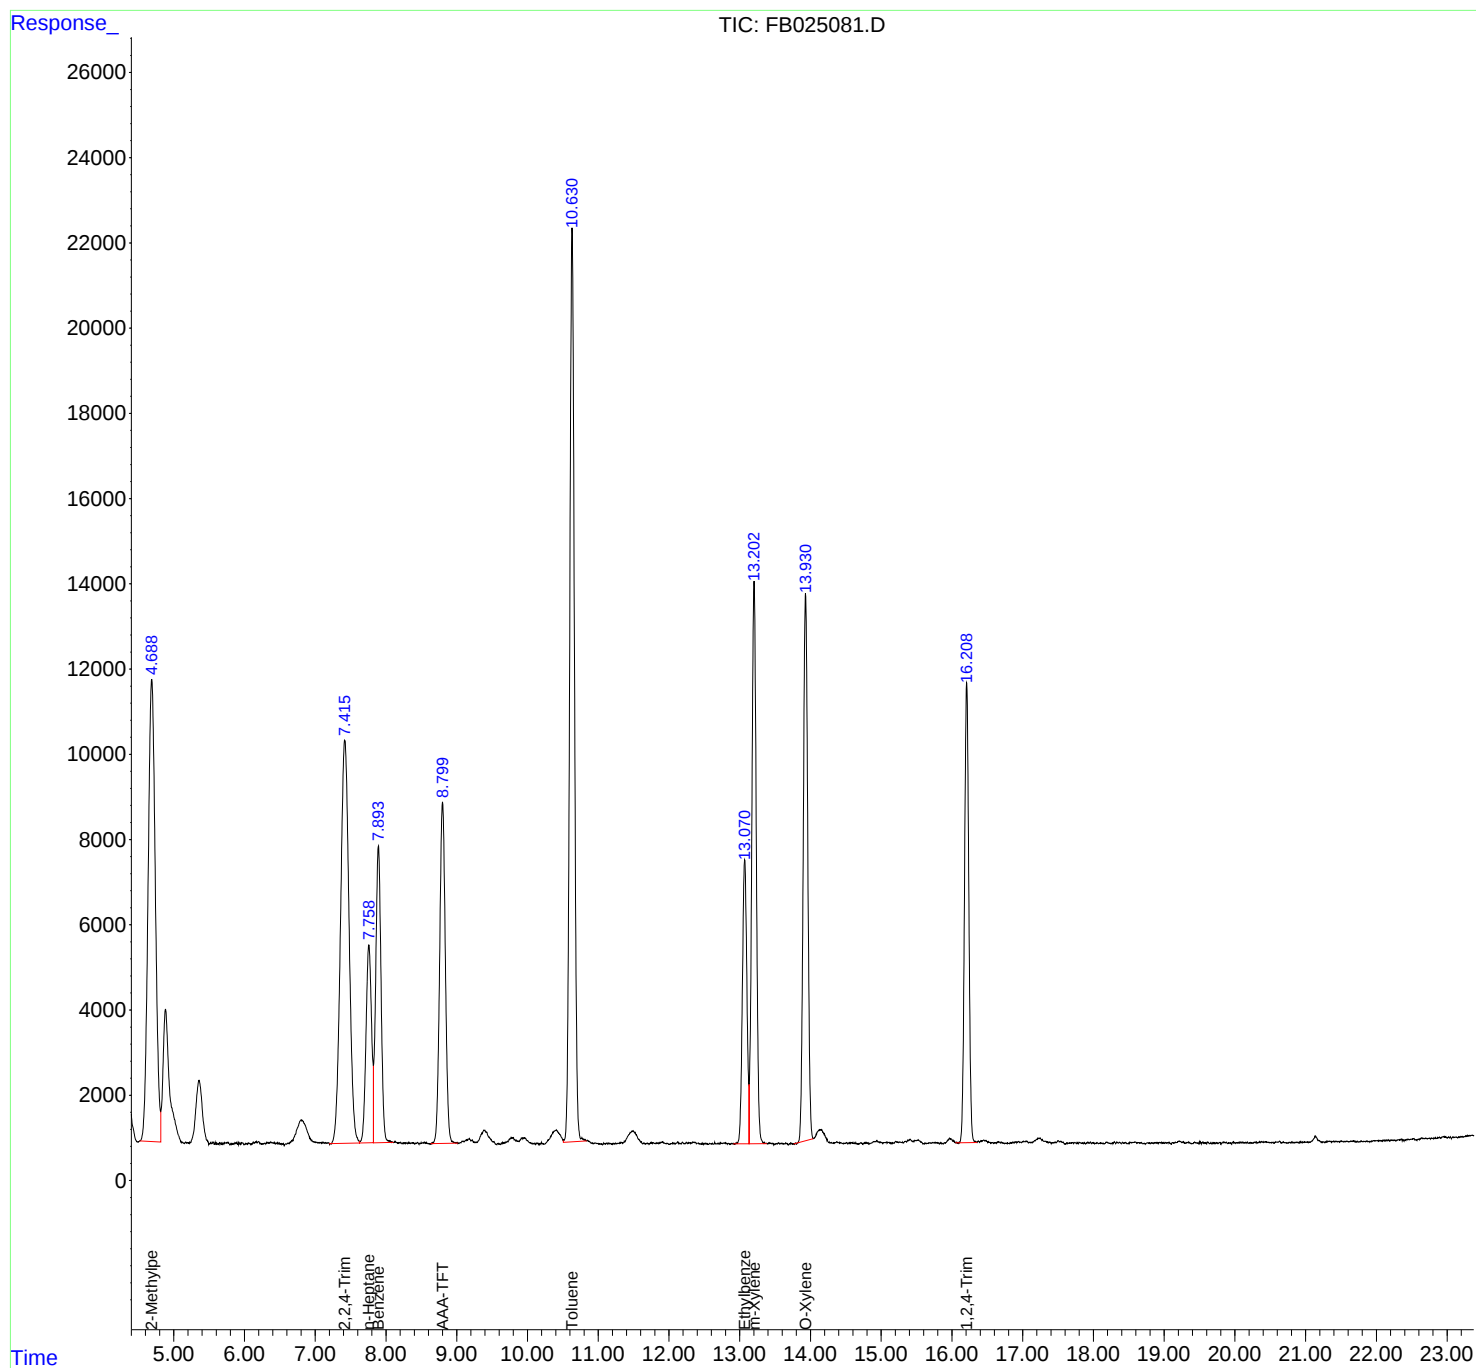

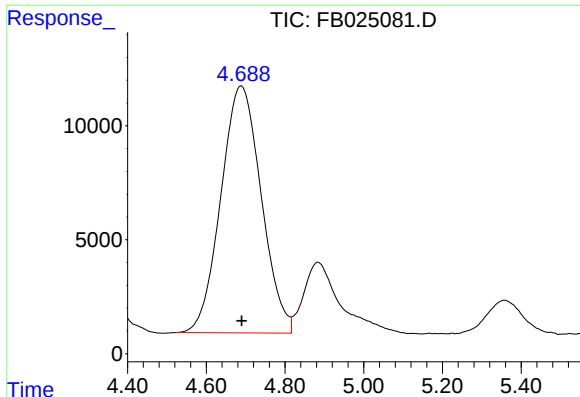


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 771855
Conc: 25.67 ng/ml

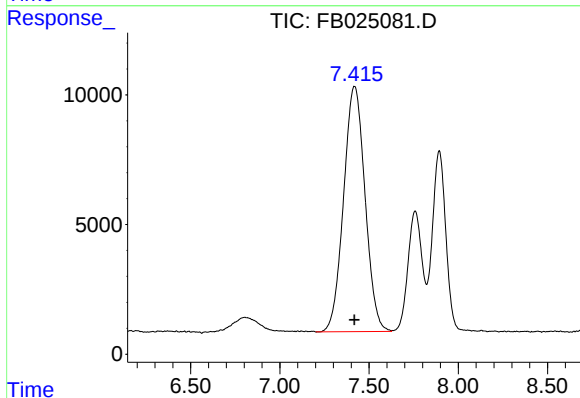


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 789673
Conc: 25.84 ng/ml

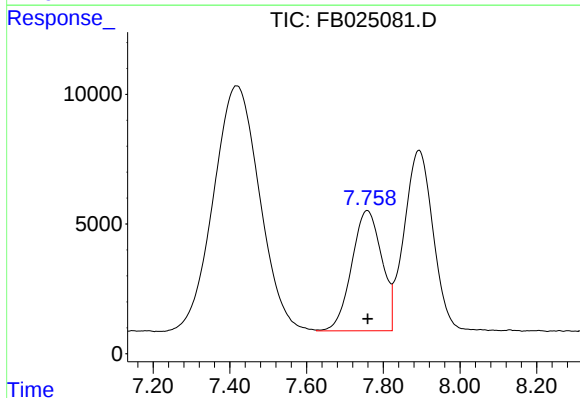


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 253097
Conc: 8.32 ng/ml

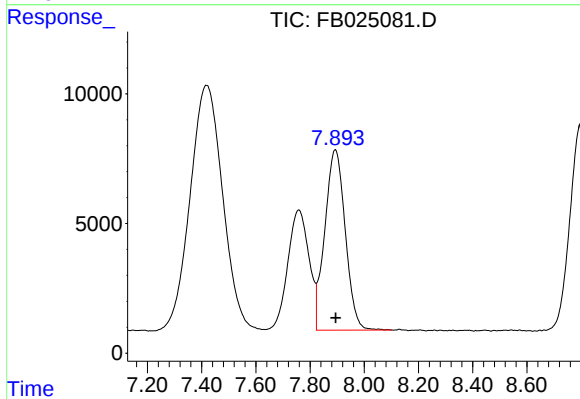


#4 Benzene

R.T.: 7.894 min
Delta R.T.: -0.001 min
Response: 364931
Conc: 9.80 ng/ml

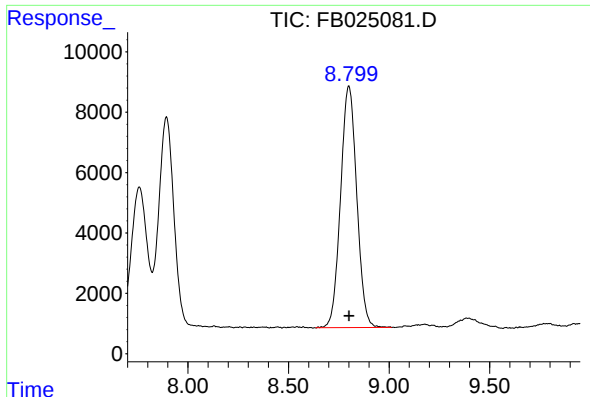


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 446995
Conc: 21.29 ng/ml

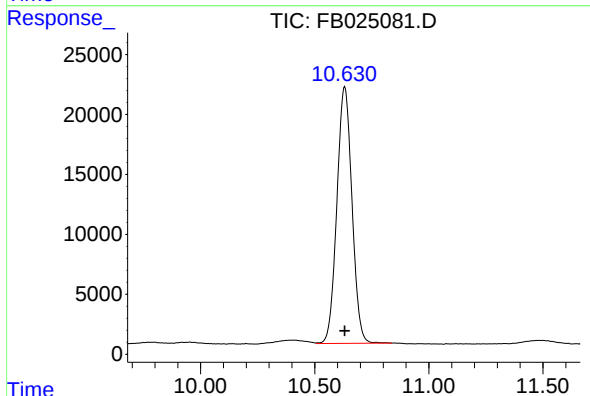


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 985125
Conc: 28.22 ng/ml

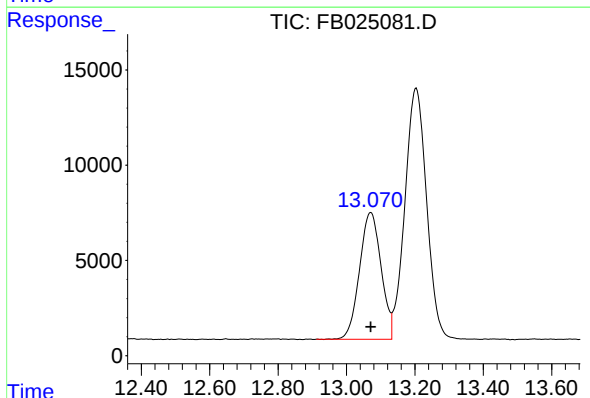


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 291518
Conc: 8.99 ng/ml

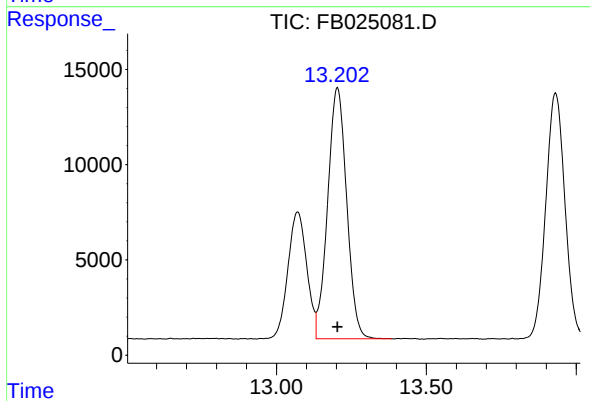


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 581979
Conc: 18.32 ng/ml

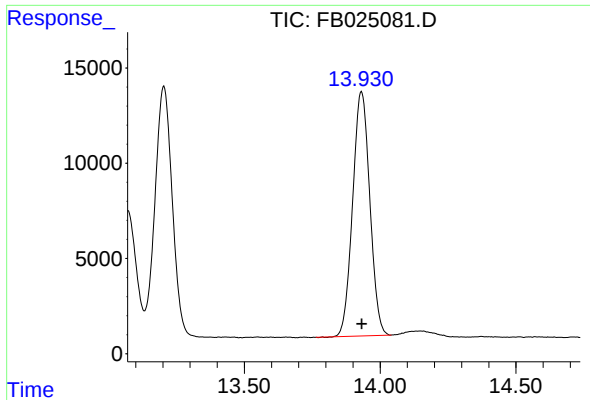

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 563926
Conc: 18.56 ng/ml

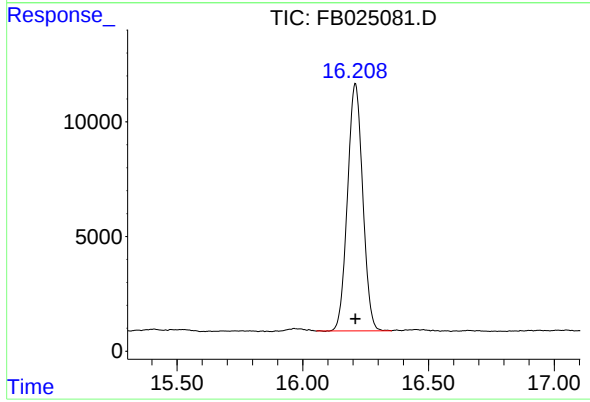

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 453713
Conc: 17.89 ng/ml