

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101718\
 Data File : FB018255.D
 Signal(s) : FID2B.CH
 Acq On : 17 Oct 2018 9:28
 Operator : MJ/SJ
 Sample : BSF1017S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 17 15:43:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.108	148829	17.280 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.959	431051	28.184 ng/ml
2) t	2,2,4-Trimethylpentane	7.725	437689	29.620 ng/ml
3) t	n-Heptane	8.062	142547	10.059 ng/ml
4) t	Benzene	8.203	179199	9.620 ng/ml
6) t	Toluene	10.957	435711	28.589 ng/ml
7) t	Ethylbenzene	13.407	147582	9.302 ng/ml
8) t	m-Xylene	13.539	314571	18.906 ng/ml
9) t	O-Xylene	14.271	330064	18.512 ng/ml
10) t	1,2,4-Trimethylbenzene	16.554	388441	19.094 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101718\
Data File : FB018255.D
Signal(s) : FID2B.CH
Acq On : 17 Oct 2018 9:28
Operator : MJ/SJ
Sample : BSF1017S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 17 15:43:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

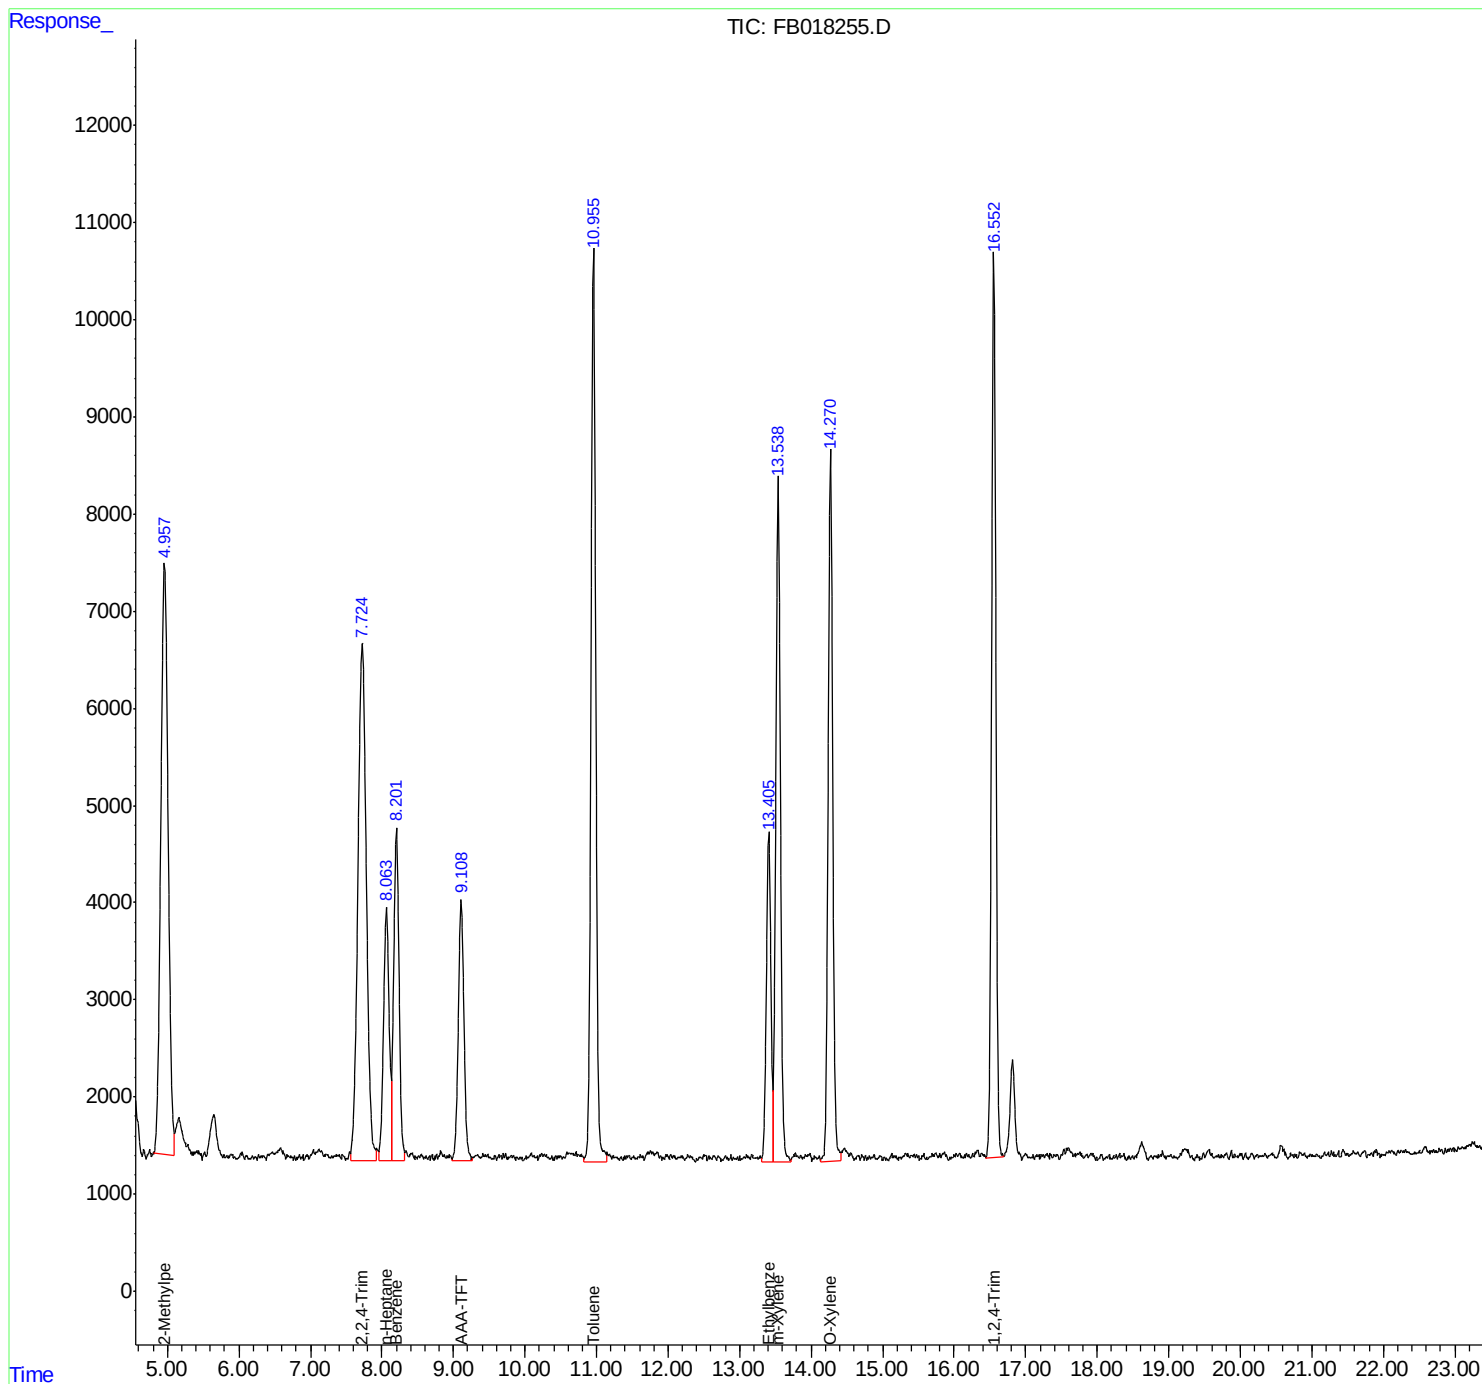

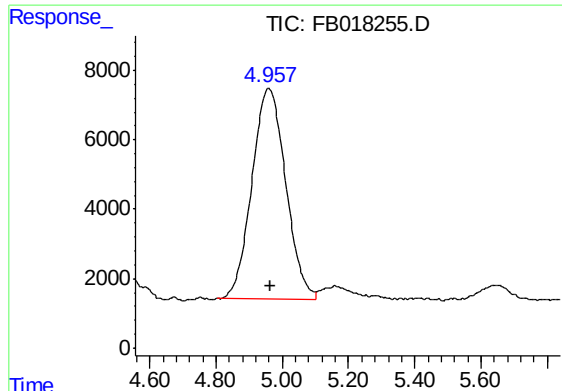


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 431051
Conc: 28.18 ng/ml

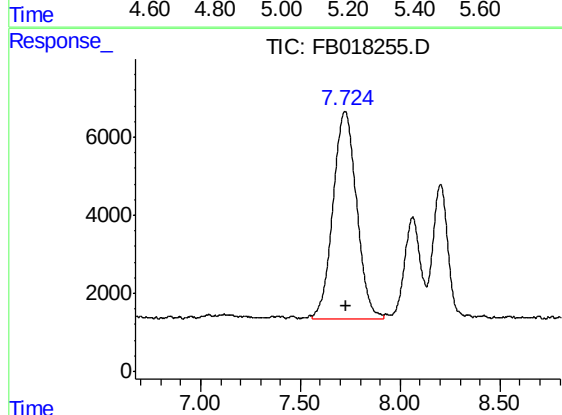


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.004 min
Response: 437689
Conc: 29.62 ng/ml

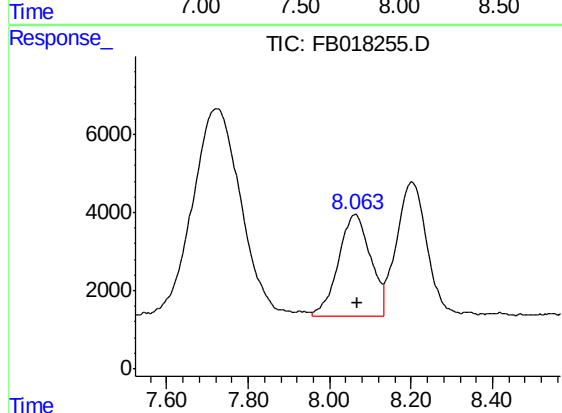


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.005 min
Response: 142547
Conc: 10.06 ng/ml

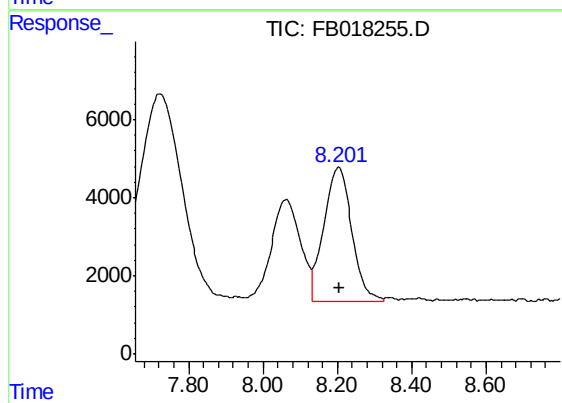


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 179199
Conc: 9.62 ng/ml

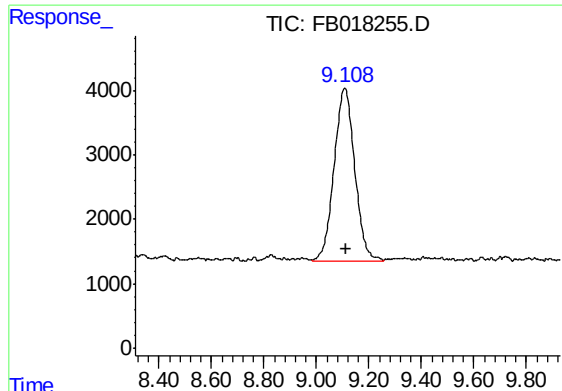


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 148829
Conc: 17.28 ng/ml

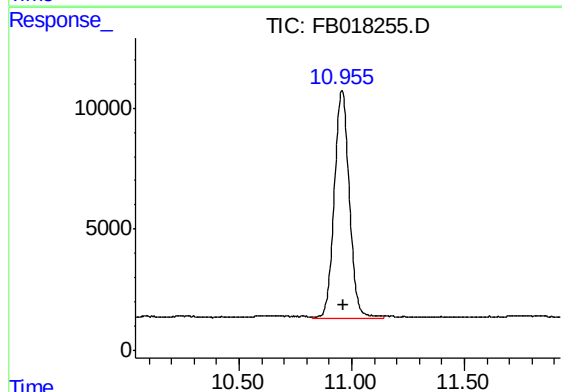


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.005 min
Response: 435711
Conc: 28.59 ng/ml

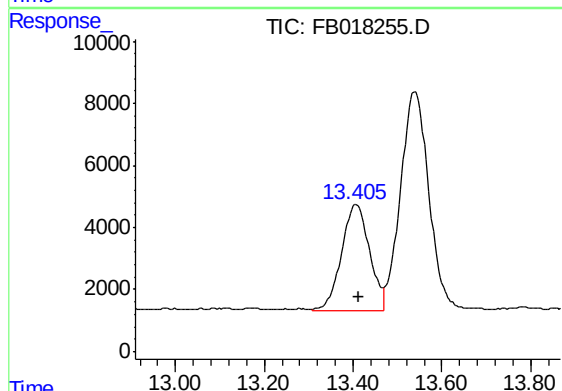


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.005 min
Response: 147582
Conc: 9.30 ng/ml

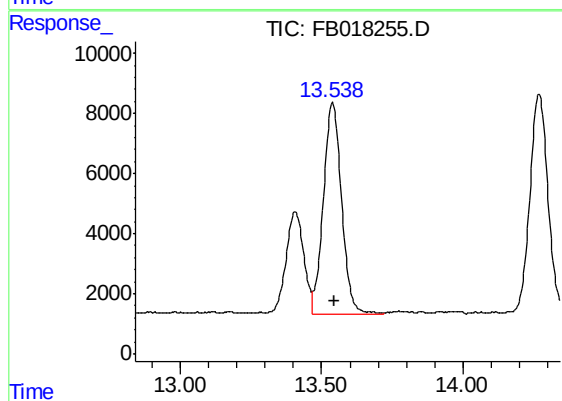


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.005 min
Response: 314571
Conc: 18.91 ng/ml

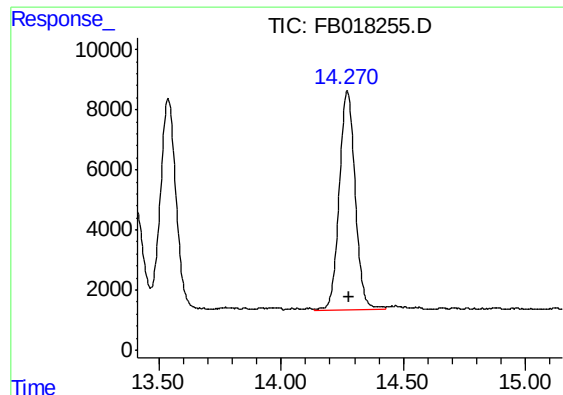

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.006 min
Response: 330064
Conc: 18.51 ng/ml

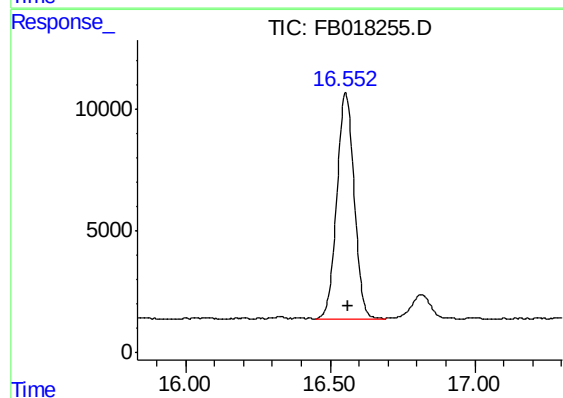

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.005 min
Response: 388441
Conc: 19.09 ng/ml