

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101719\
 Data File : FB022768.D
 Signal(s) : FID2B.CH
 Acq On : 18 Oct 2019 1:40
 Operator : DD/AJ
 Sample : K5436-02MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 3425-28MSD

Integration File: Calibration.e
 Quant Time: Oct 18 02:18:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	475875	18.806 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	699767	20.591 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	685613	18.842 ng/ml
3) t n-Heptane	7.758	206004	5.646 ng/ml
4) t Benzene	7.892	345459	7.824 ng/ml
6) t Toluene	10.631	968432	22.469 ng/ml
7) t Ethylbenzene	13.071	306868	7.555 ng/ml
8) t m-Xylene	13.204	576902	14.994 ng/ml
9) t O-Xylene	13.932	570414	15.661 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	411170	14.429 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101719\
Data File : FB022768.D
Signal(s) : FID2B.CH
Acq On : 18 Oct 2019 1:40
Operator : DD/AJ
Sample : K5436-02MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
3425-28MSD

Integration File: Calibration.e
Quant Time: Oct 18 02:18:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

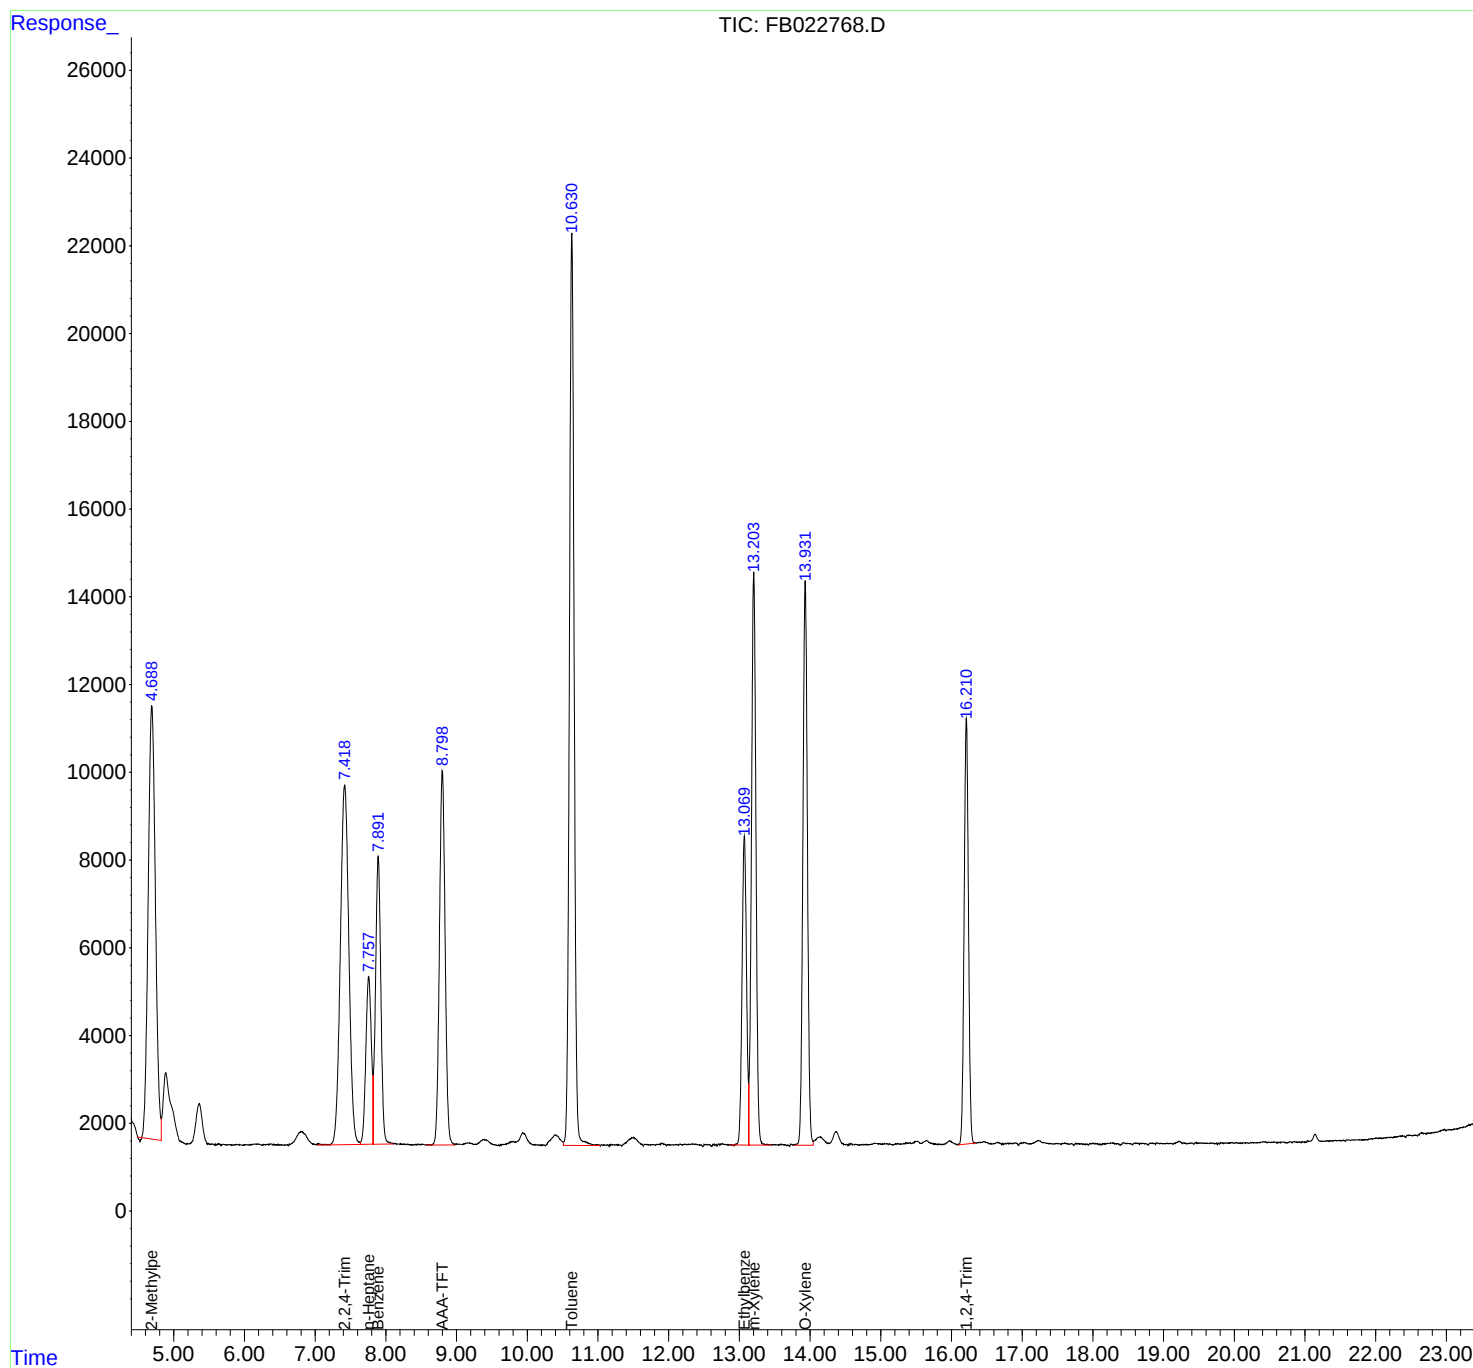


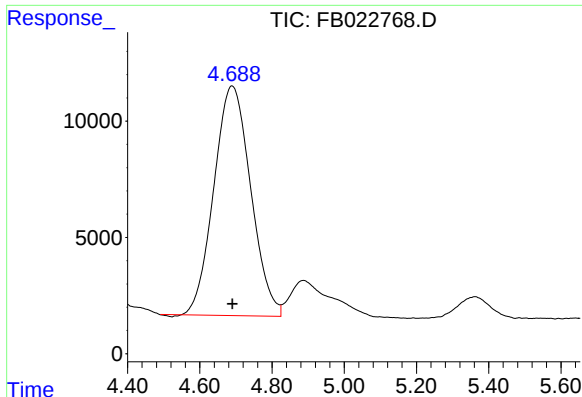

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 699767
Conc: 20.59 ng/ml

Instrument :
FID_B
ClientSampleId :
3425-28MSD

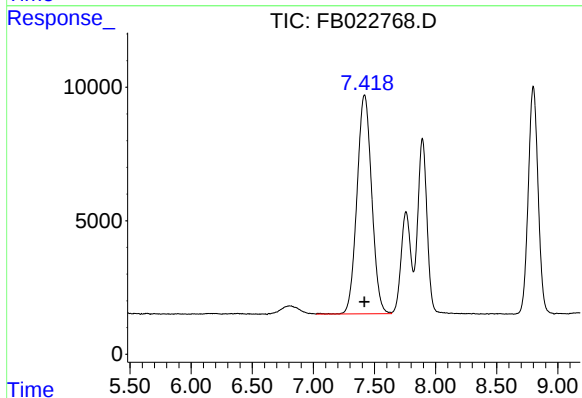


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 685613
Conc: 18.84 ng/ml

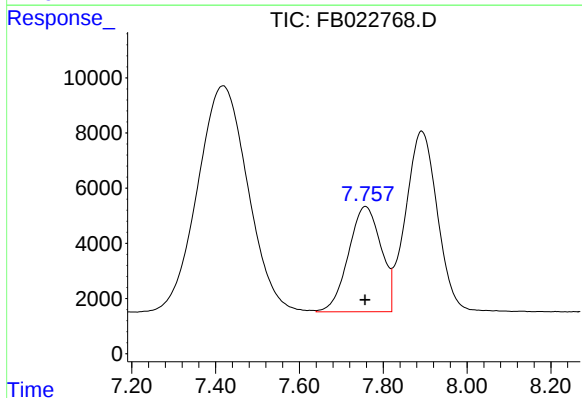


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 206004
Conc: 5.65 ng/ml

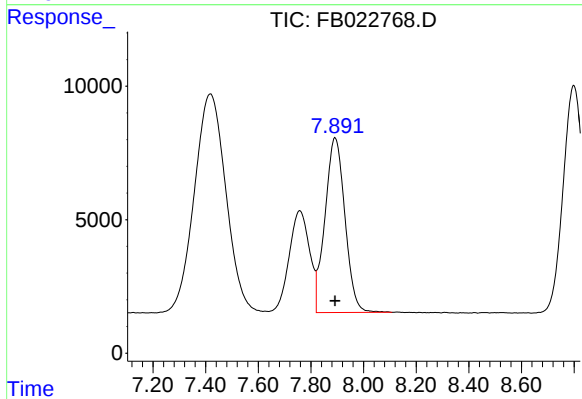

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 345459
Conc: 7.82 ng/ml

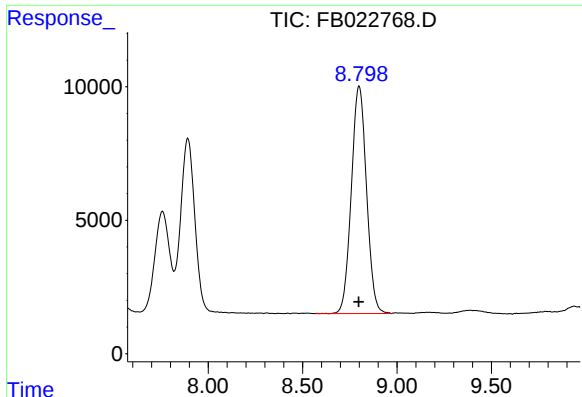

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.001 min
Response: 475875
Conc: 18.81 ng/ml

Instrument :
FID_B
ClientSampleId :
3425-28MSD

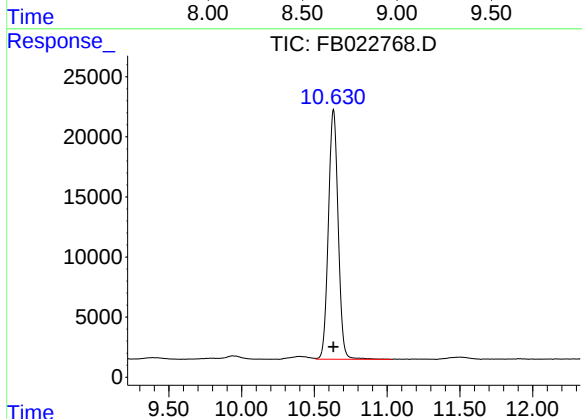


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.001 min
Response: 968432
Conc: 22.47 ng/ml

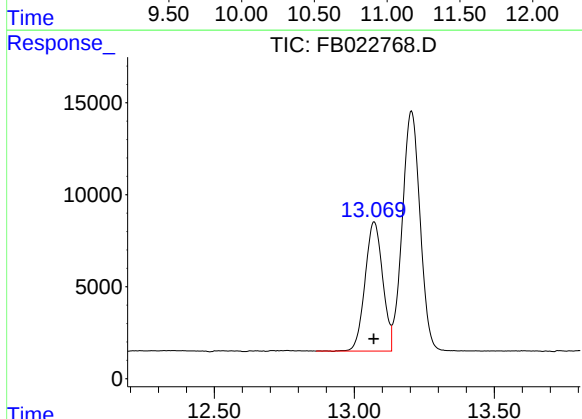


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.001 min
Response: 306868
Conc: 7.56 ng/ml

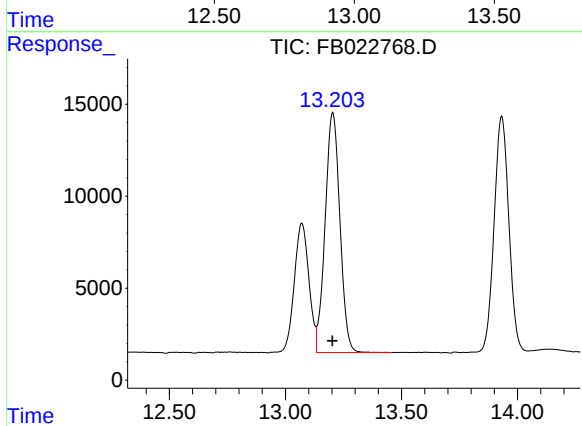

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.001 min
Response: 576902
Conc: 14.99 ng/ml

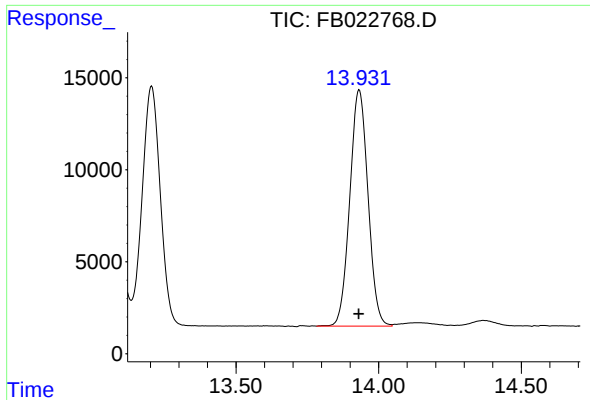

#9 O-Xylene


R.T.: 13.932 min

Delta R.T.: 0.002 min

Response: 570414

Conc: 15.66 ng/ml

Instrument :
FID_B
ClientSampleId :
3425-28MSD

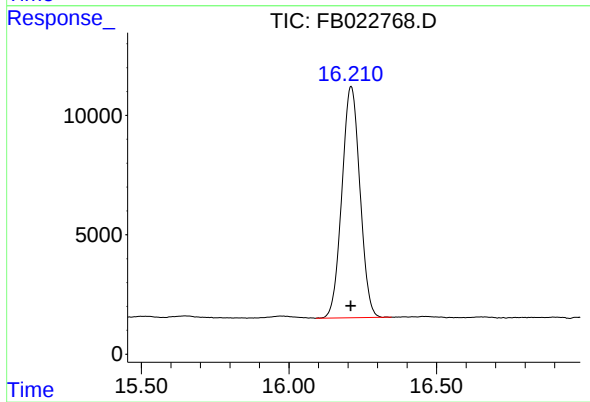

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min

Delta R.T.: 0.001 min

Response: 411170

Conc: 14.43 ng/ml