

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101818\
 Data File : FB018265.D
 Signal(s) : FID2B.CH
 Acq On : 18 Oct 2018 9:08
 Operator : MJ/SJ
 Sample : BSF1018S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 18 11:30:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.103	158673	18.423 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	411177	26.884 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	424729	28.743 ng/ml
3) t n-Heptane	8.059	136057	9.601 ng/ml
4) t Benzene	8.200	169735	9.112 ng/ml
6) t Toluene	10.953	433037	28.413 ng/ml
7) t Ethylbenzene	13.403	156257	9.849 ng/ml
8) t m-Xylene	13.536	328299	19.731 ng/ml
9) t O-Xylene	14.268	340420	19.093 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	387294	19.038 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101818\
Data File : FB018265.D
Signal(s) : FID2B.CH
Acq On : 18 Oct 2018 9:08
Operator : MJ/SJ
Sample : BSF1018S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 18 11:30:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

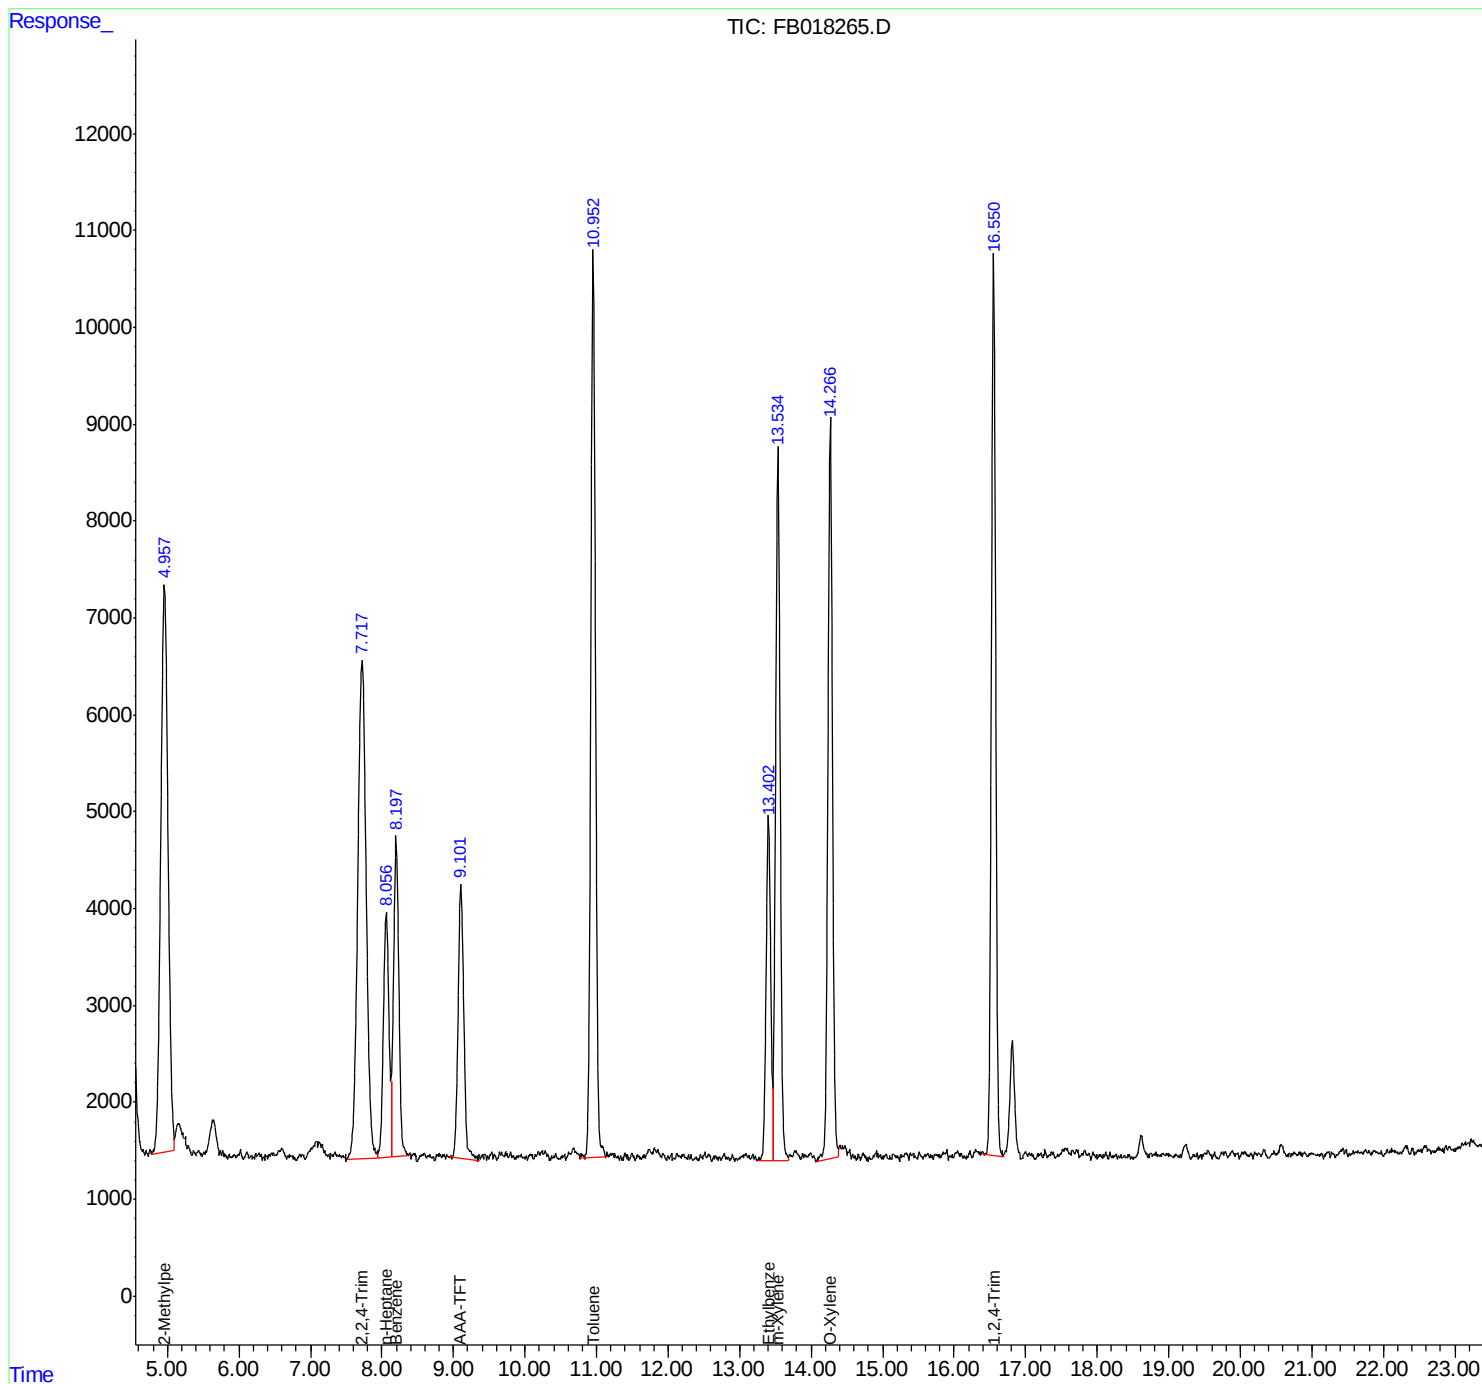

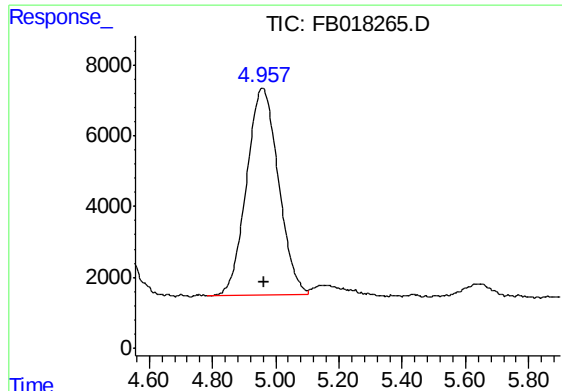


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 411177
Conc: 26.88 ng/ml

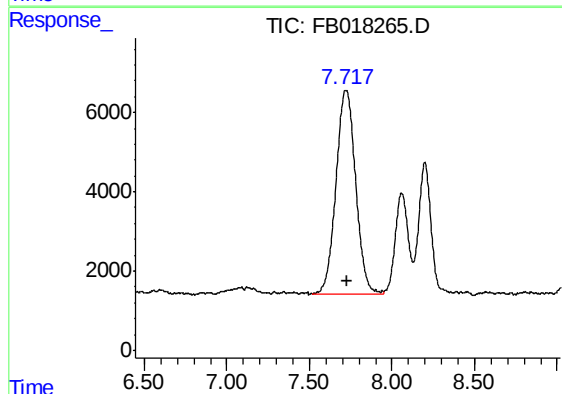


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.009 min
Response: 424729
Conc: 28.74 ng/ml

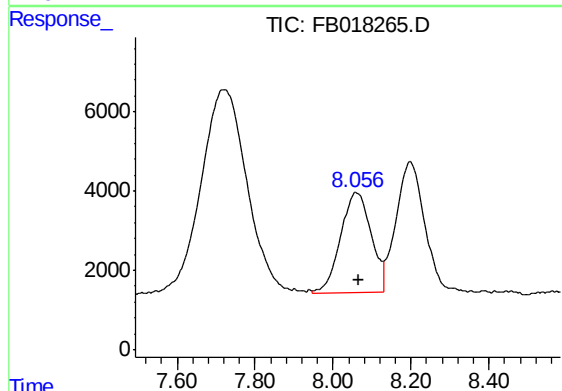


#3 n-Heptane

R.T.: 8.059 min
Delta R.T.: -0.008 min
Response: 136057
Conc: 9.60 ng/ml

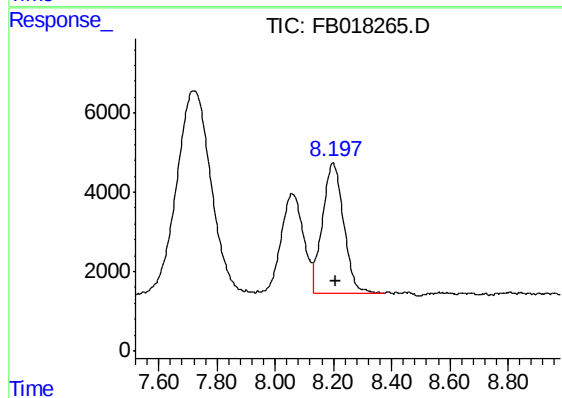


#4 Benzene

R.T.: 8.200 min
Delta R.T.: -0.007 min
Response: 169735
Conc: 9.11 ng/ml

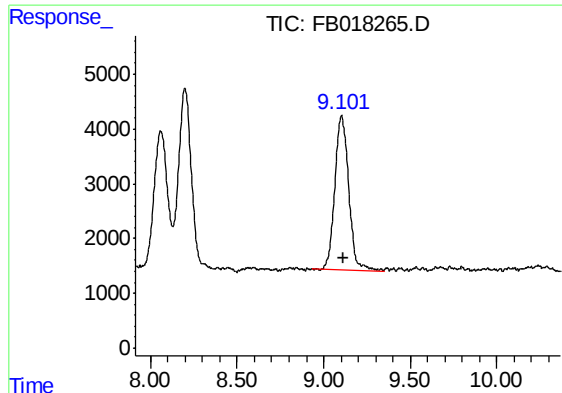


#5 AAA-TFT

R.T.: 9.103 min
Delta R.T.: -0.009 min
Response: 158673
Conc: 18.42 ng/ml

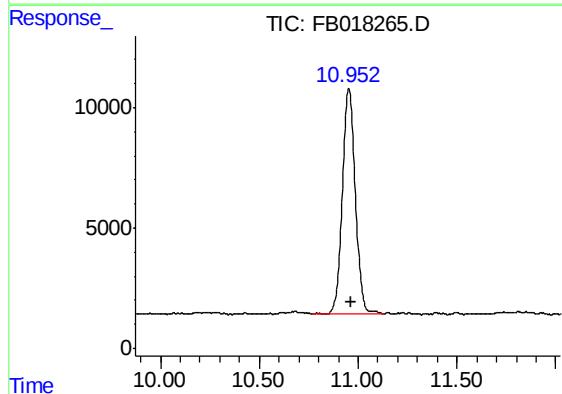


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.009 min
Response: 433037
Conc: 28.41 ng/ml

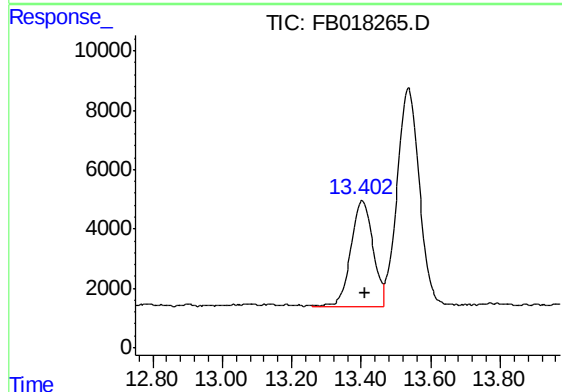


#7 Ethylbenzene

R.T.: 13.403 min
Delta R.T.: -0.009 min
Response: 156257
Conc: 9.85 ng/ml

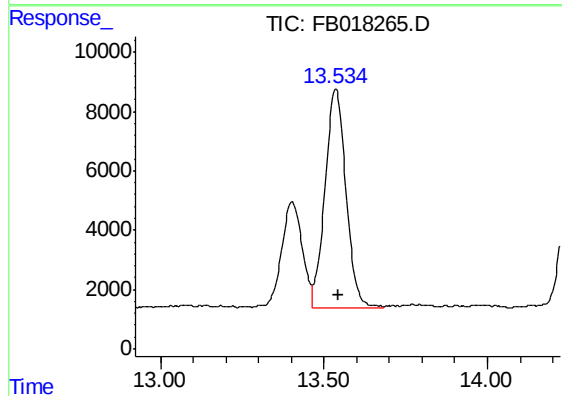


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.008 min
Response: 328299
Conc: 19.73 ng/ml

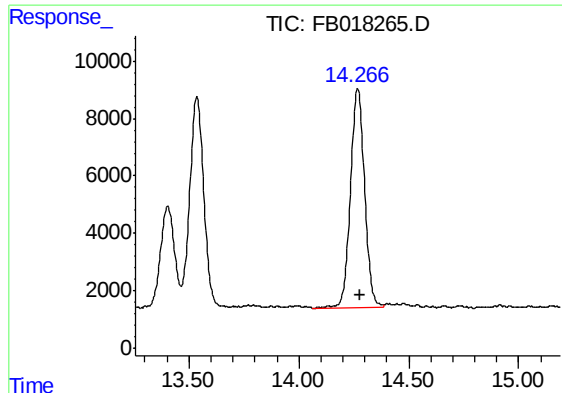

#9 O-Xylene

R.T.: 14.268 min
Delta R.T.: -0.009 min
Response: 340420
Conc: 19.09 ng/ml

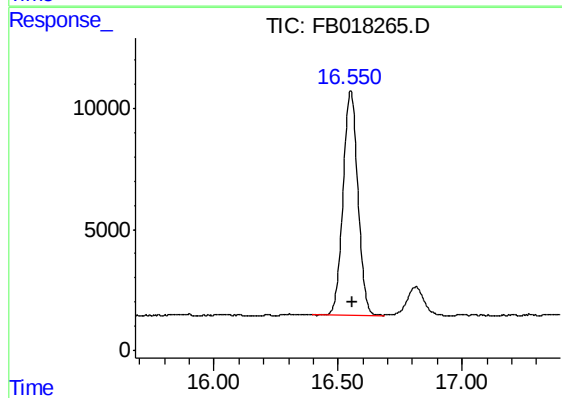

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.008 min
Response: 387294
Conc: 19.04 ng/ml