

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101818\
 Data File : FB018279.D
 Signal(s) : FID2B.CH
 Acq On : 18 Oct 2018 16:09
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 18 16:29:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	177190	20.573 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	483893	31.639 ng/ml
2) t 2,2,4-Trimethylpentane	7.722	480769	32.536 ng/ml
3) t n-Heptane	8.062	156533	11.046 ng/ml
4) t Benzene	8.202	200335	10.754 ng/ml
6) t Toluene	10.956	499810	32.794 ng/ml
7) t Ethylbenzene	13.405	165517	10.432 ng/ml
8) t m-Xylene	13.538	350367	21.057 ng/ml
9) t O-Xylene	14.270	371836	20.855 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	430301	21.152 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101818\
Data File : FB018279.D
Signal(s) : FID2B.CH
Acq On : 18 Oct 2018 16:09
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.03g/5.00mL DI Water
ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 18 16:29:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

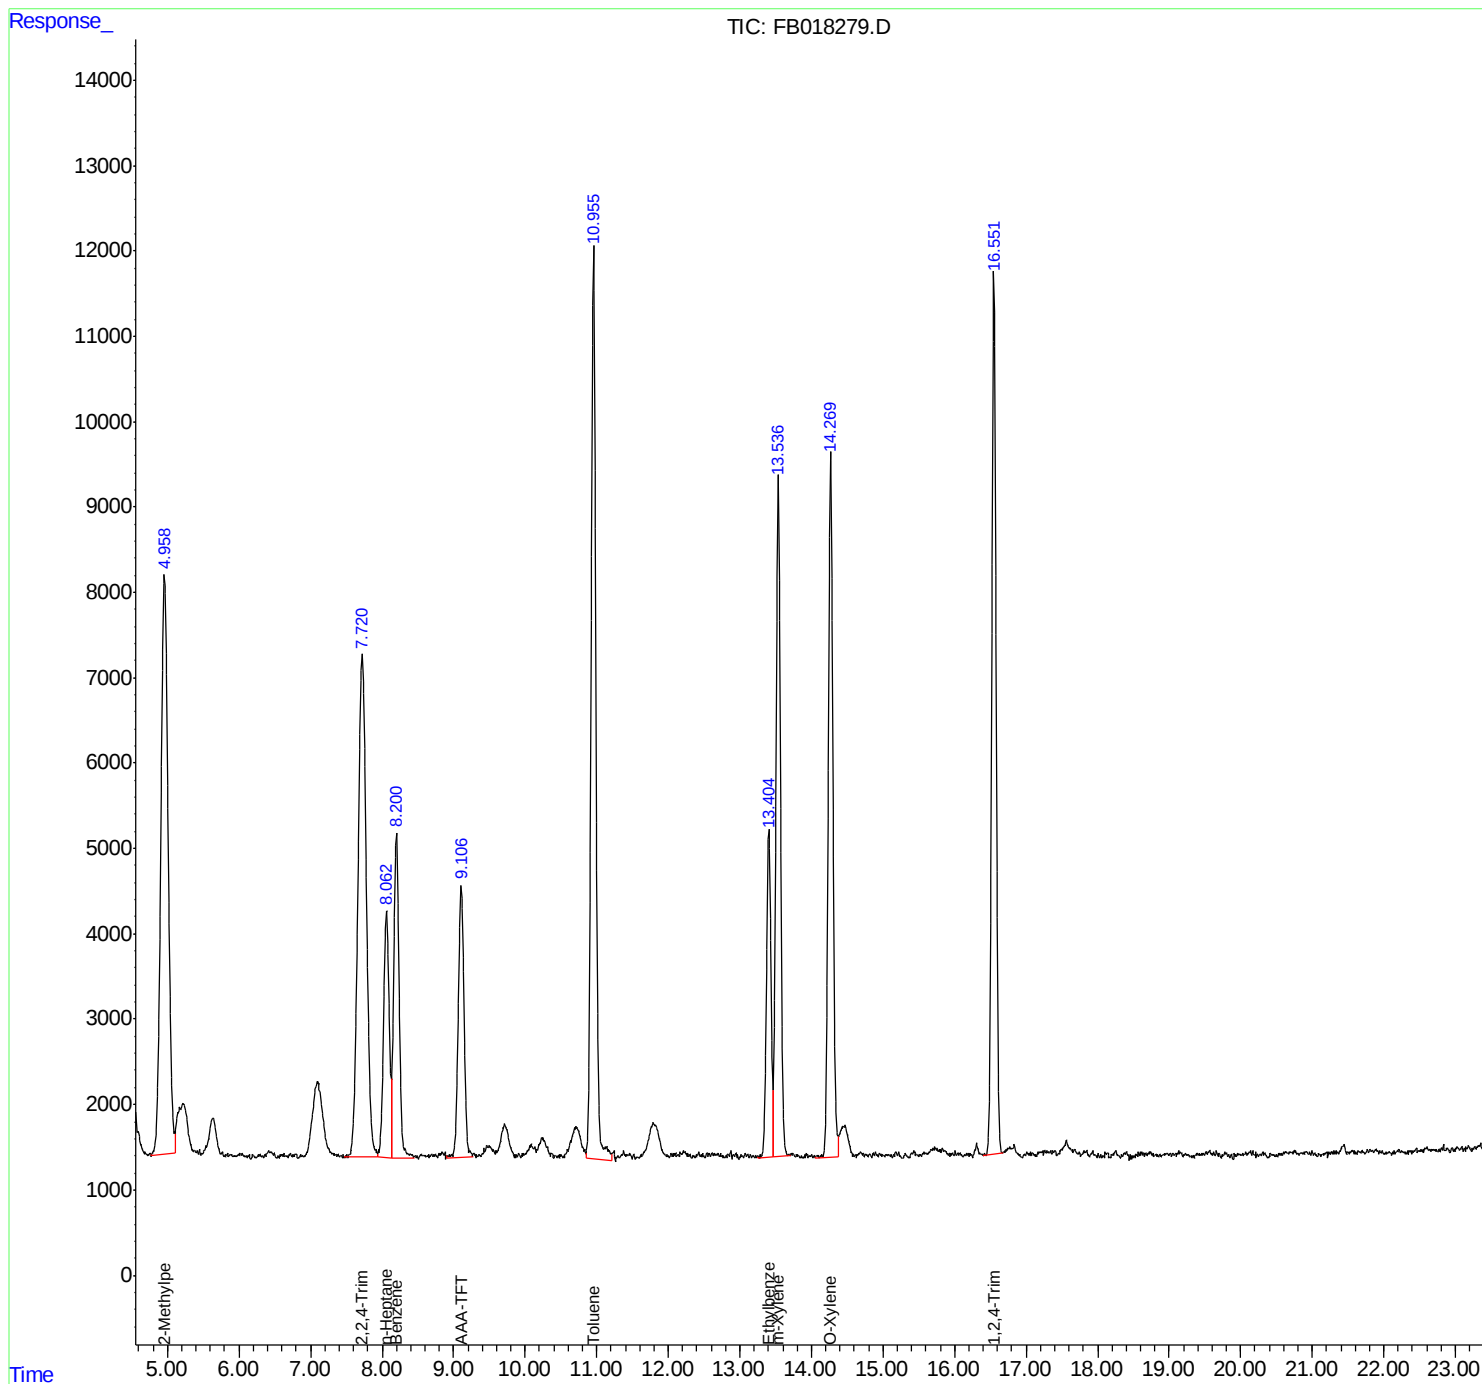

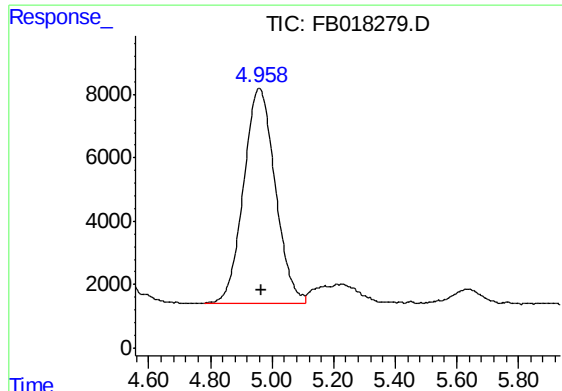


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 483893
Conc: 31.64 ng/ml

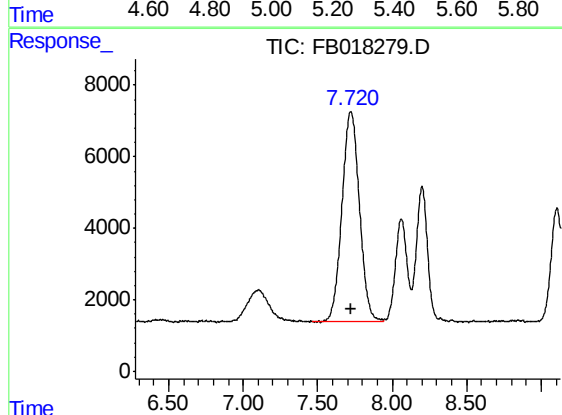


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: -0.007 min
Response: 480769
Conc: 32.54 ng/ml

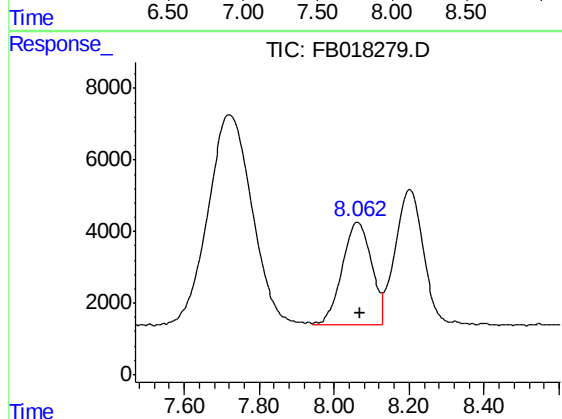


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.005 min
Response: 156533
Conc: 11.05 ng/ml

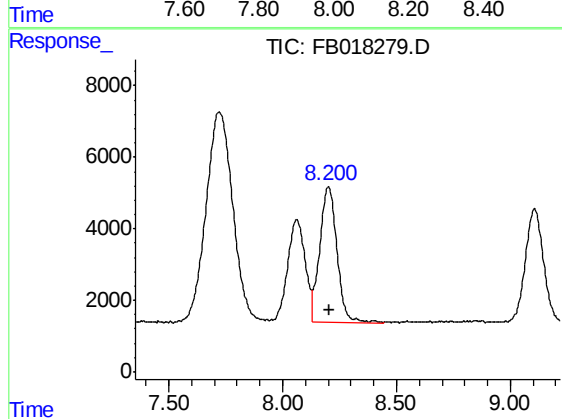


#4 Benzene

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 200335
Conc: 10.75 ng/ml

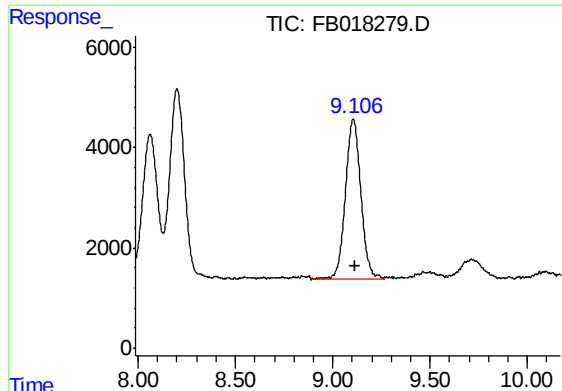


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.006 min
Response: 177190
Conc: 20.57 ng/ml

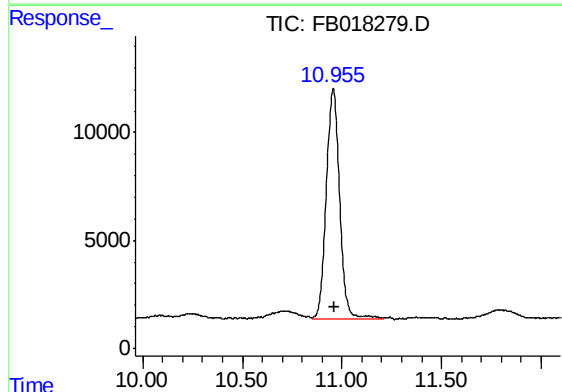


#6 Toluene

R.T.: 10.956 min
Delta R.T.: -0.006 min
Response: 499810
Conc: 32.79 ng/ml

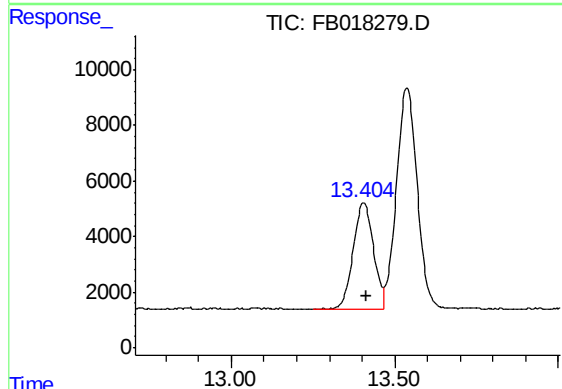


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: -0.007 min
Response: 165517
Conc: 10.43 ng/ml

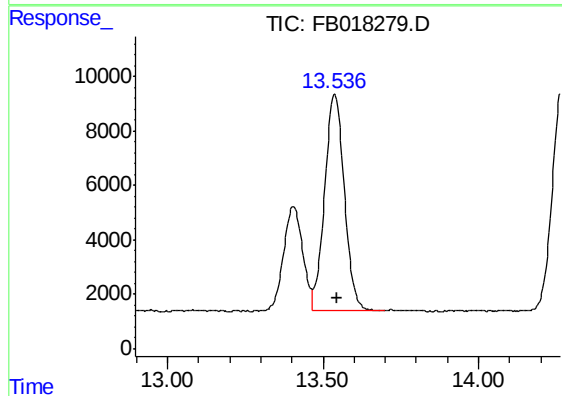


#8 m-Xylene

R.T.: 13.538 min
Delta R.T.: -0.007 min
Response: 350367
Conc: 21.06 ng/ml

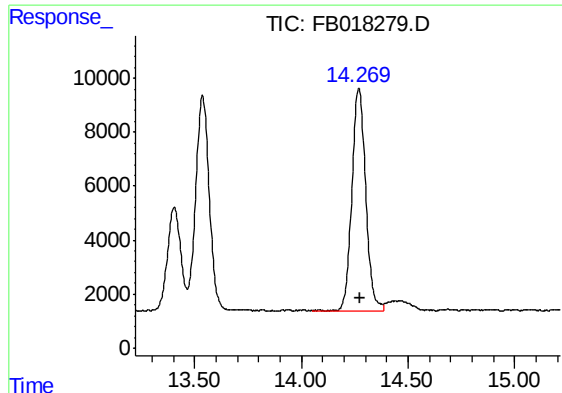

#9 O-Xylene

R.T.: 14.270 min
Delta R.T.: -0.007 min
Response: 371836
Conc: 20.85 ng/ml

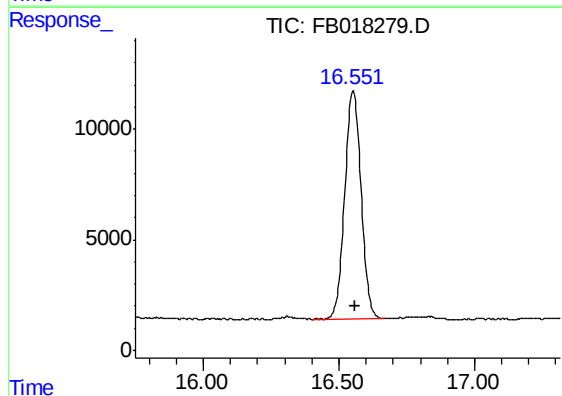

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: -0.007 min
Response: 430301
Conc: 21.15 ng/ml