

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101819\
 Data File : FB022772.D
 Signal(s) : FID2B.CH
 Acq On : 18 Oct 2019 19:10
 Operator : DD/AJ
 Sample : BSF1018S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 19 00:22:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	511371	20.209 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	1016198	29.902 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	1123990	30.890 ng/ml
3) t n-Heptane	7.755	371364	10.178 ng/ml
4) t Benzene	7.889	435895	9.873 ng/ml
6) t Toluene	10.628	1261233	29.263 ng/ml
7) t Ethylbenzene	13.068	392328	9.660 ng/ml
8) t m-Xylene	13.201	734355	19.086 ng/ml
9) t O-Xylene	13.929	696426	19.121 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	558018	19.583 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101819\
Data File : FB022772.D
Signal(s) : FID2B.CH
Acq On : 18 Oct 2019 19:10
Operator : DD/AJ
Sample : BSF1018S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 19 00:22:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

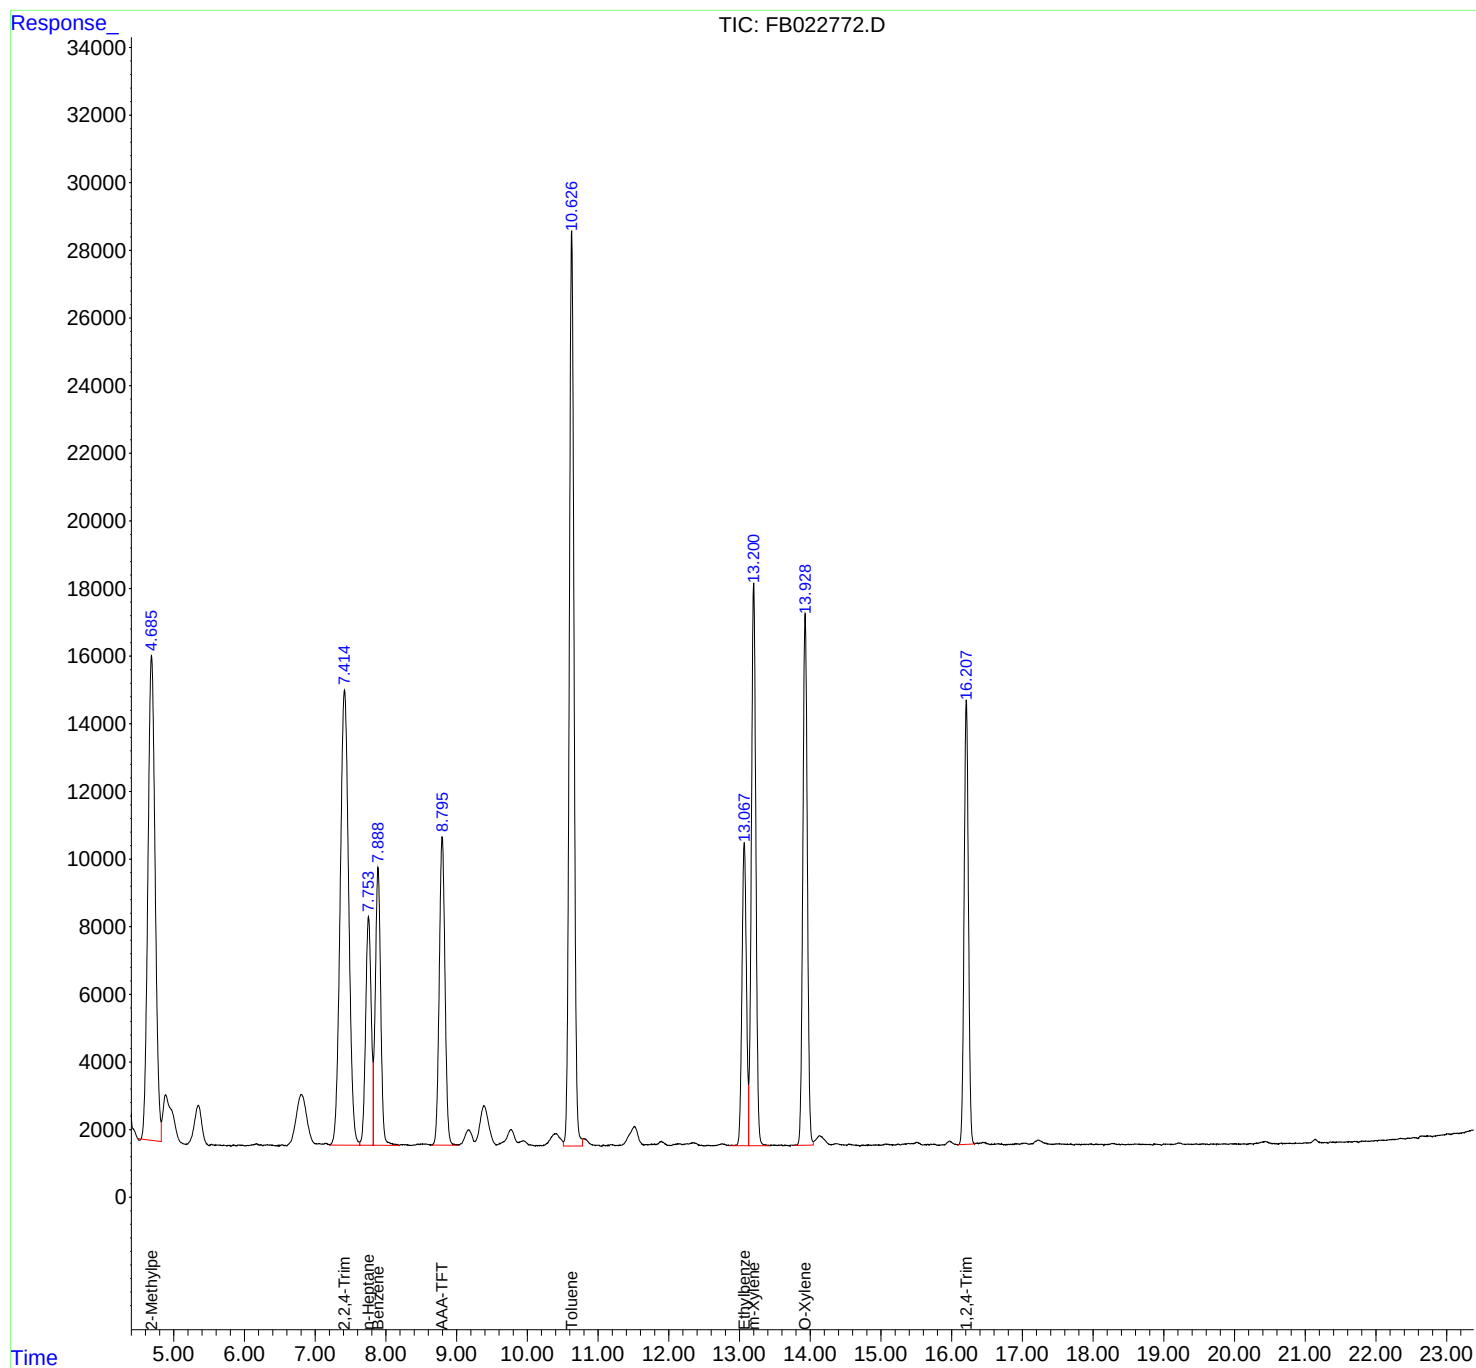

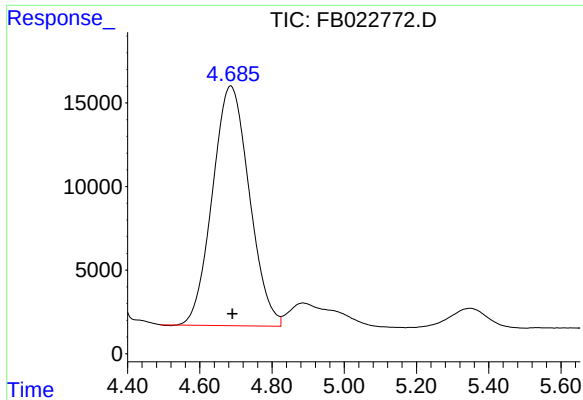


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.004 min
Response: 1016198
Conc: 29.90 ng/ml

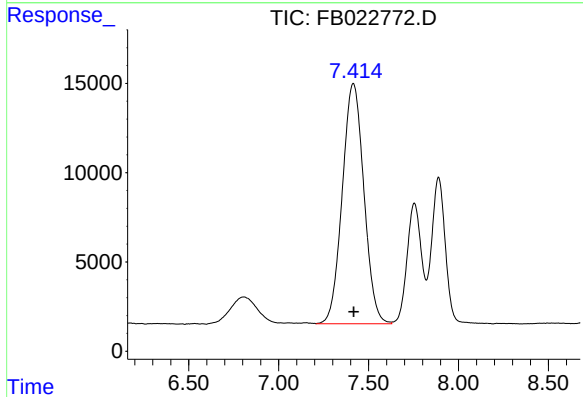


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 1123990
Conc: 30.89 ng/ml

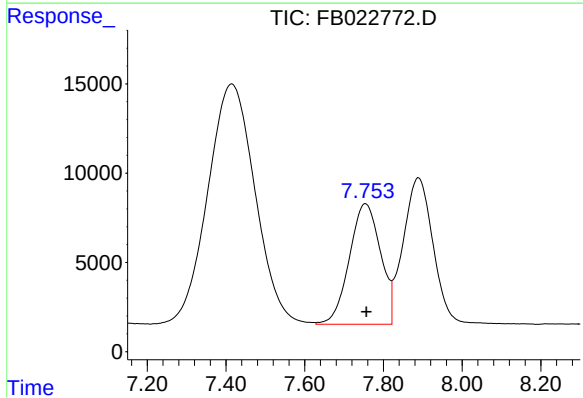


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 371364
Conc: 10.18 ng/ml

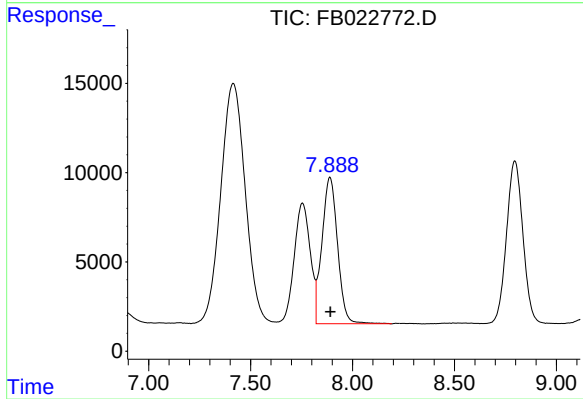


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 435895
Conc: 9.87 ng/ml

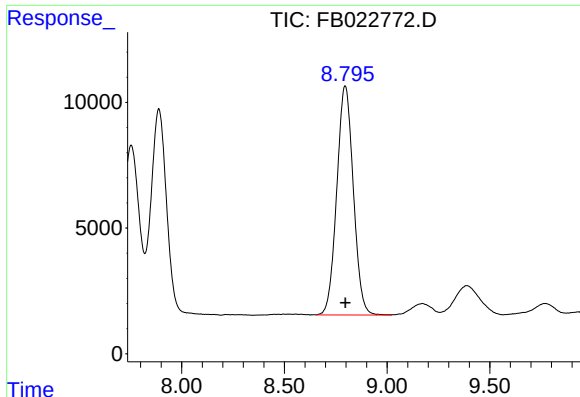


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 511371
Conc: 20.21 ng/ml

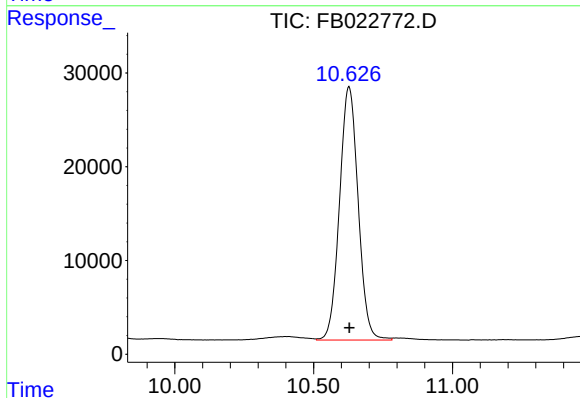


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1261233
Conc: 29.26 ng/ml

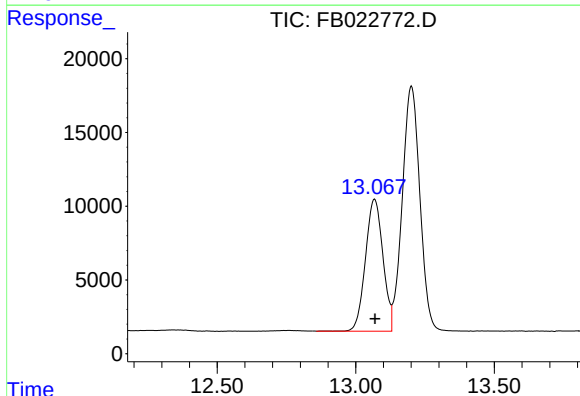


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 392328
Conc: 9.66 ng/ml

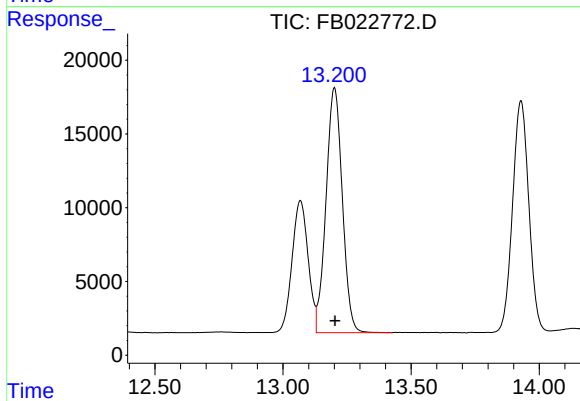


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 734355
Conc: 19.09 ng/ml

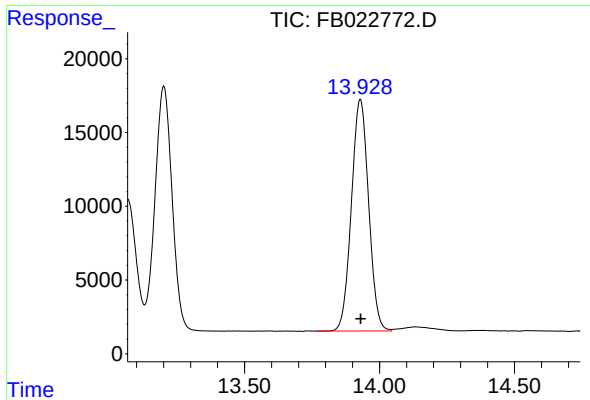

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 696426
Conc: 19.12 ng/ml

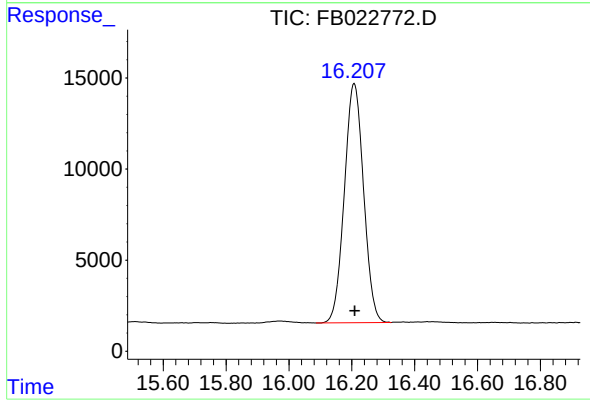

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 558018
Conc: 19.58 ng/ml