

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101819\
 Data File : FB022782.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2019 00:08
 Operator : DD/AJ
 Sample : K5436-05MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 19 00:23:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	505786	19.988 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	967456	28.467 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1067058	29.325 ng/ml
3) t	n-Heptane	7.756	349977	9.592 ng/ml
4) t	Benzene	7.891	411250	9.314 ng/ml
6) t	Toluene	10.629	1207197	28.009 ng/ml
7) t	Ethylbenzene	13.068	375804	9.253 ng/ml
8) t	m-Xylene	13.201	707594	18.391 ng/ml
9) t	O-Xylene	13.929	672469	18.463 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	517833	18.172 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101819\
Data File : FB022782.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2019 00:08
Operator : DD/AJ
Sample : K5436-05MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 19 00:23:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

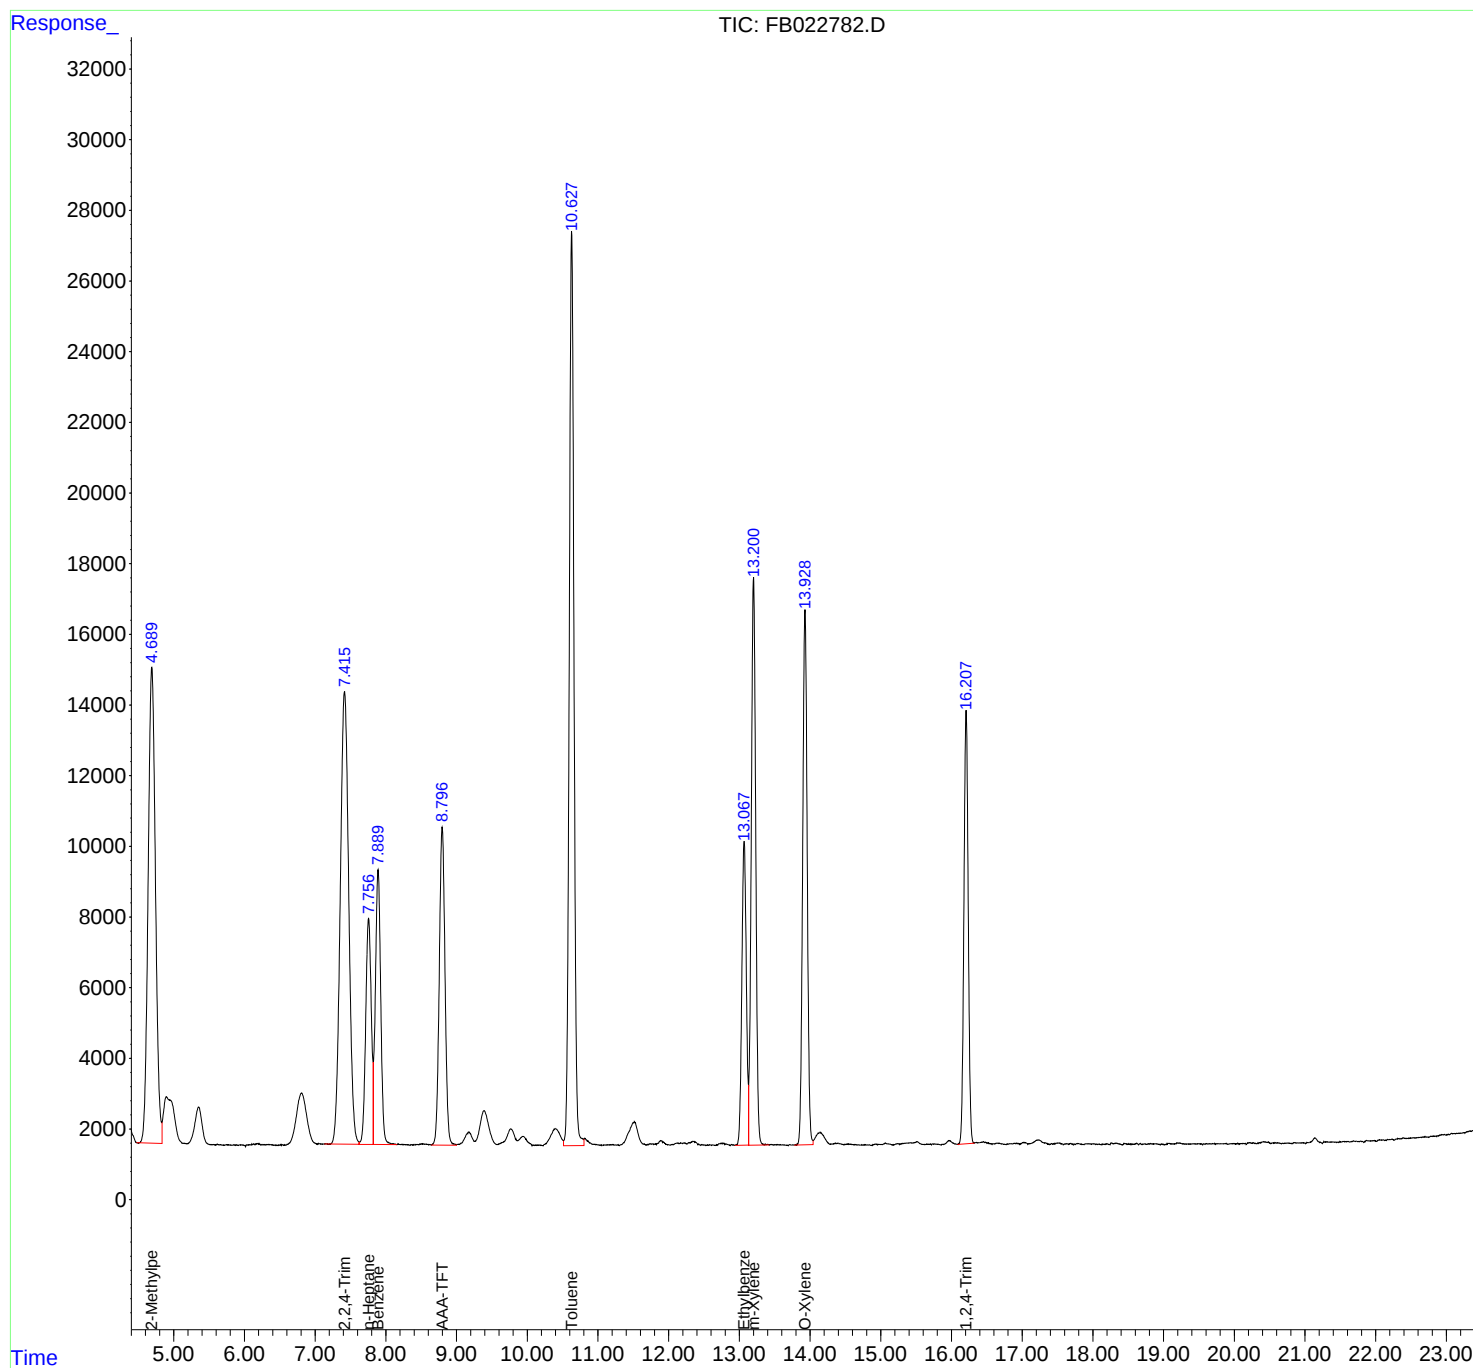

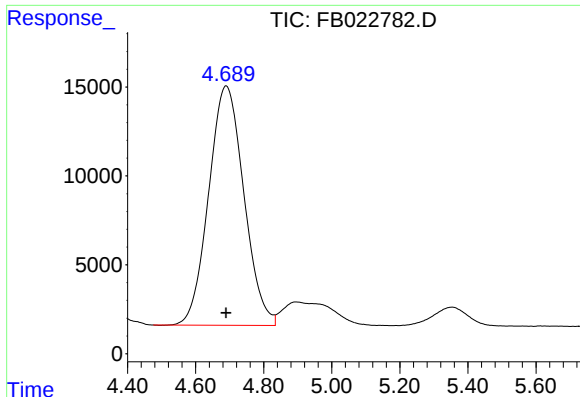


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 967456
Conc: 28.47 ng/ml

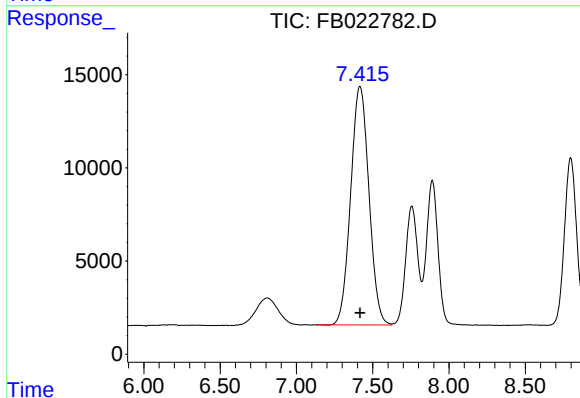


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 1067058
Conc: 29.33 ng/ml

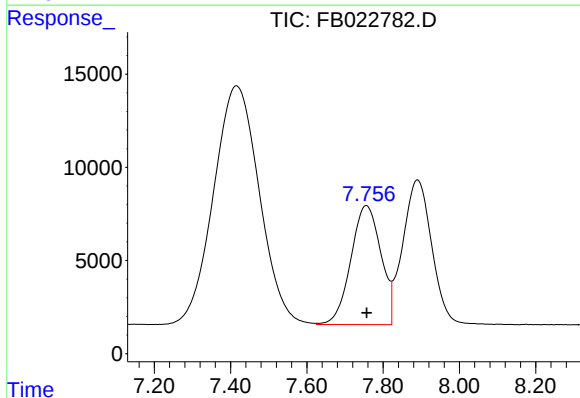


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 349977
Conc: 9.59 ng/ml

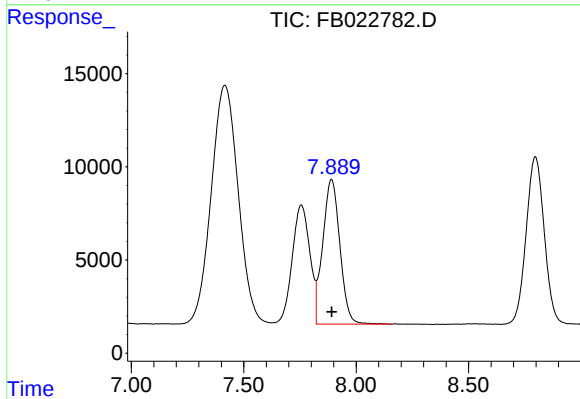


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 411250
Conc: 9.31 ng/ml

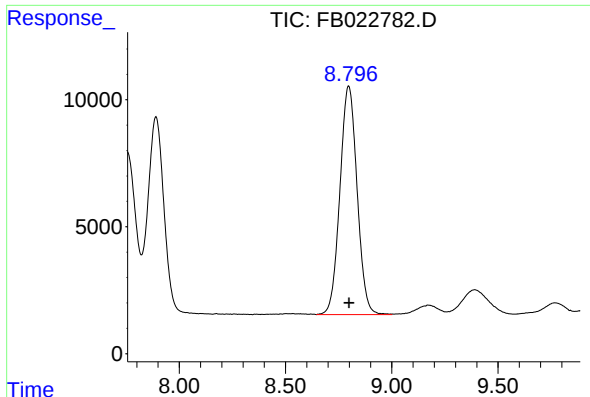


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 505786
Conc: 19.99 ng/ml

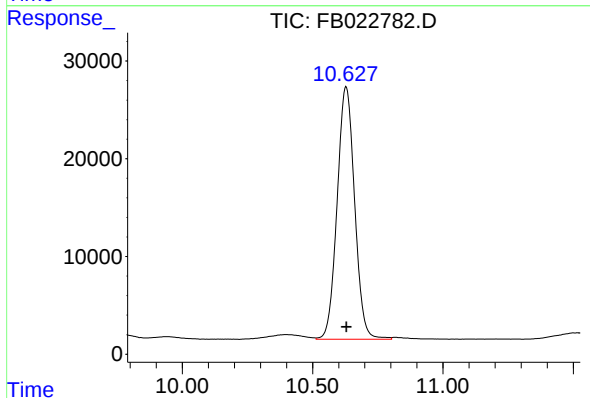


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1207197
Conc: 28.01 ng/ml

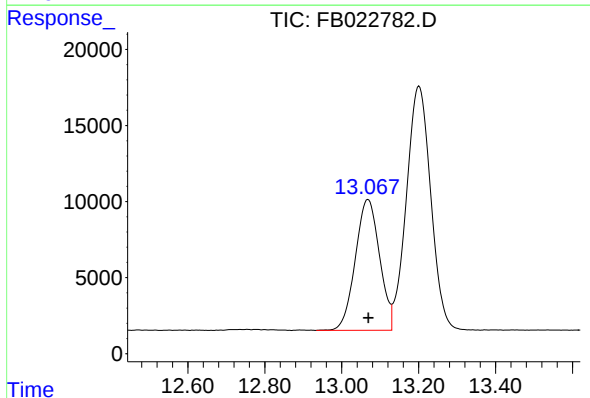


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.001 min
Response: 375804
Conc: 9.25 ng/ml

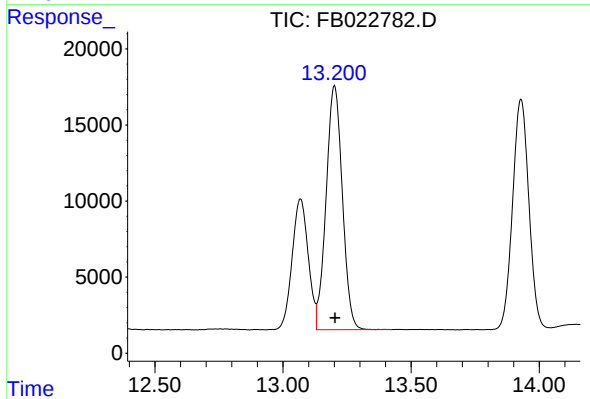


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 707594
Conc: 18.39 ng/ml

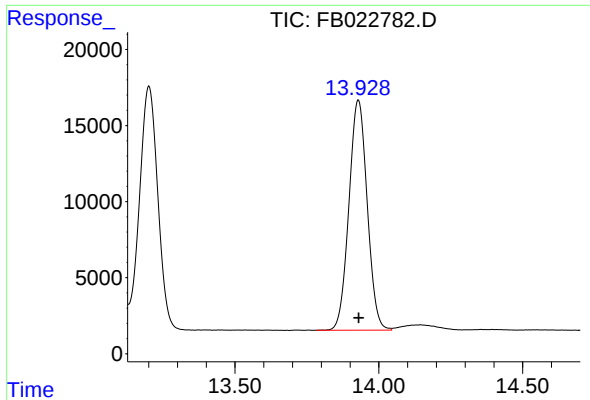

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 672469
Conc: 18.46 ng/ml

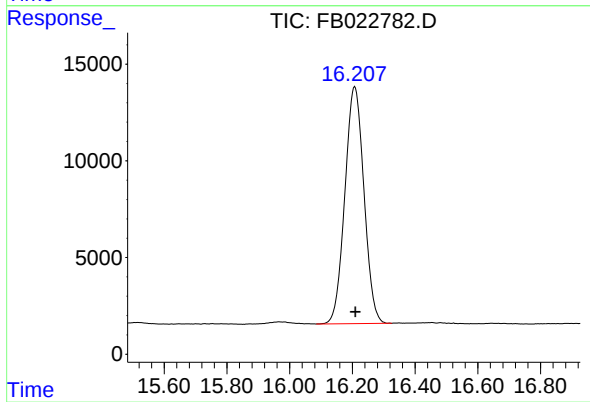

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 517833
Conc: 18.17 ng/ml