

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
 Data File : FB025104.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2020 21:41
 Operator : DD/AJ
 Sample : L4433-01MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 20 01:02:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	453010	21.220 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	900747	29.616 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	805022	25.842 ng/ml
3) t n-Heptane	7.759	168064	5.466 ng/ml
4) t Benzene	7.893	391499	10.417 ng/ml
6) t Toluene	10.630	1092592	30.657 ng/ml
7) t Ethylbenzene	13.069	325445	9.998 ng/ml
8) t m-Xylene	13.202	654799	20.417 ng/ml
9) t O-Xylene	13.930	641259	20.802 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	481703	18.450 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
Data File : FB025104.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2020 21:41
Operator : DD/AJ
Sample : L4433-01MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 20 01:02:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

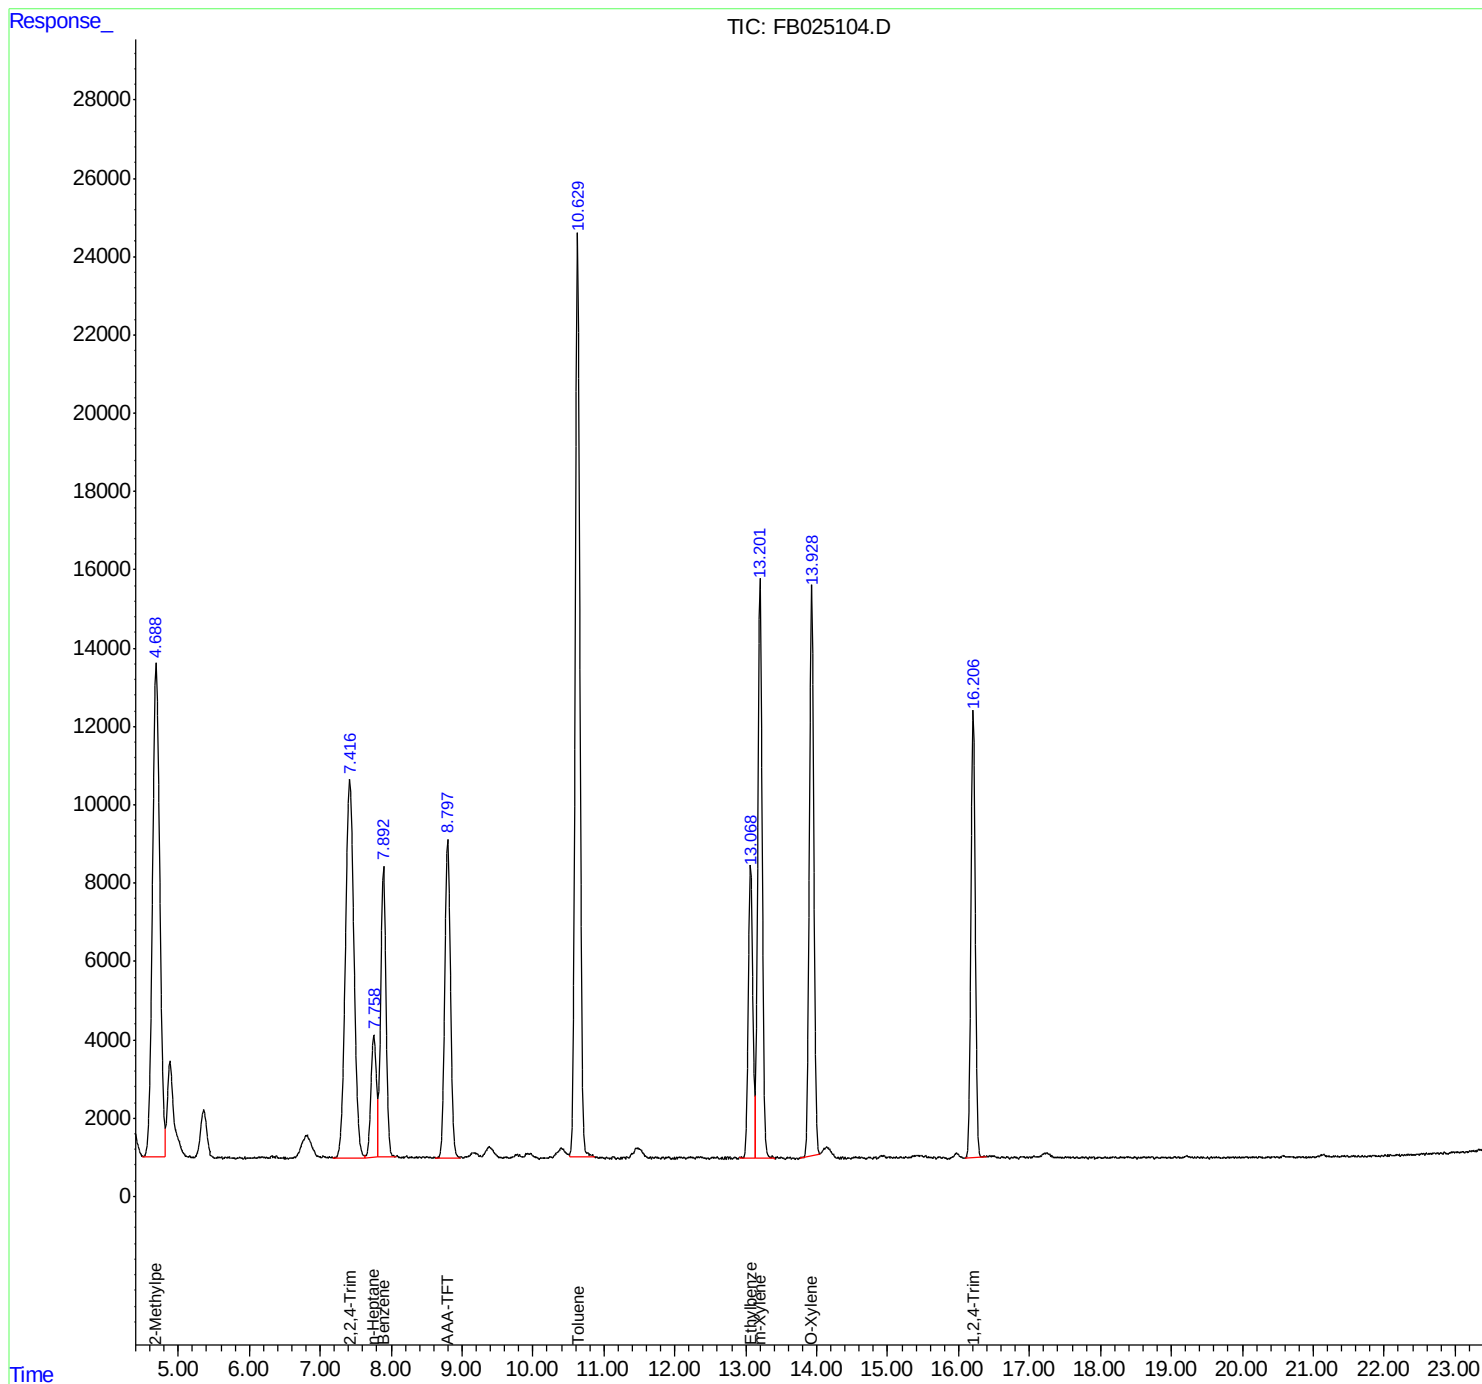

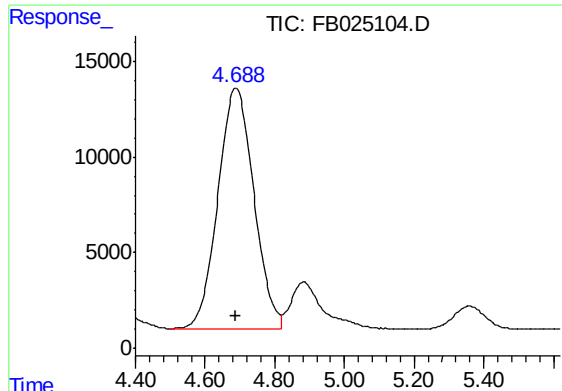


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.001 min
Response: 900747
Conc: 29.62 ng/ml

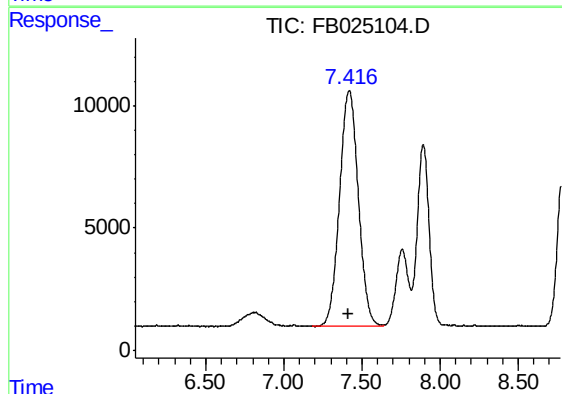


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 805022
Conc: 25.84 ng/ml

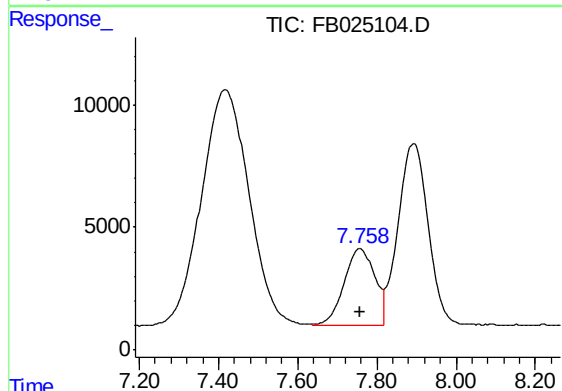


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 168064
Conc: 5.47 ng/ml

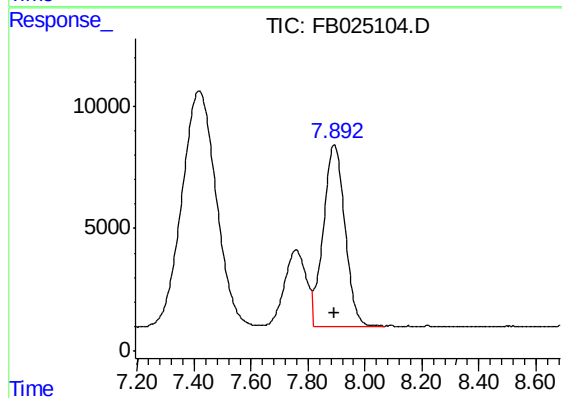


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 391499
Conc: 10.42 ng/ml

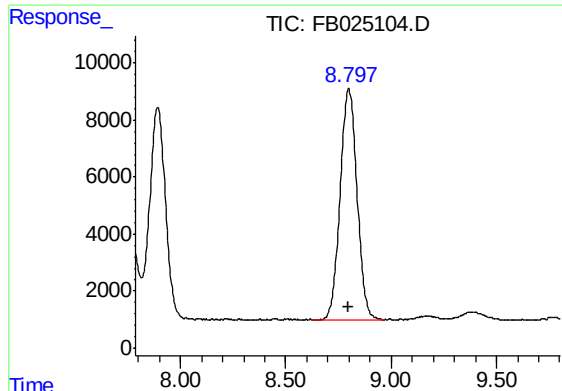


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 453010
Conc: 21.22 ng/ml

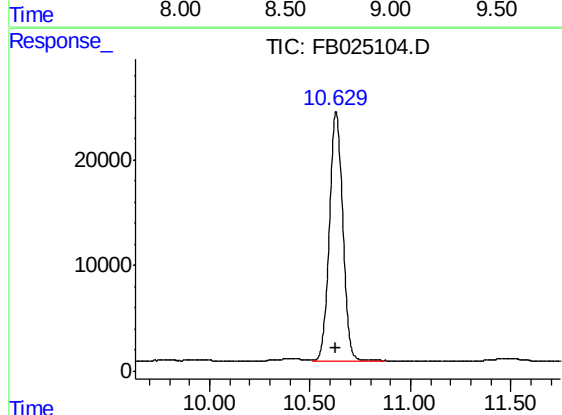


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1092592
Conc: 30.66 ng/ml

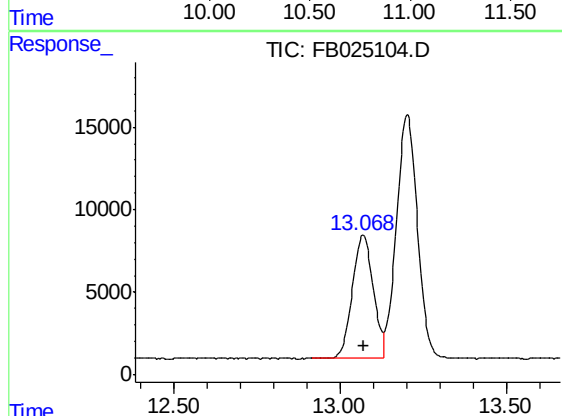


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 325445
Conc: 10.00 ng/ml

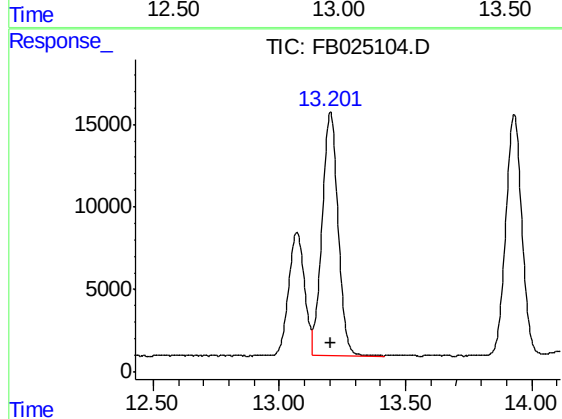


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 654799
Conc: 20.42 ng/ml

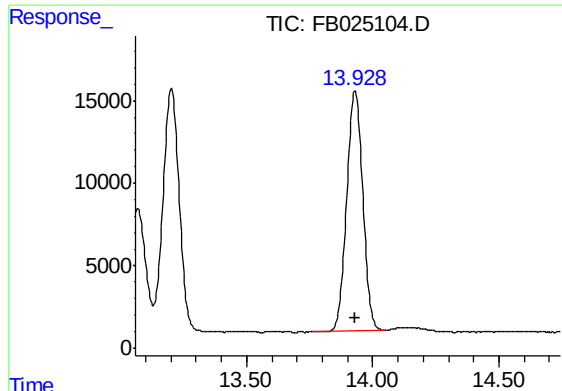

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 641259
Conc: 20.80 ng/ml

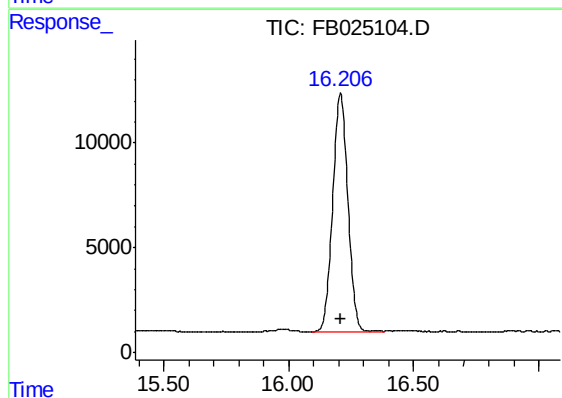

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 481703
Conc: 18.45 ng/ml