

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
 Data File : FB025105.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2020 22:12
 Operator : DD/AJ
 Sample : L4433-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 20 01:02:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	474402	22.222 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	906370	29.800 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	785499	25.215 ng/ml
3) t n-Heptane	7.758	164415	5.348 ng/ml
4) t Benzene	7.892	403027	10.724 ng/ml
6) t Toluene	10.631	1104065	30.979 ng/ml
7) t Ethylbenzene	13.070	323474	9.937 ng/ml
8) t m-Xylene	13.203	652865	20.357 ng/ml
9) t O-Xylene	13.931	643682	20.881 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	476976	18.269 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
Data File : FB025105.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2020 22:12
Operator : DD/AJ
Sample : L4433-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 20 01:02:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

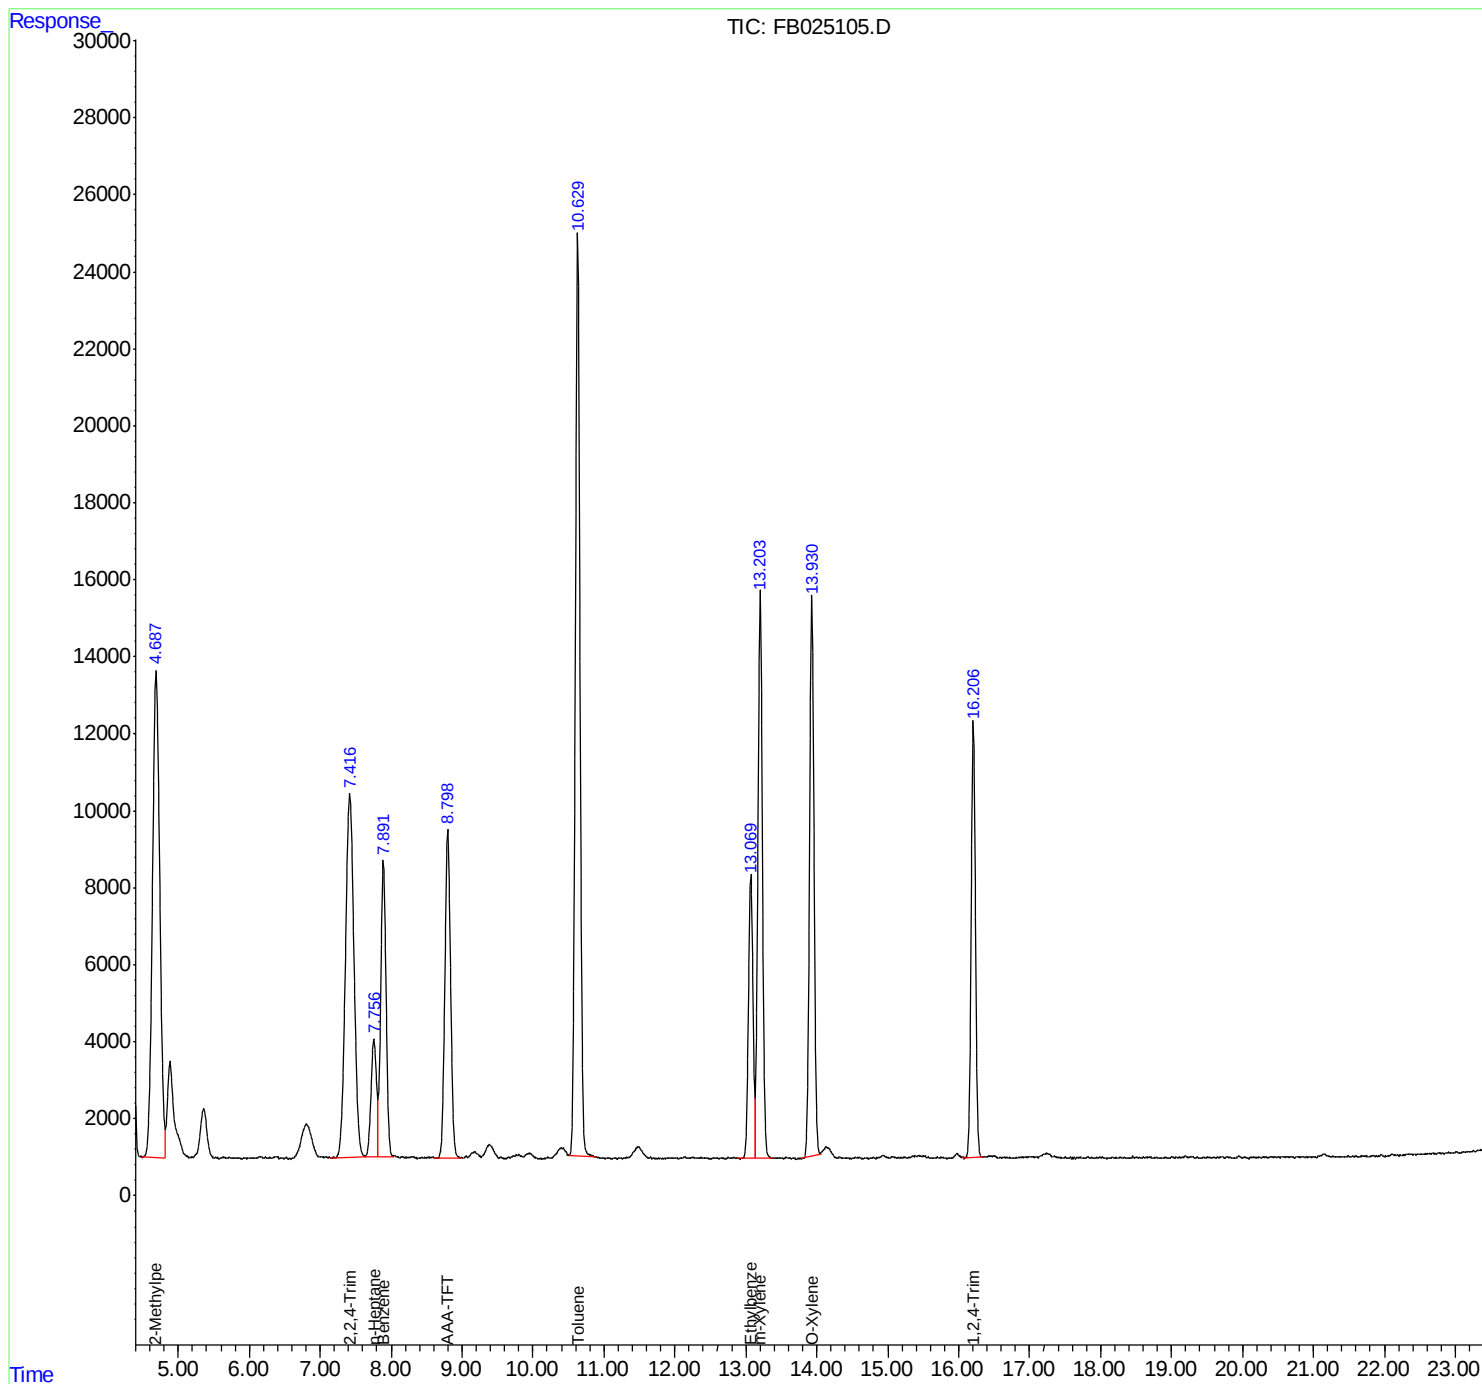

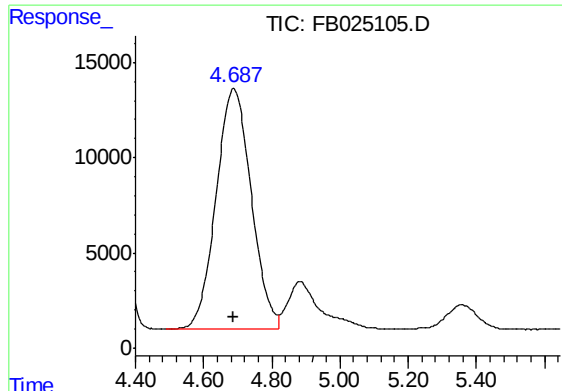


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 906370
Conc: 29.80 ng/ml

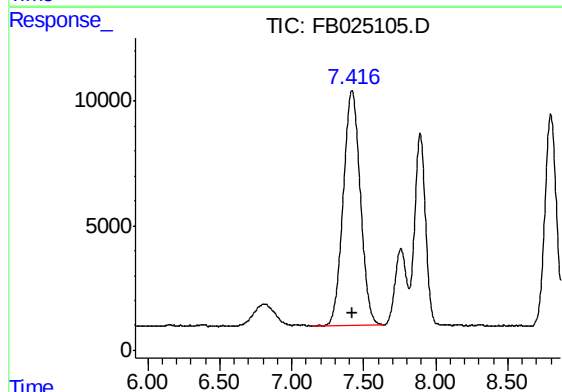


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 785499
Conc: 25.22 ng/ml

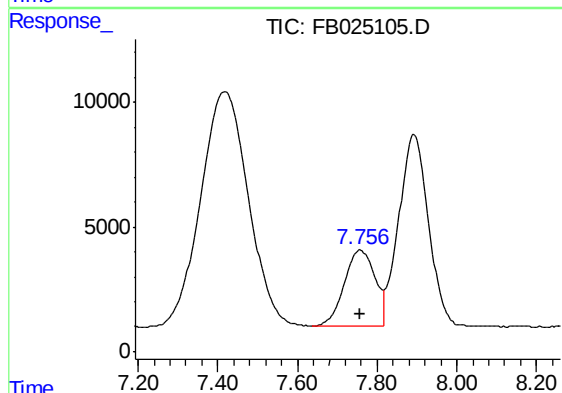


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 164415
Conc: 5.35 ng/ml

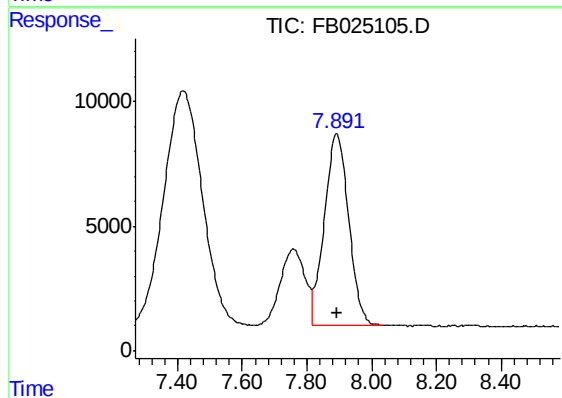


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 403027
Conc: 10.72 ng/ml

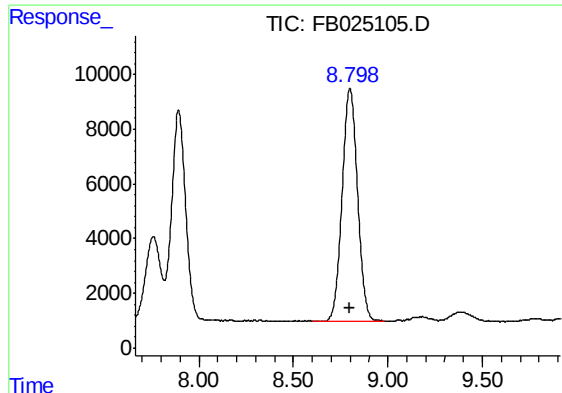


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 474402
Conc: 22.22 ng/ml

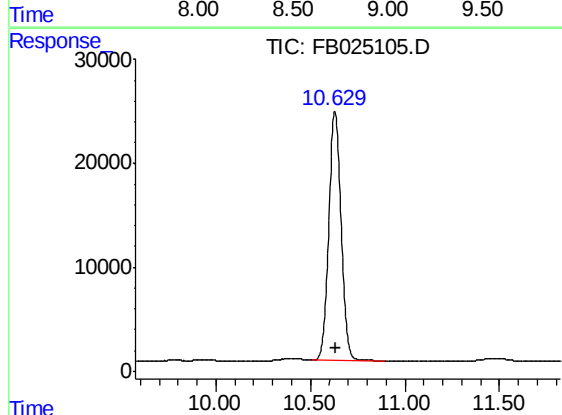


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1104065
Conc: 30.98 ng/ml

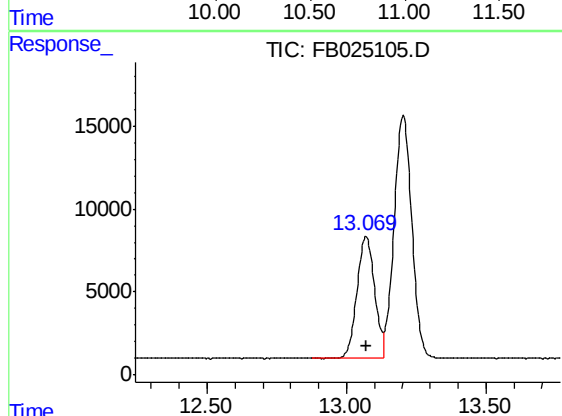


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 323474
Conc: 9.94 ng/ml

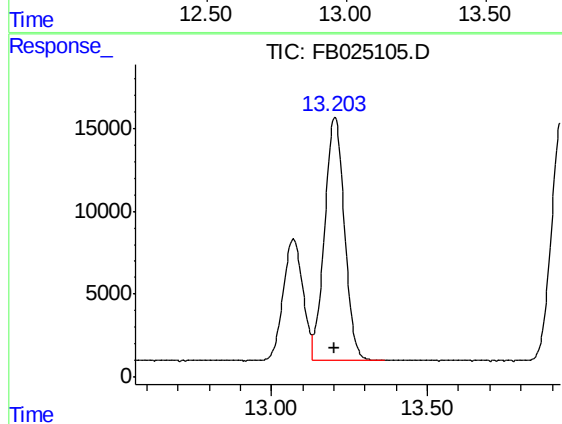


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 652865
Conc: 20.36 ng/ml

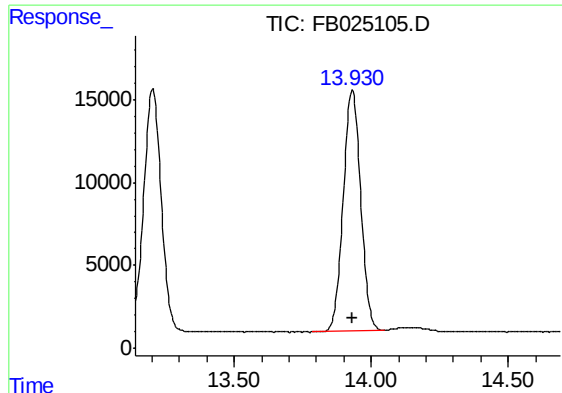

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 643682
Conc: 20.88 ng/ml

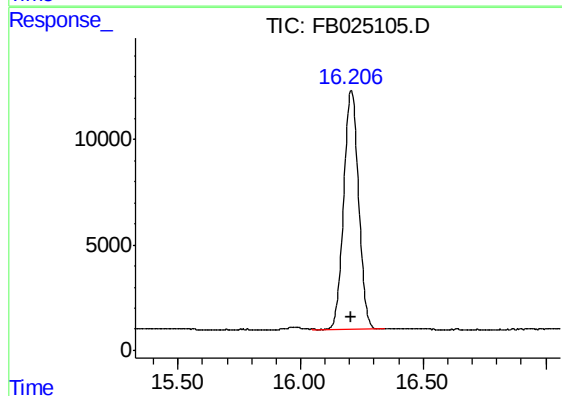

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 476976
Conc: 18.27 ng/ml