

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
 Data File : FB025094.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2020 16:02
 Operator : DD/AJ
 Sample : L4214-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 20 08:07:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	423116	19.820 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	206794	6.799 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	214726	6.893 ng/ml
3) t	n-Heptane	7.760	69731	2.268 ng/ml
4) t	Benzene	7.892	82196	2.187 ng/ml
6) t	Toluene	10.632	233119	6.541 ng/ml
7) t	Ethylbenzene	13.071	75954	2.333 ng/ml
8) t	m-Xylene	13.204	146963	4.582 ng/ml
9) t	O-Xylene	13.931	142746	4.631 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	112585	4.312 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
Data File : FB025094.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2020 16:02
Operator : DD/AJ
Sample : L4214-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 20 08:07:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

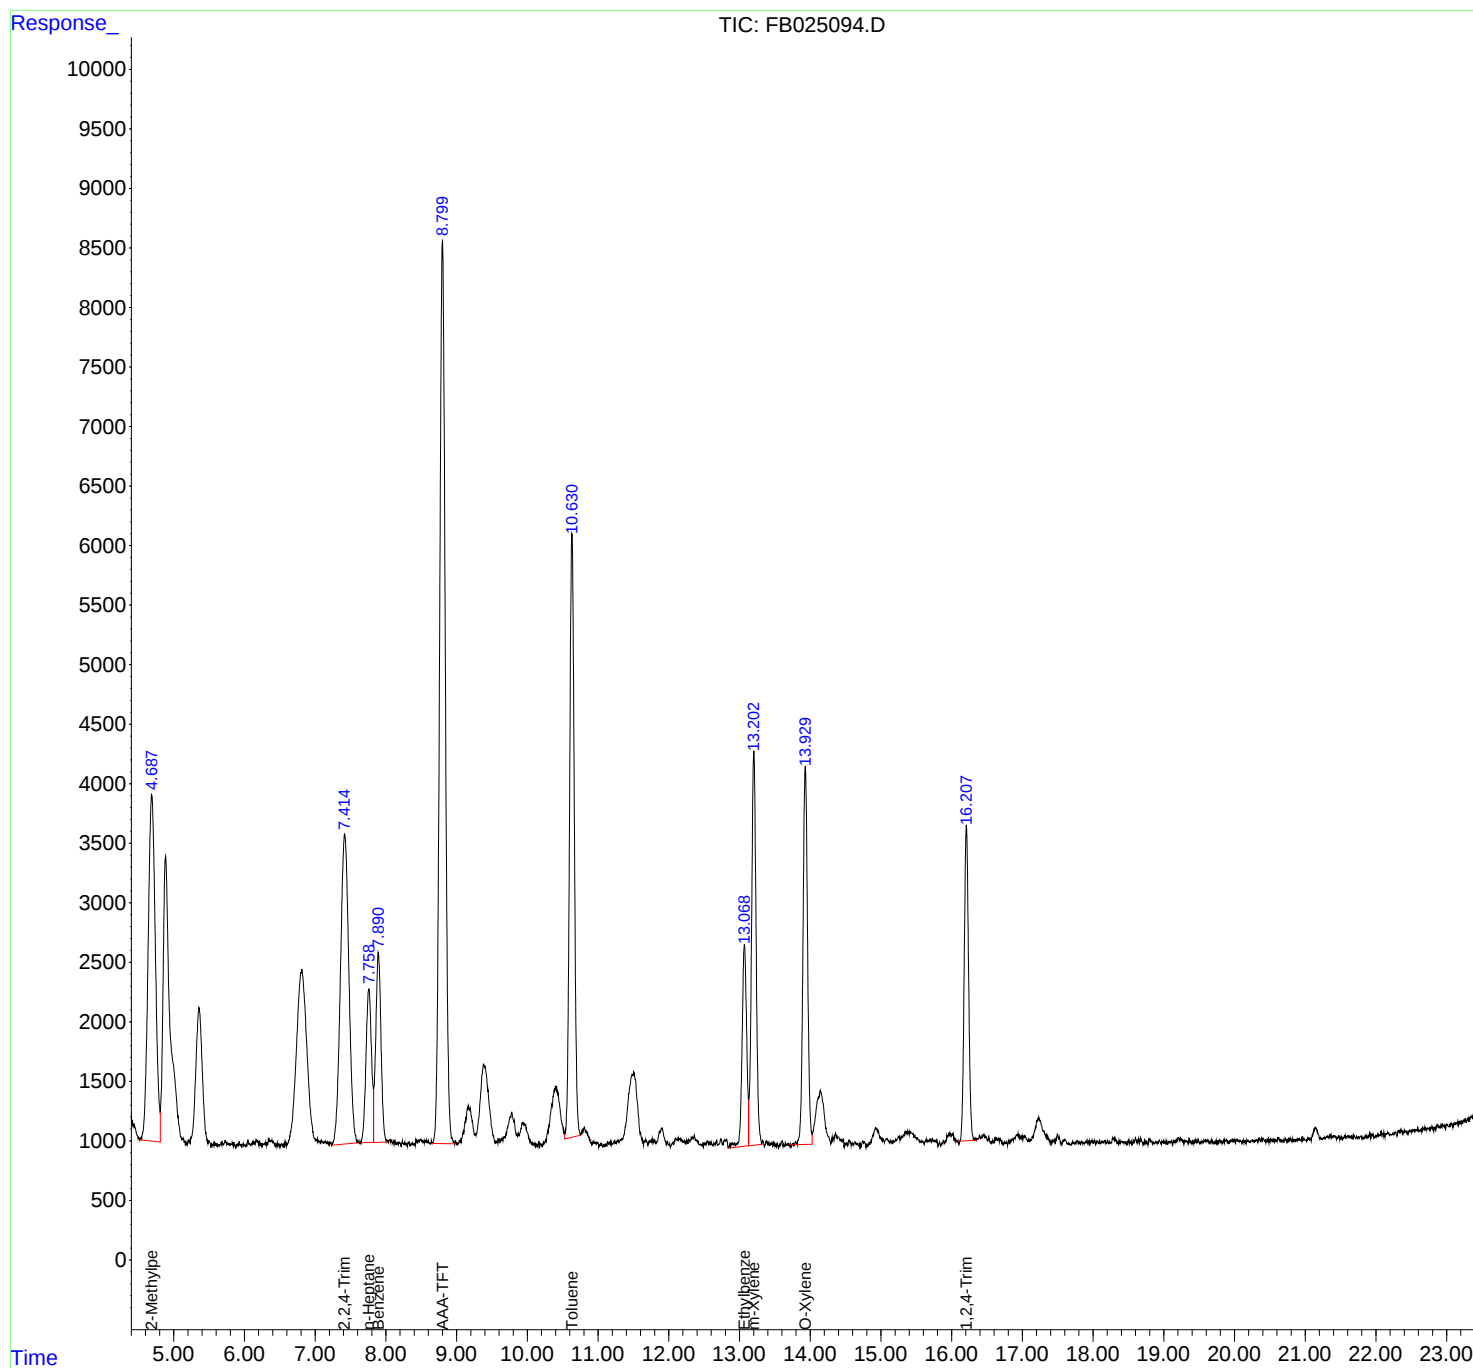

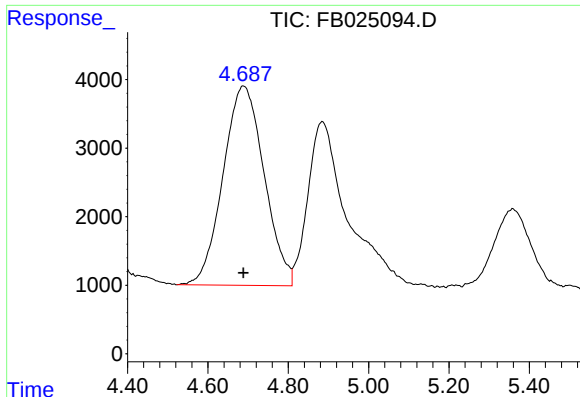


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 206794
Conc: 6.80 ng/ml

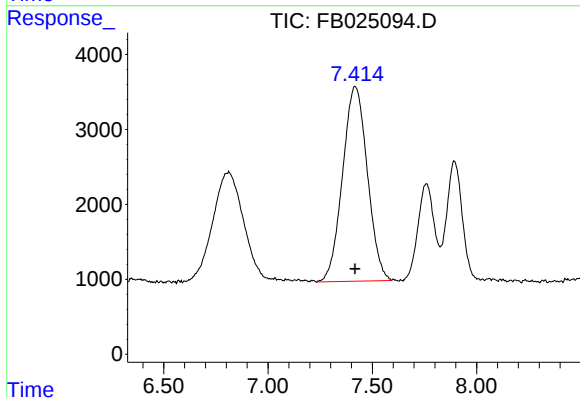


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 214726
Conc: 6.89 ng/ml

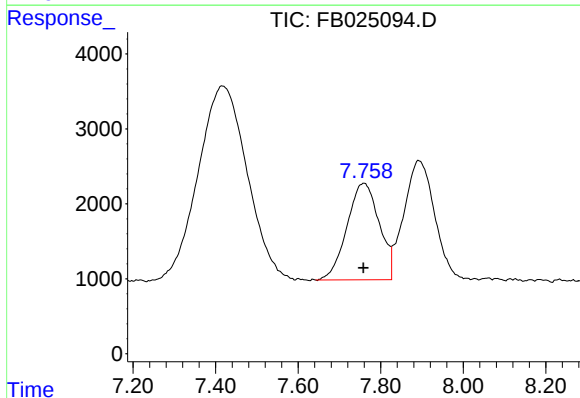


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 69731
Conc: 2.27 ng/ml

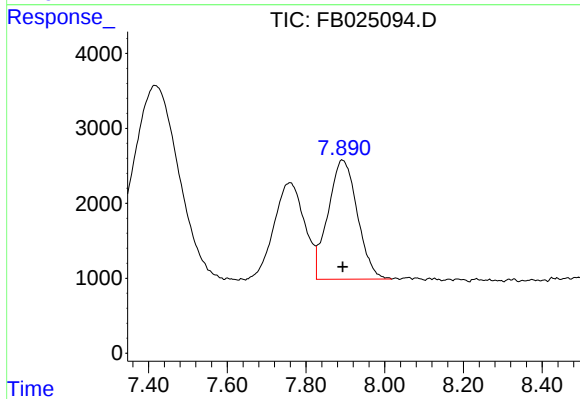


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 82196
Conc: 2.19 ng/ml

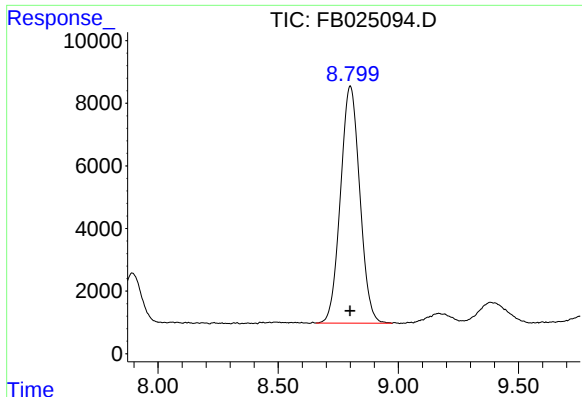


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 423116
Conc: 19.82 ng/ml

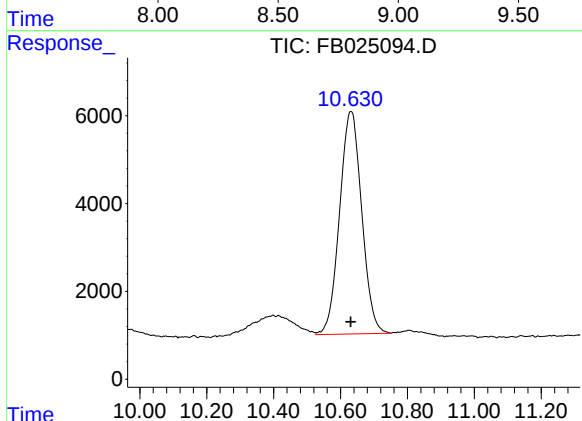


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 233119
Conc: 6.54 ng/ml

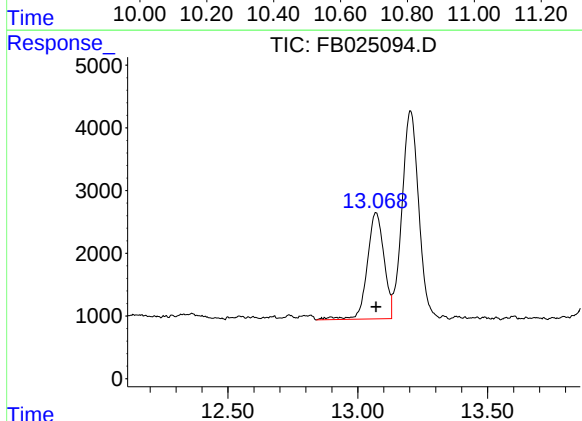


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 75954
Conc: 2.33 ng/ml

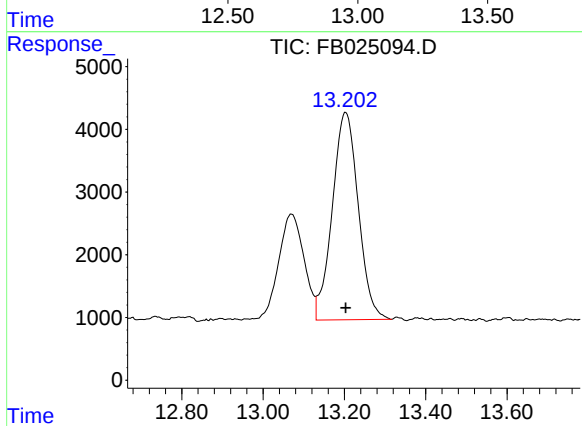


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 146963
Conc: 4.58 ng/ml

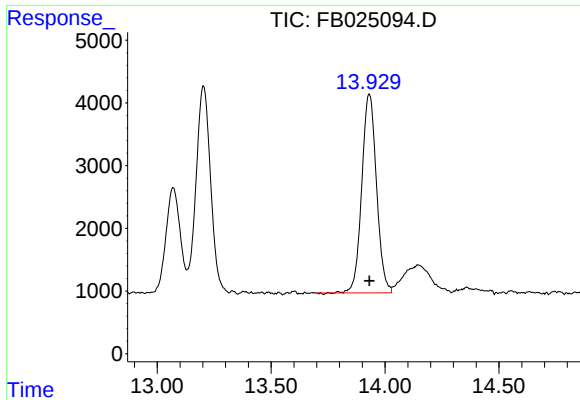

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 142746
Conc: 4.63 ng/ml

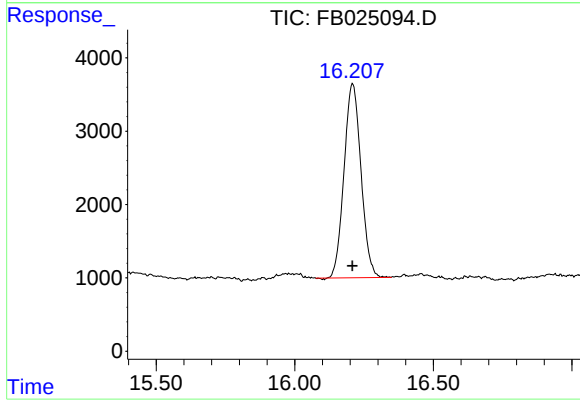

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 112585
Conc: 4.31 ng/ml