

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
 Data File : FB025095.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2020 16:33
 Operator : DD/AJ
 Sample : L4214-02
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 20 08:07:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	426858	19.995 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	254750	8.376 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	257916	8.279 ng/ml
3) t	n-Heptane	7.757	85911	2.794 ng/ml
4) t	Benzene	7.893	99821	2.656 ng/ml
6) t	Toluene	10.631	284019	7.969 ng/ml
7) t	Ethylbenzene	13.071	90982	2.795 ng/ml
8) t	m-Xylene	13.203	180638	5.632 ng/ml
9) t	O-Xylene	13.931	176373	5.721 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	141284	5.411 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101920\
Data File : FB025095.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2020 16:33
Operator : DD/AJ
Sample : L4214-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 20 08:07:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

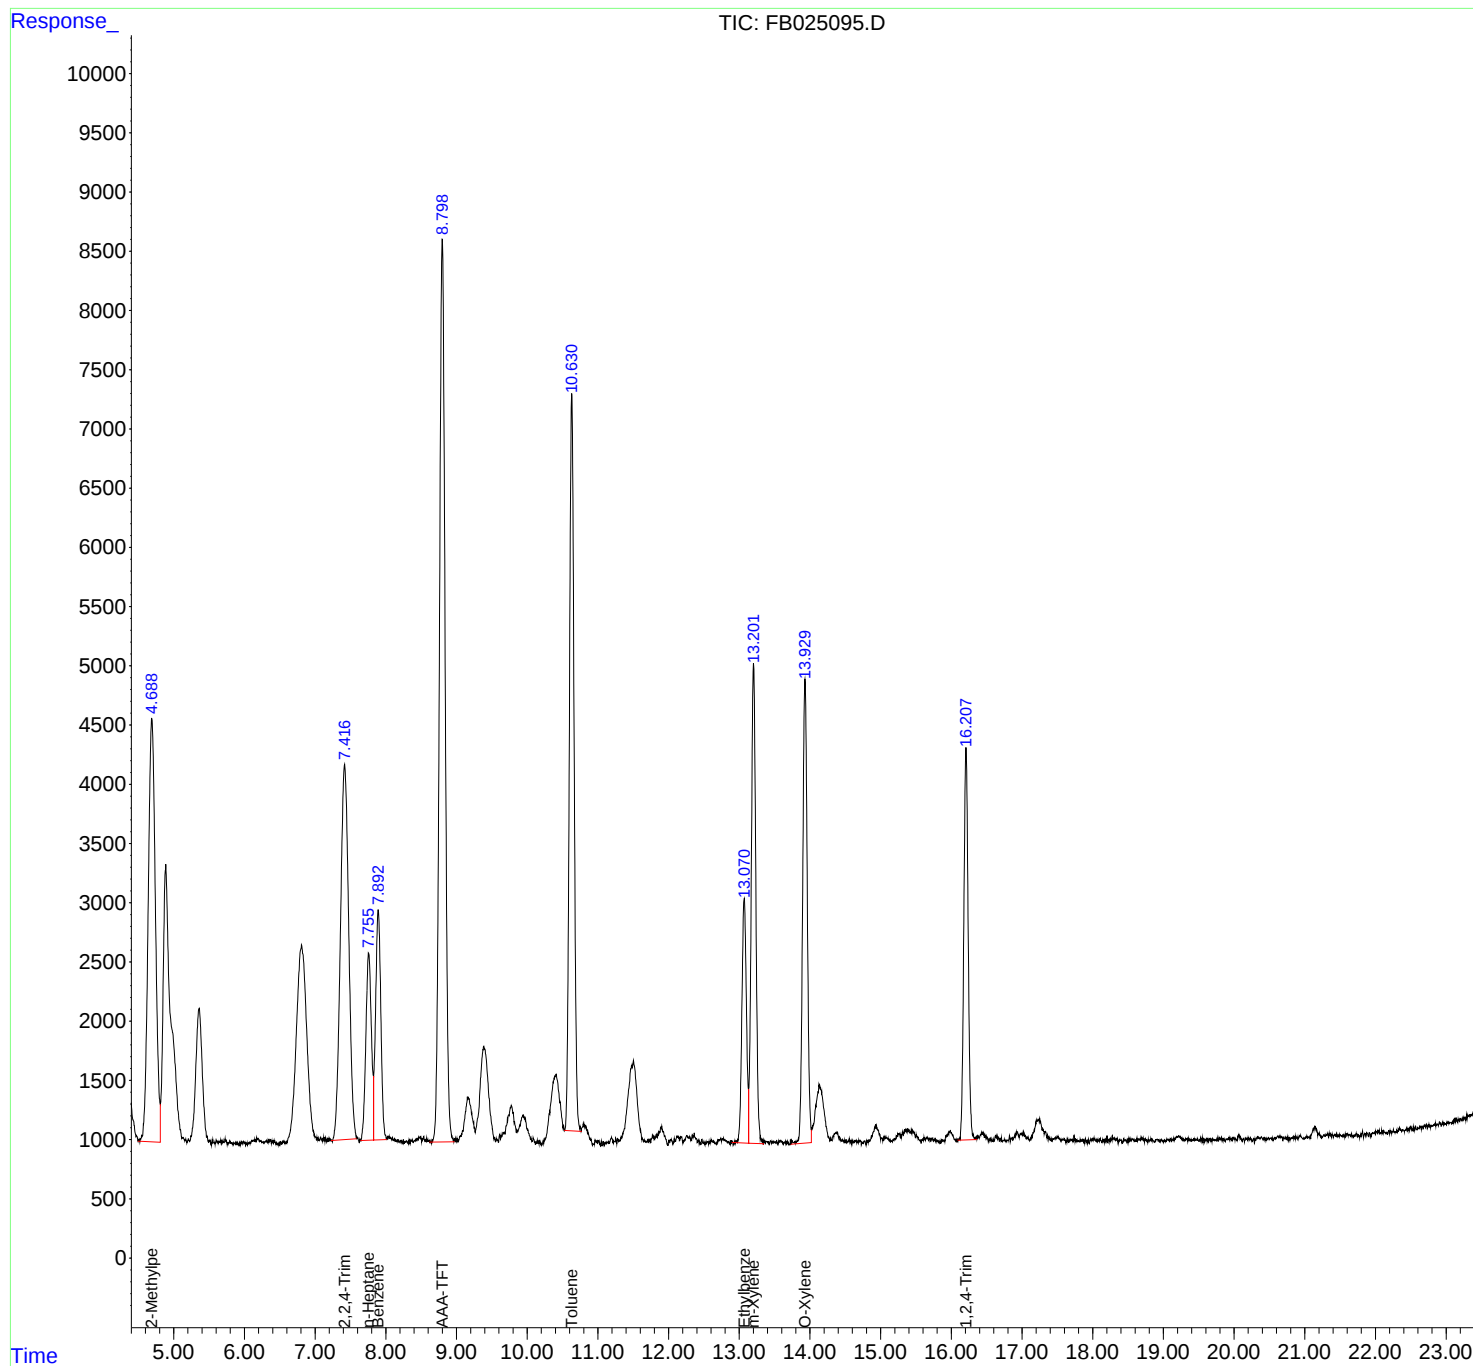

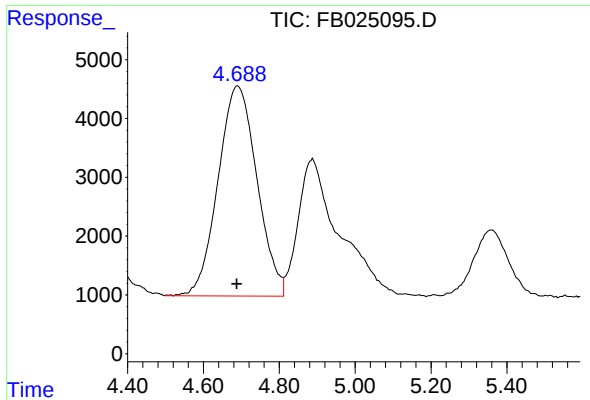


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 254750
Conc: 8.38 ng/ml

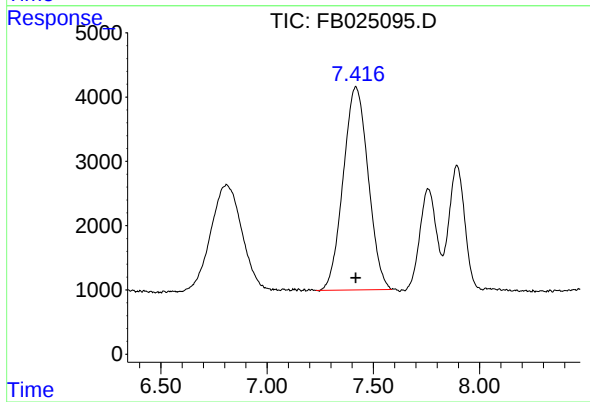


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 257916
Conc: 8.28 ng/ml

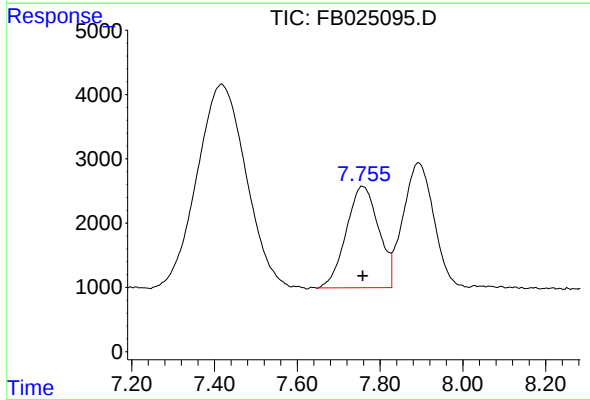


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 85911
Conc: 2.79 ng/ml

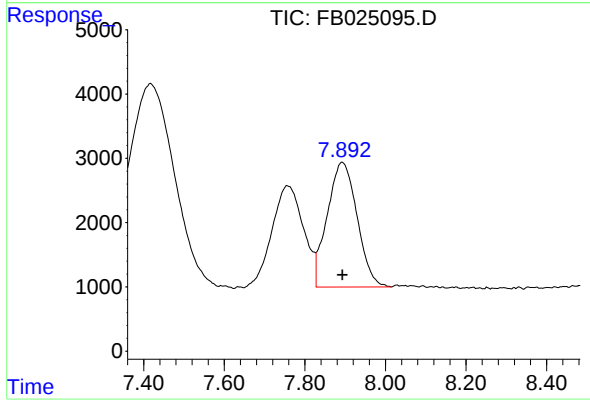


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 99821
Conc: 2.66 ng/ml

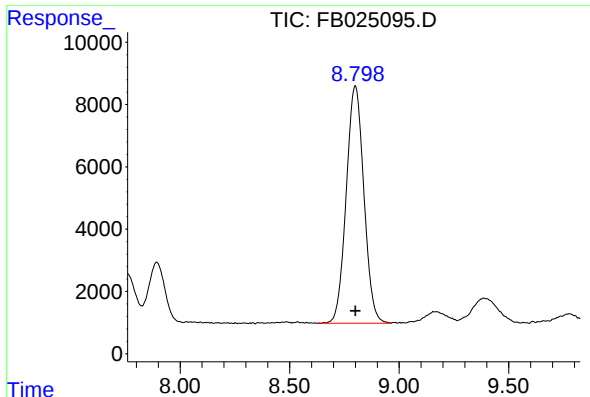


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 426858
Conc: 20.00 ng/ml

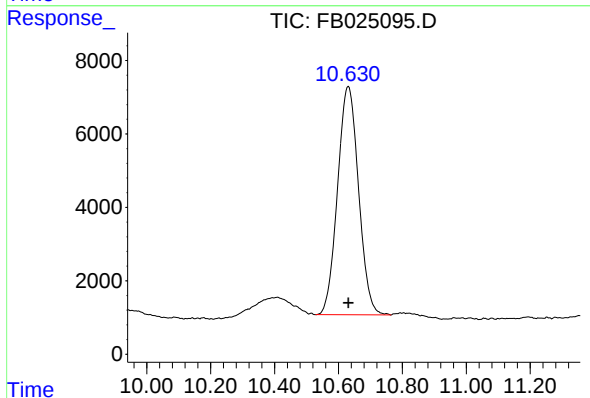


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 284019
Conc: 7.97 ng/ml

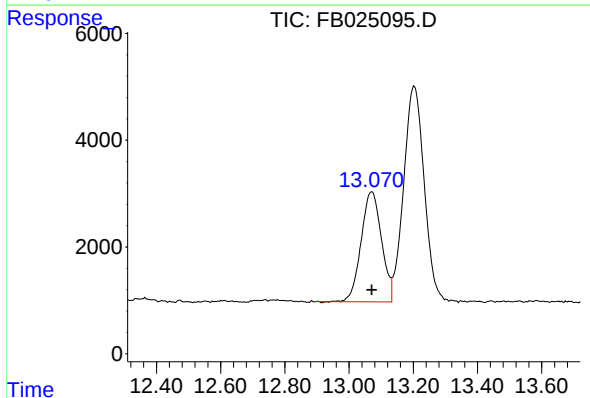


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 90982
Conc: 2.80 ng/ml

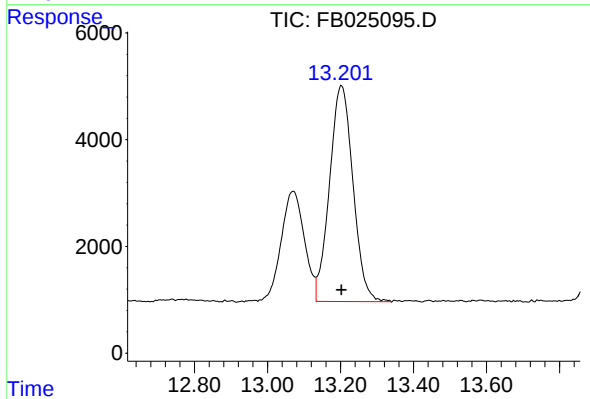


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 180638
Conc: 5.63 ng/ml

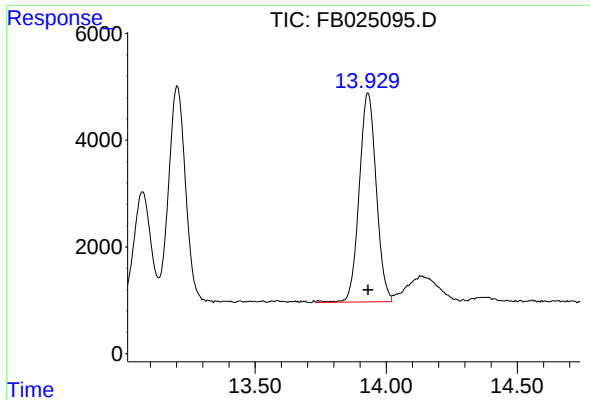

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 176373
Conc: 5.72 ng/ml

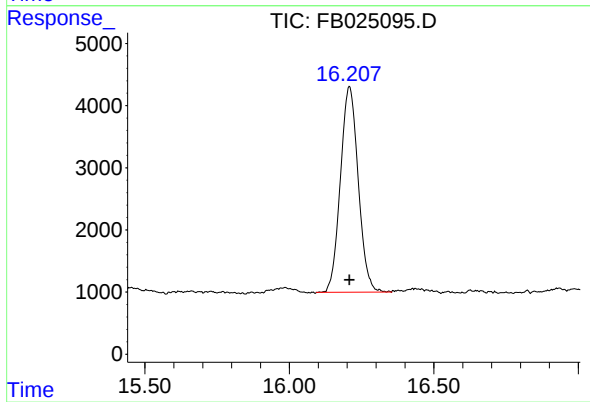

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 141284
Conc: 5.41 ng/ml