

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101921\
 Data File : FB026298.D
 Signal(s) : FID2B.CH
 Acq On : 19 Oct 2021 13:05
 Operator : AJ/MA
 Sample : BSF1019S1
 Misc : 4.99G/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 19 14:41:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.843	219987	14.598 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.843	450514	25.880 ng/ml
2) t 2,2,4-Trimethylpentane	7.521	556306	26.932 ng/ml
3) t n-Heptane	7.816	169684	7.243 ng/ml
4) t Benzene	7.955	197761	7.558 ng/ml
6) t Toluene	10.657	571367	22.054 ng/ml
7) t Ethylbenzene	13.080	179329	7.852 ng/ml
8) t m-Xylene	13.212	365296	16.285 ng/ml
9) t O-Xylene	13.938	367204	17.358 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	414712	17.822 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101921\
Data File : FB026298.D
Signal(s) : FID2B.CH
Acq On : 19 Oct 2021 13:05
Operator : AJ/MA
Sample : BSF1019S1
Misc : 4.99G/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 19 14:41:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

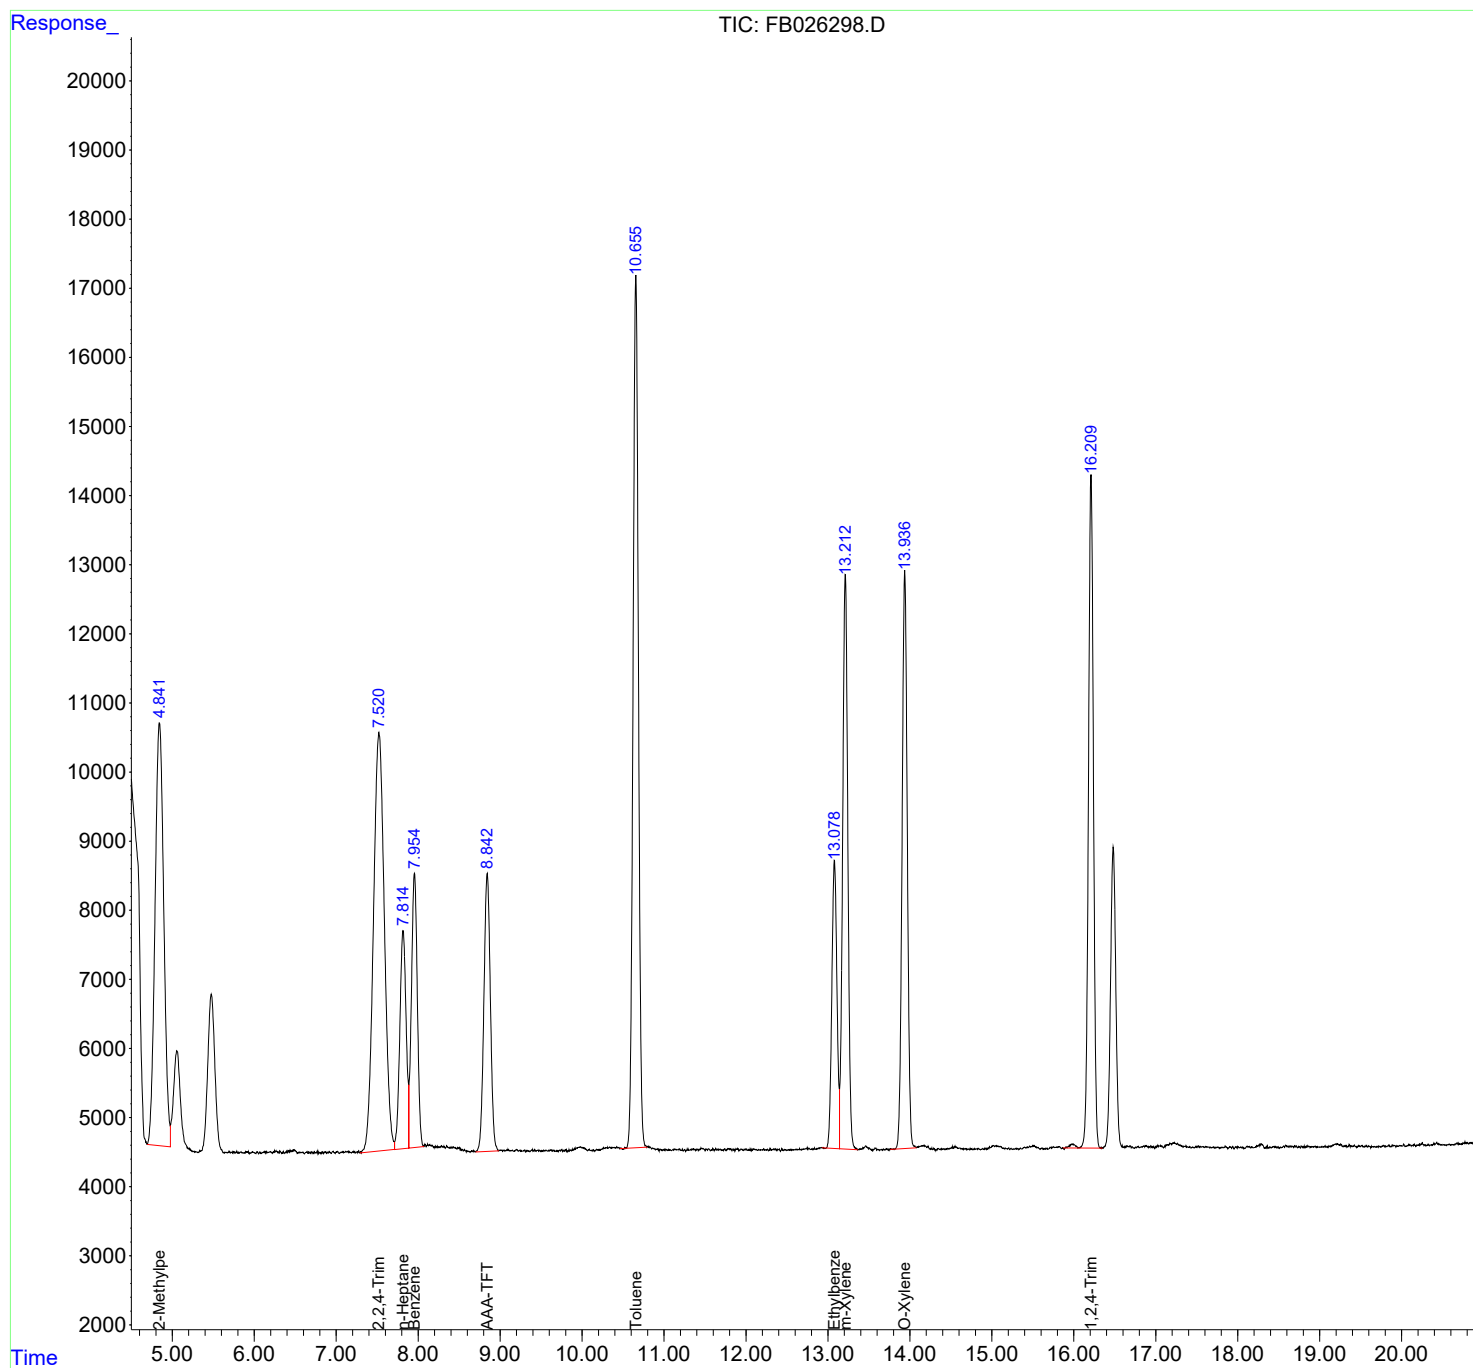


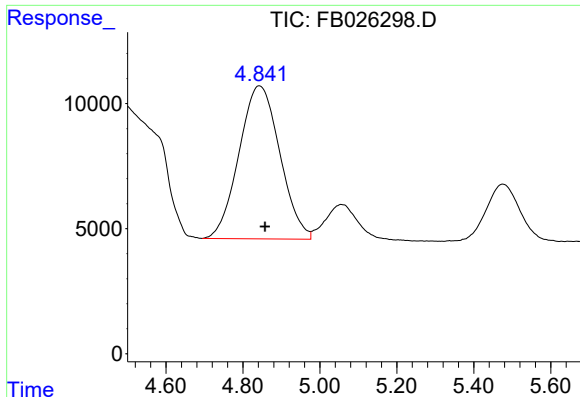

#1 2-Methylpentane


R.T.: 4.843 min
Delta R.T.: -0.014 min
Response: 450514
Conc: 25.88 ng/ml

Instrument :
FID_B
ClientSampleId :

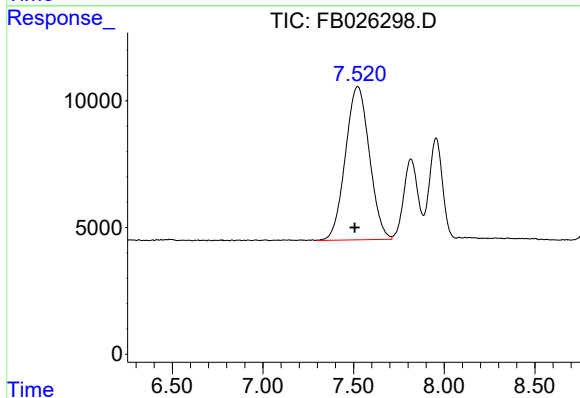


#2 2,2,4-Trimethylpentane

R.T.: 7.521 min
Delta R.T.: 0.015 min
Response: 556306
Conc: 26.93 ng/ml

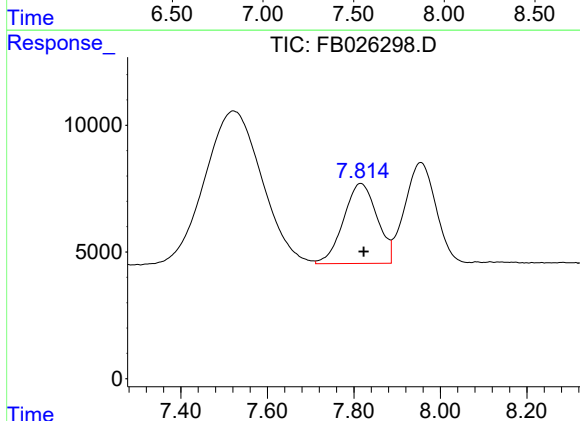


#3 n-Heptane

R.T.: 7.816 min
Delta R.T.: -0.007 min
Response: 169684
Conc: 7.24 ng/ml

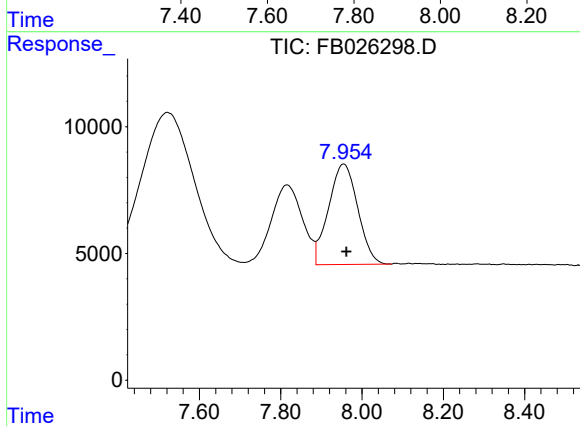

#4 Benzene


R.T.: 7.955 min
Delta R.T.: -0.006 min
Response: 197761
Conc: 7.56 ng/ml

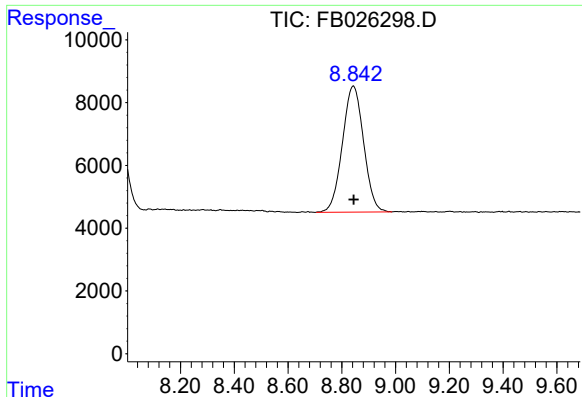

#5 AAA-TFT


R.T.: 8.843 min
Delta R.T.: -0.001 min
Response: 219987
Conc: 14.60 ng/ml

Instrument :
FID_B
ClientSampleId :

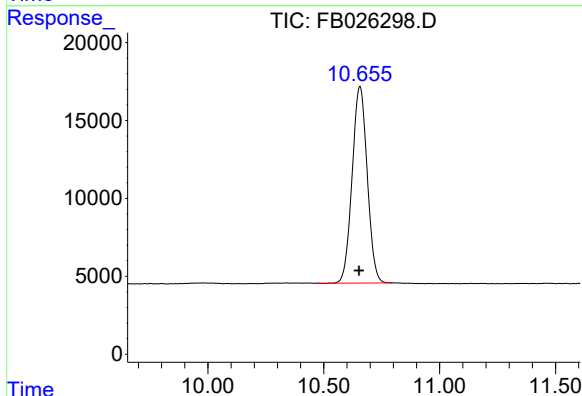


#6 Toluene

R.T.: 10.657 min
Delta R.T.: 0.004 min
Response: 571367
Conc: 22.05 ng/ml

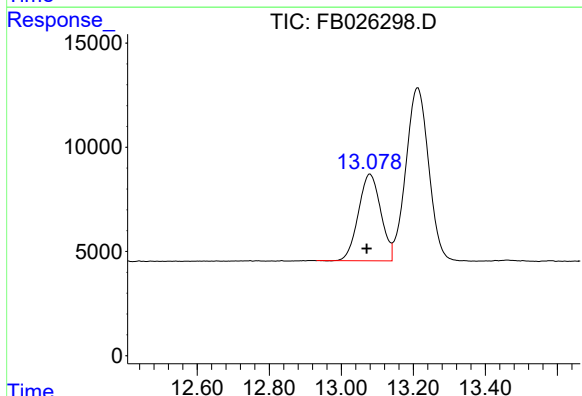


#7 Ethylbenzene

R.T.: 13.080 min
Delta R.T.: 0.009 min
Response: 179329
Conc: 7.85 ng/ml

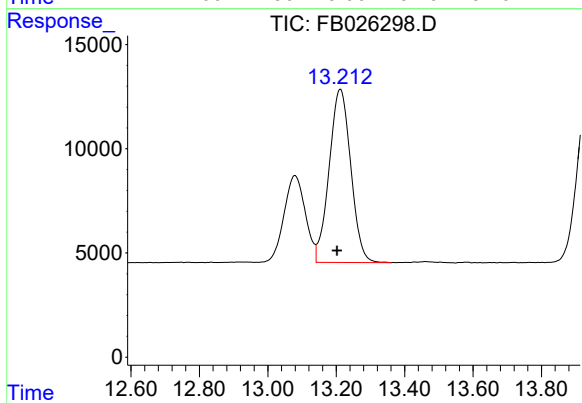

#8 m-Xylene

R.T.: 13.212 min
Delta R.T.: 0.010 min
Response: 365296
Conc: 16.28 ng/ml

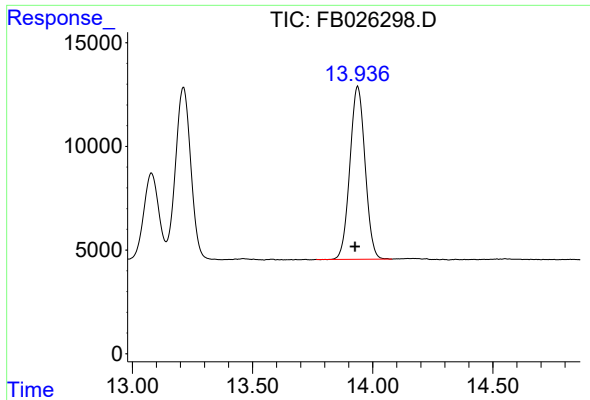

#9 O-Xylene


R.T.: 13.938 min

Delta R.T.: 0.011 min

Response: 367204

Conc: 17.36 ng/ml

Instrument :
FID_B
ClientSampleId :

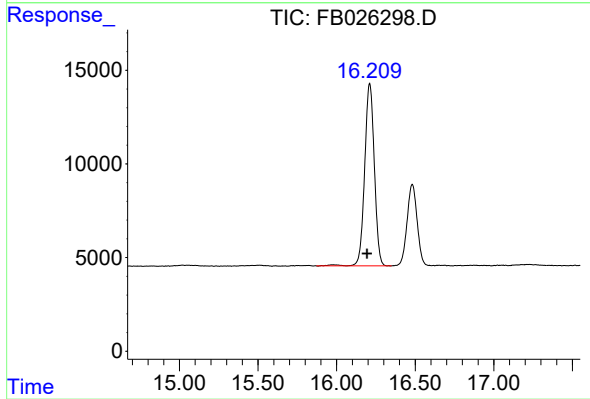

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min

Delta R.T.: 0.016 min

Response: 414712

Conc: 17.82 ng/ml