

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
 Data File : FB025109.D
 Signal(s) : FID2B.CH
 Acq On : 20 Oct 2020 10:30
 Operator : DD/AJ
 Sample : BSF1019S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 21 00:30:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	434479	20.352 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	998872	32.842 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	1049698	33.696 ng/ml
3) t	n-Heptane	7.758	347346	11.297 ng/ml
4) t	Benzene	7.893	409456	10.895 ng/ml
6) t	Toluene	10.631	1163896	32.658 ng/ml
7) t	Ethylbenzene	13.070	356136	10.941 ng/ml
8) t	m-Xylene	13.203	703785	21.945 ng/ml
9) t	O-Xylene	13.930	673723	21.855 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	573926	21.982 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
Data File : FB025109.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2020 10:30
Operator : DD/AJ
Sample : BSF1019S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 21 00:30:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

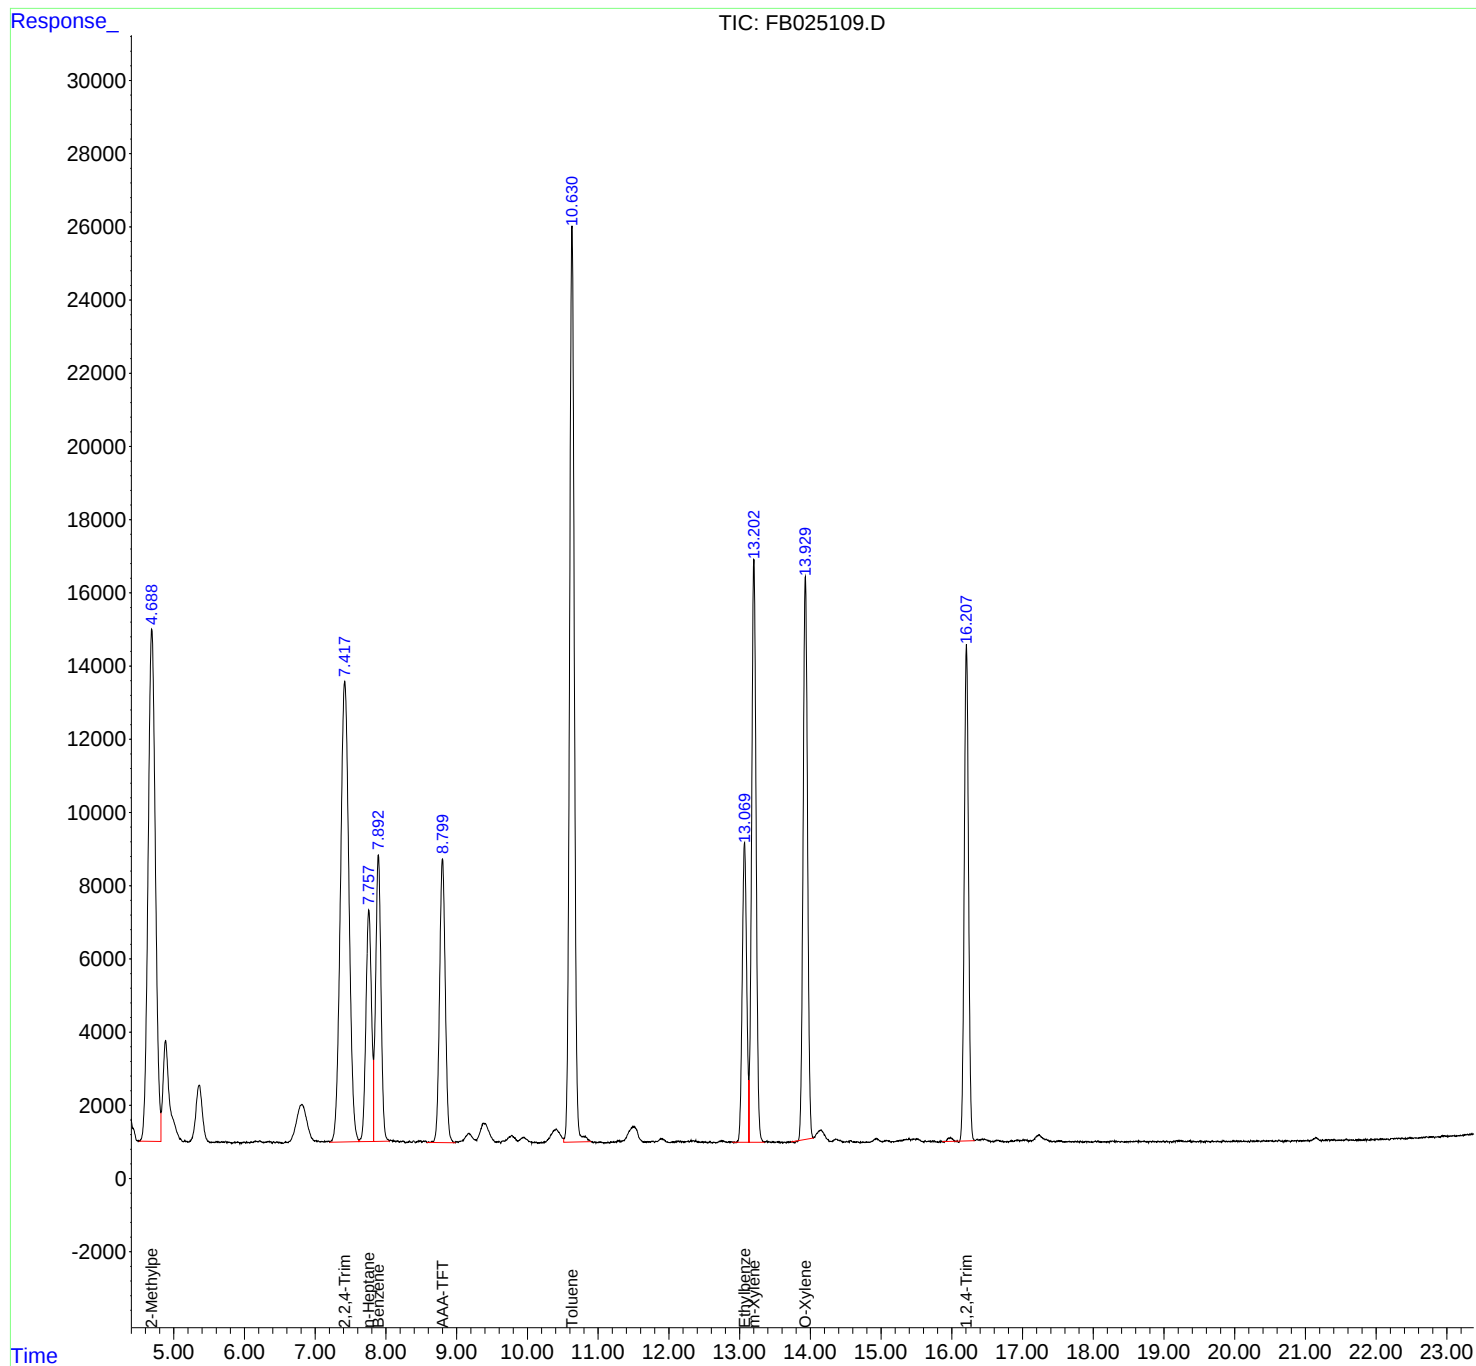

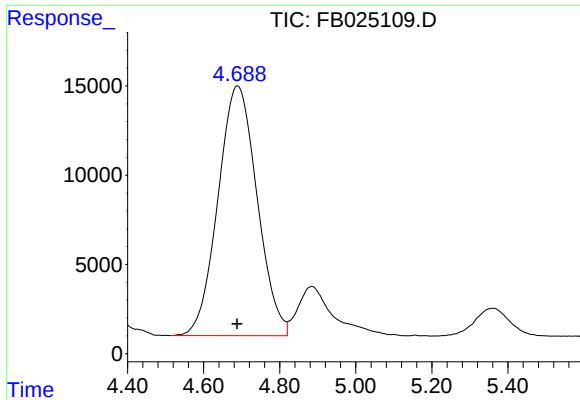


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.001 min
Response: 998872
Conc: 32.84 ng/ml

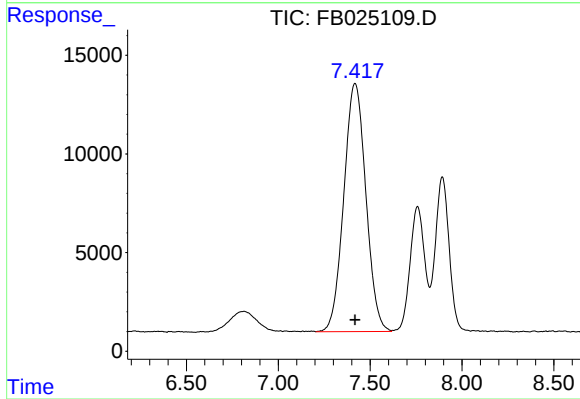


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1049698
Conc: 33.70 ng/ml

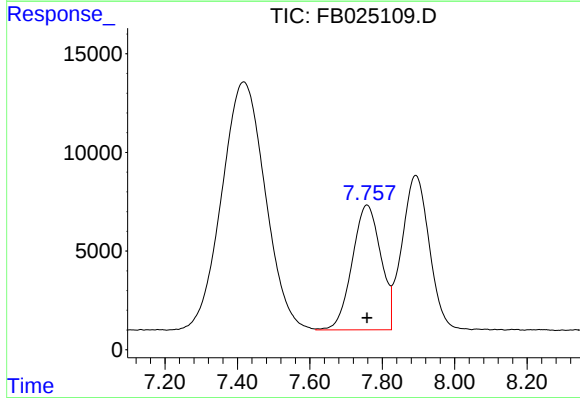


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 347346
Conc: 11.30 ng/ml

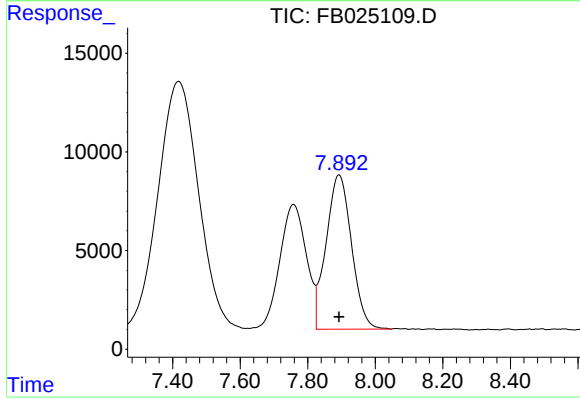


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 409456
Conc: 10.89 ng/ml

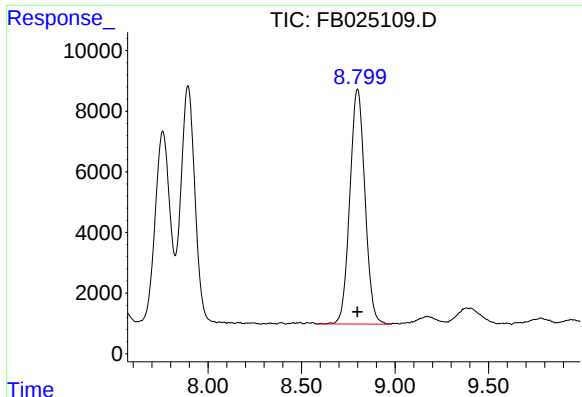


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 434479
Conc: 20.35 ng/ml

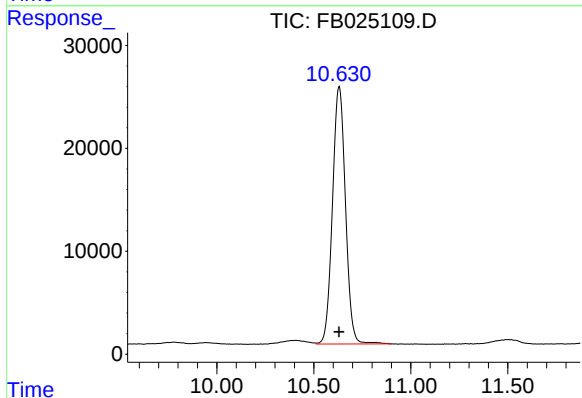


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1163896
Conc: 32.66 ng/ml

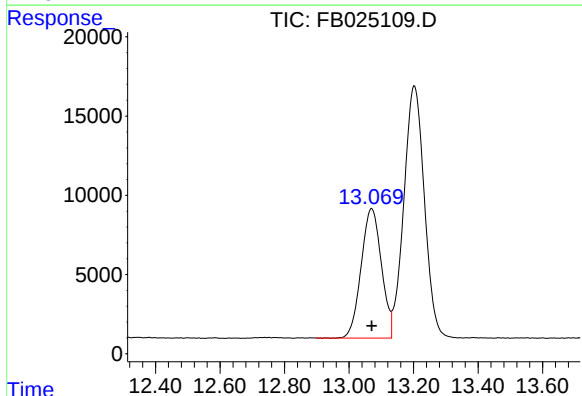


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 356136
Conc: 10.94 ng/ml

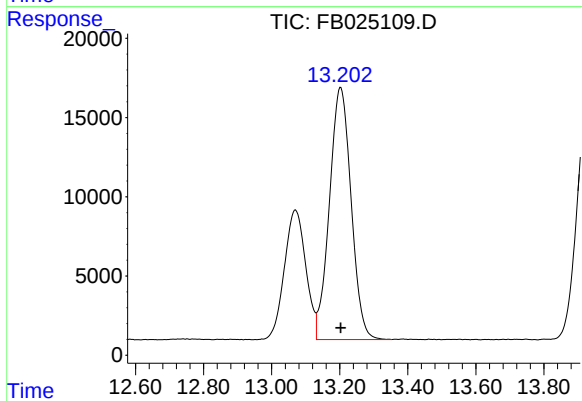


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 703785
Conc: 21.94 ng/ml

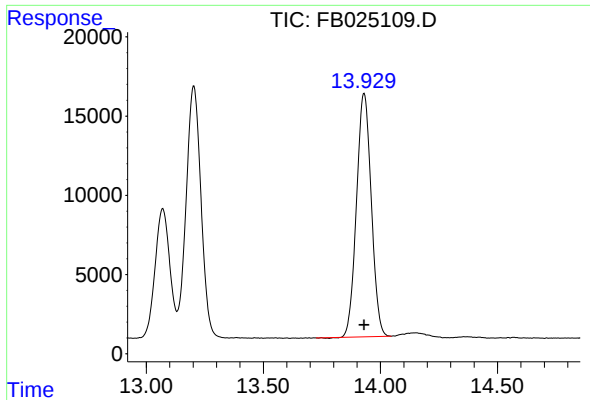

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 673723
Conc: 21.86 ng/ml

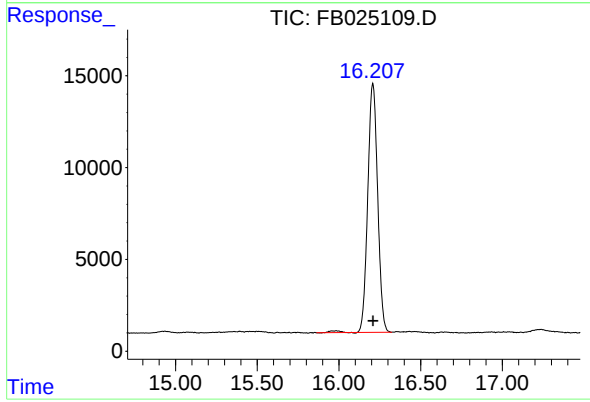

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 573926
Conc: 21.98 ng/ml