

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
 Data File : FB025110.D
 Signal(s) : FID2B.CH
 Acq On : 20 Oct 2020 11:01
 Operator : DD/AJ
 Sample : L4214-03
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 21 01:06:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	428013	20.049 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	49849	1.639 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	56866	1.825 ng/ml
3) t n-Heptane	7.759	23989	0.780 ng/mlm
4) t Benzene	7.889	19842	0.528 ng/mlm
6) t Toluene	10.631	59969	1.683 ng/ml
7) t Ethylbenzene	13.071	20673	0.635 ng/ml
8) t m-Xylene	13.199	40466	1.262 ng/ml
9) t O-Xylene	13.929	38859	1.261 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	32188	1.233 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
Data File : FB025110.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2020 11:01
Operator : DD/AJ
Sample : L4214-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 21 01:06:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

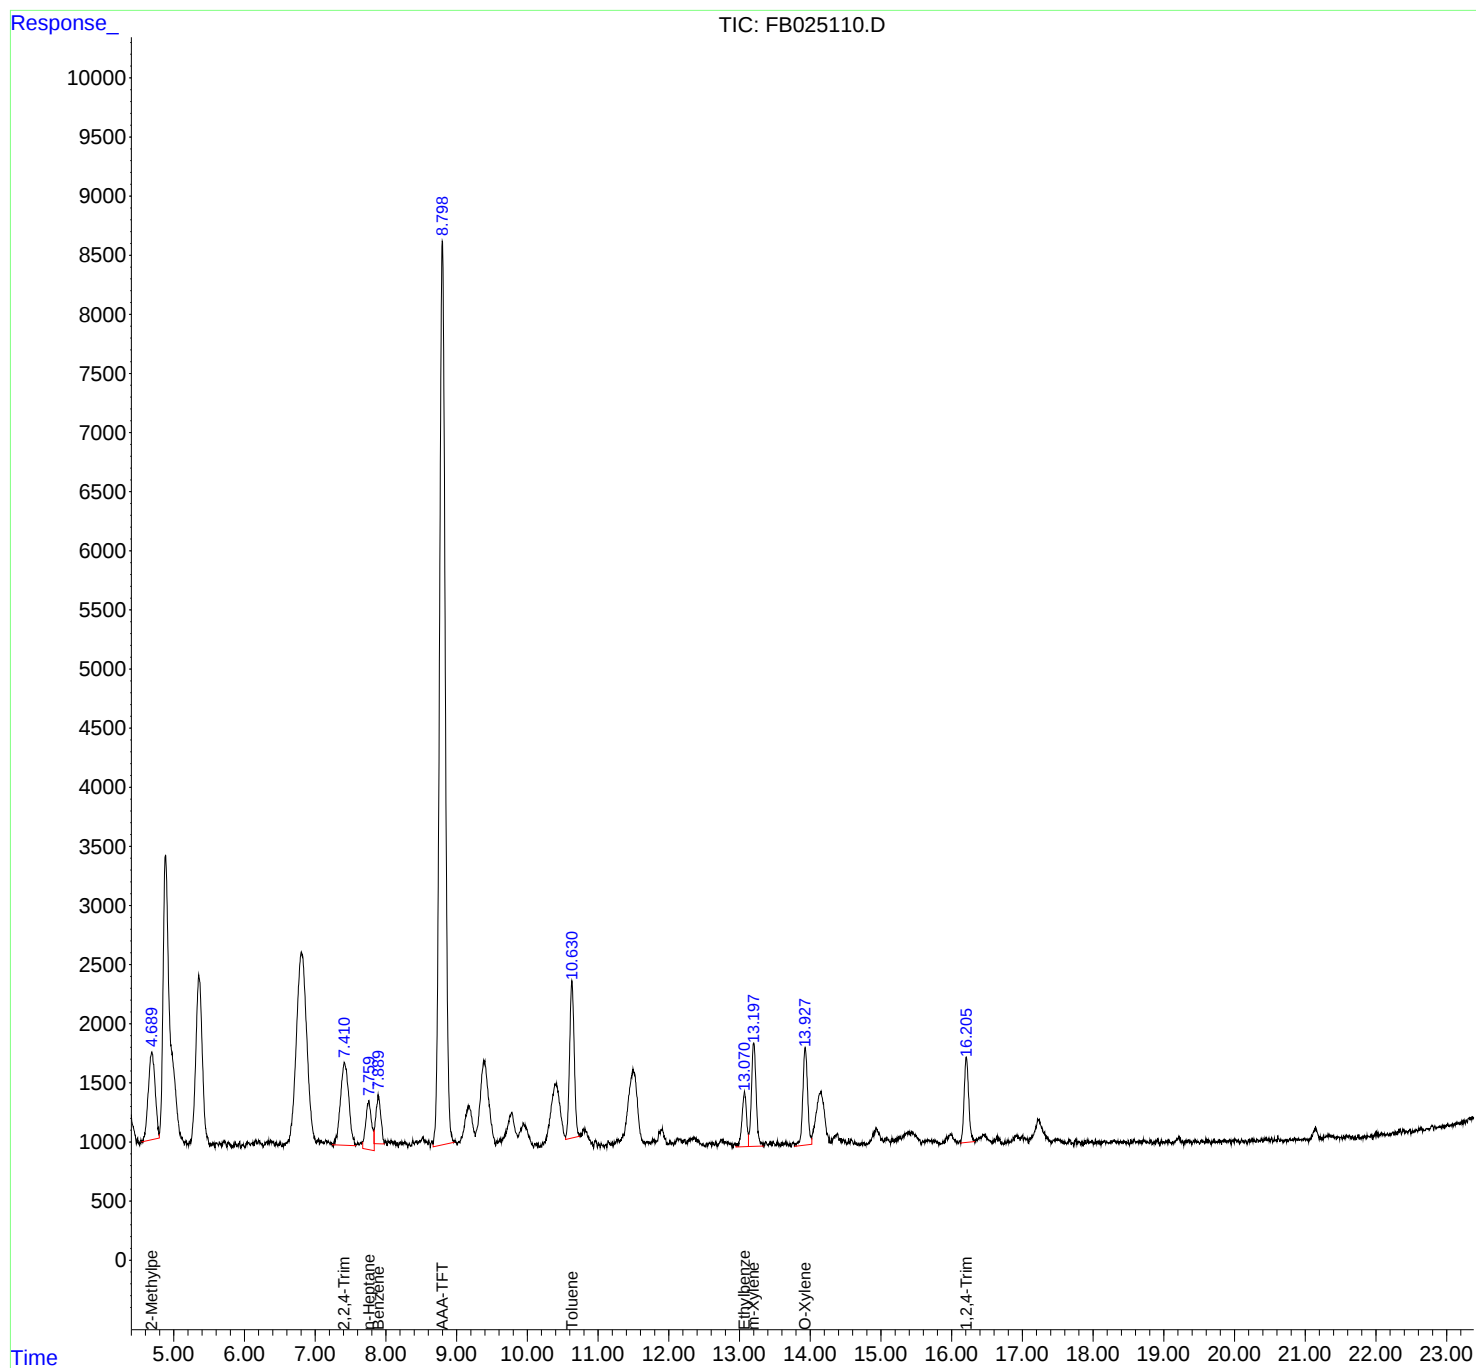

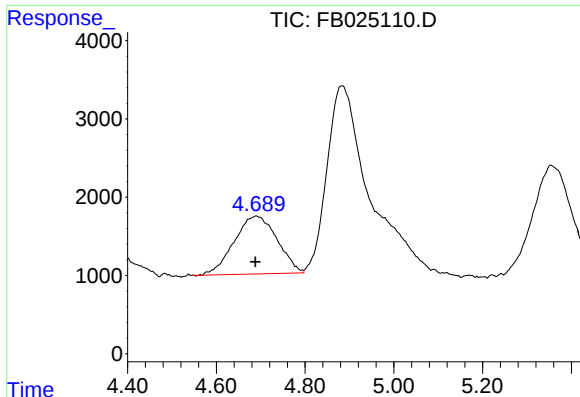


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.003 min
Response: 49849
Conc: 1.64 ng/ml

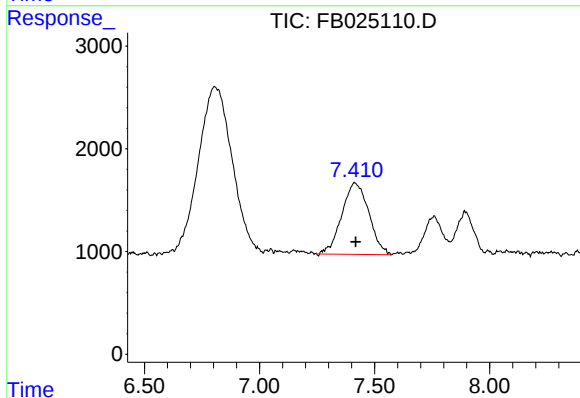


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 56866
Conc: 1.83 ng/ml

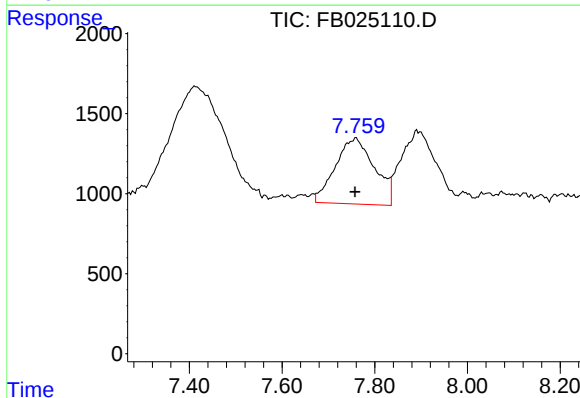


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 23989
Conc: 0.78 ng/ml m

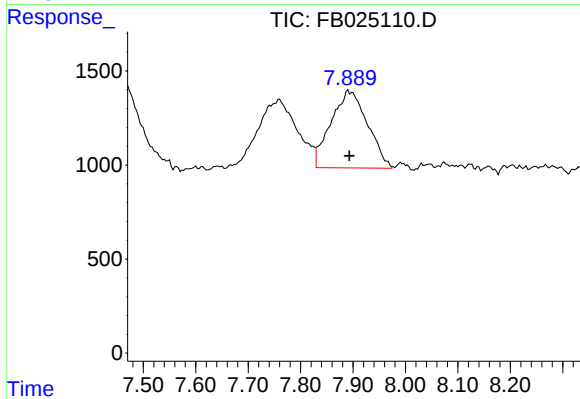


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 19842
Conc: 0.53 ng/ml m

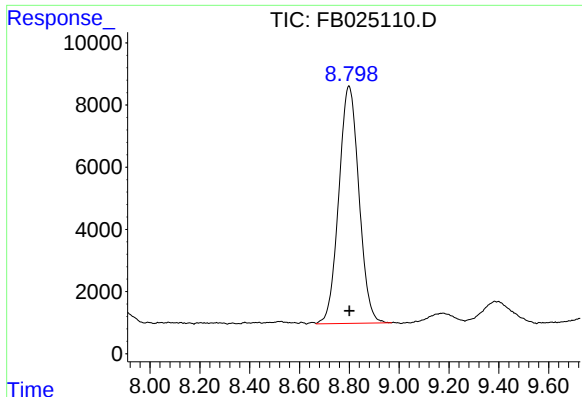


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 428013
Conc: 20.05 ng/ml

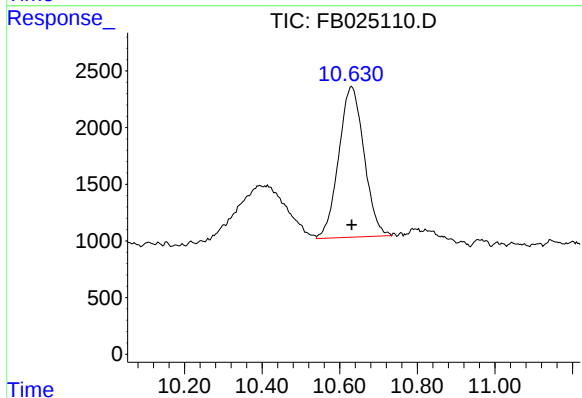


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 59969
Conc: 1.68 ng/ml

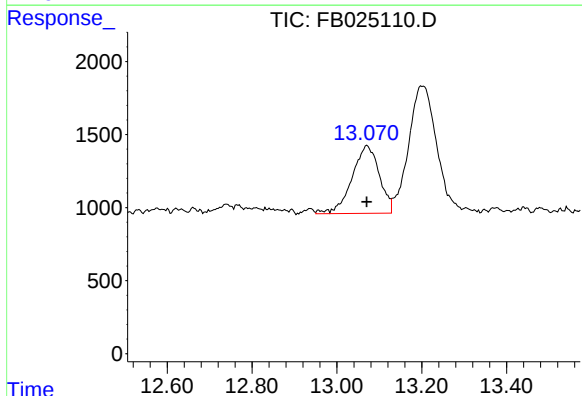


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 20673
Conc: 0.64 ng/ml

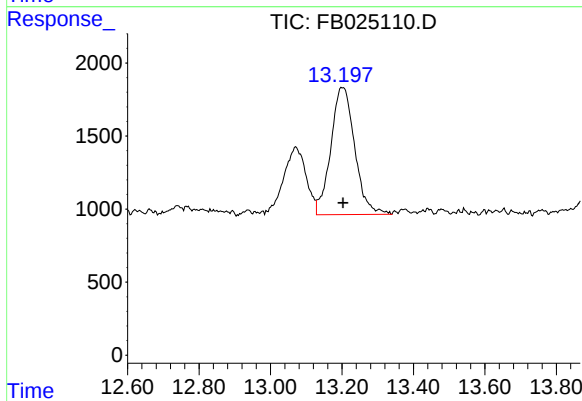


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 40466
Conc: 1.26 ng/ml

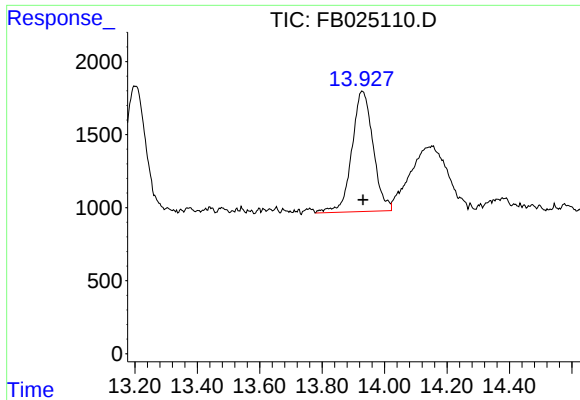

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 38859
Conc: 1.26 ng/ml

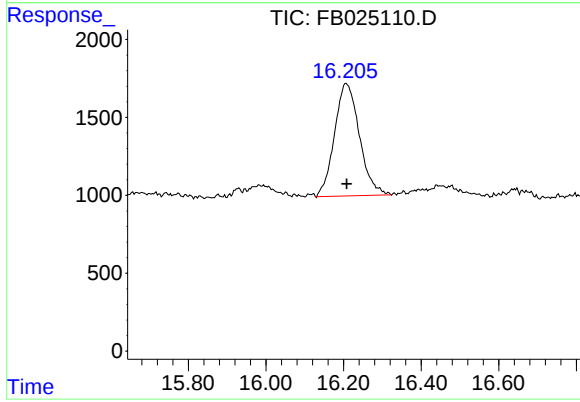

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.001 min
Response: 32188
Conc: 1.23 ng/ml