

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
 Data File : FB025116.D
 Signal(s) : FID2B.CH
 Acq On : 20 Oct 2020 14:05
 Operator : DD/AJ
 Sample : L4222-02MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 21 00:31:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	364793	17.088 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	691334	22.730 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	655737	21.050 ng/ml
3) t n-Heptane	7.758	123214	4.008 ng/ml
4) t Benzene	7.894	303953	8.087 ng/ml
6) t Toluene	10.632	784475	22.012 ng/ml
7) t Ethylbenzene	13.068	407568	12.521 ng/ml
8) t m-Xylene	13.204	398251	12.418 ng/ml
9) t O-Xylene	13.931	543952	17.645 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	489287	18.740 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102020\
Data File : FB025116.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2020 14:05
Operator : DD/AJ
Sample : L4222-02MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 21 00:31:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

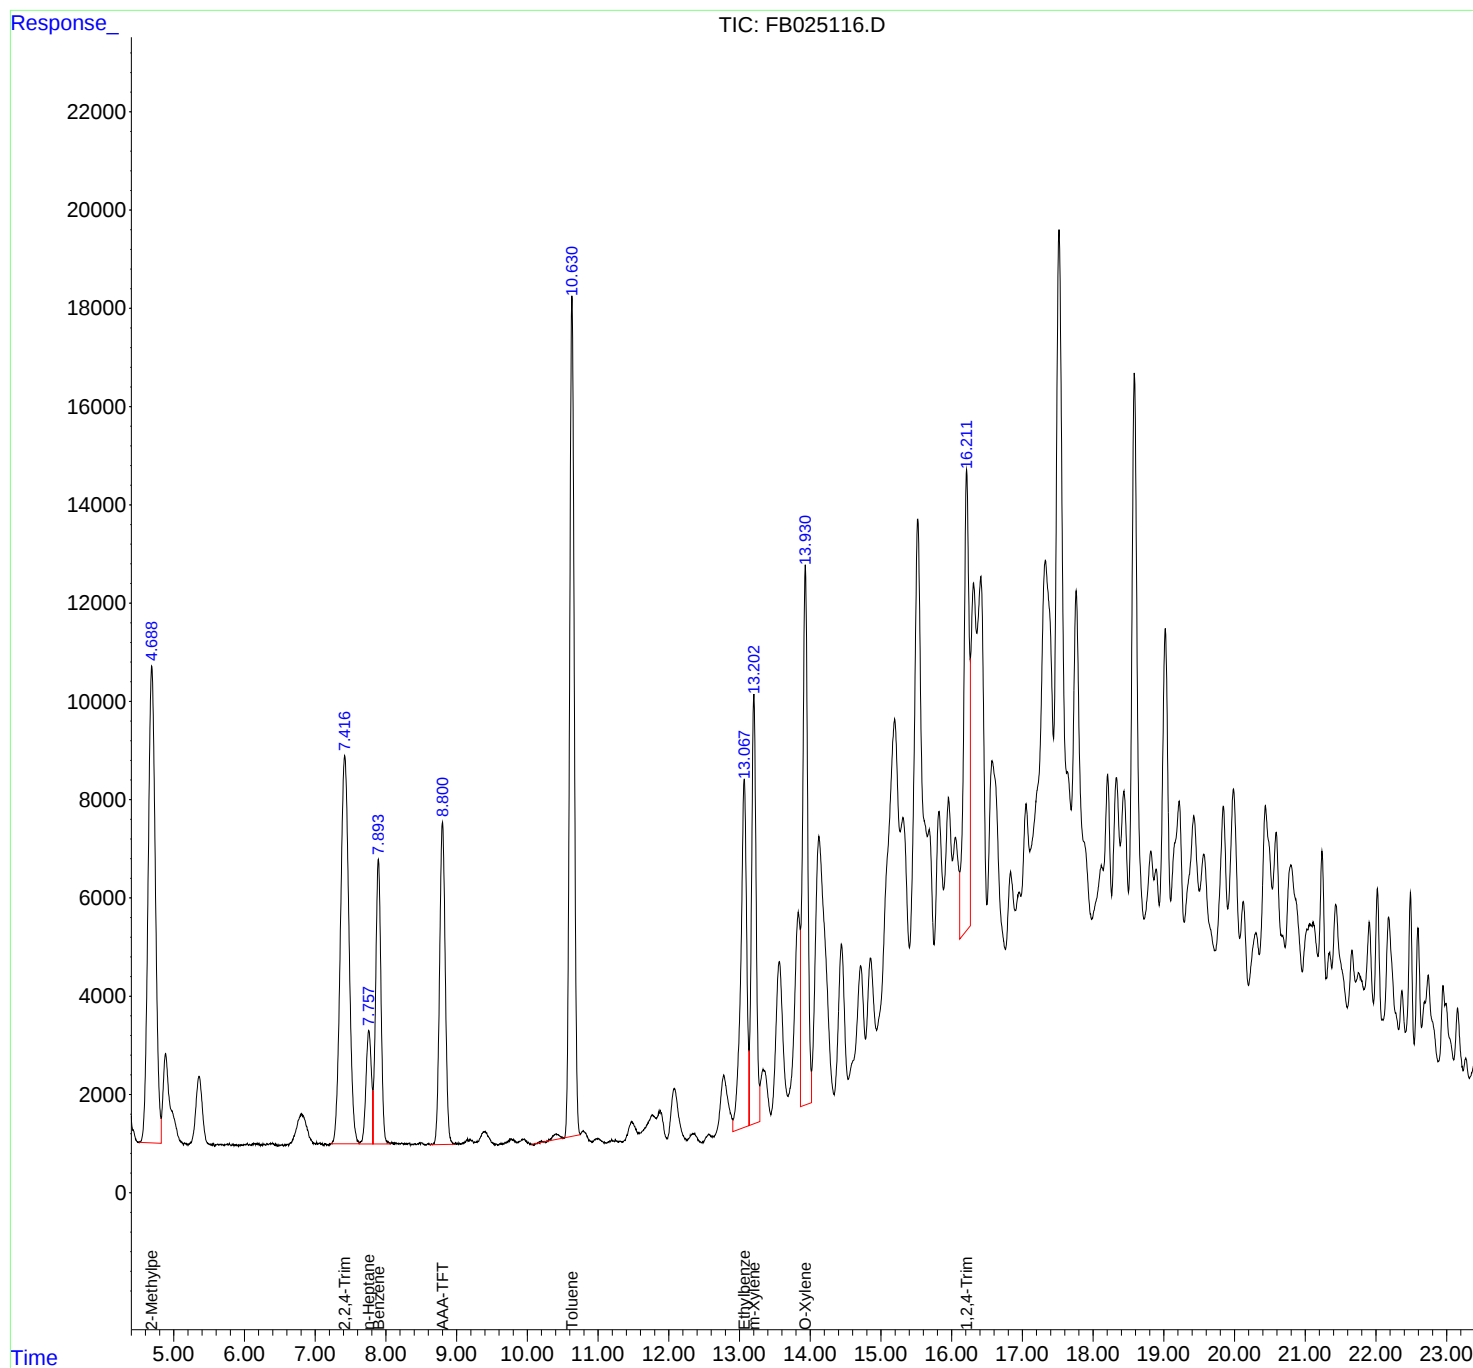

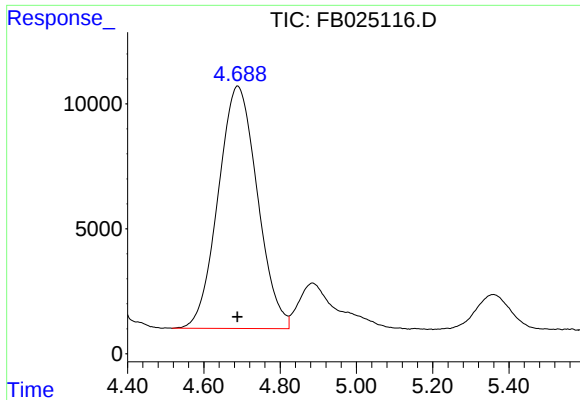


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.001 min
Response: 691334
Conc: 22.73 ng/ml

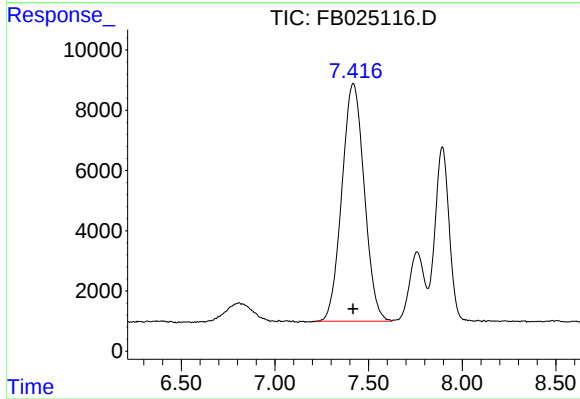


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 655737
Conc: 21.05 ng/ml

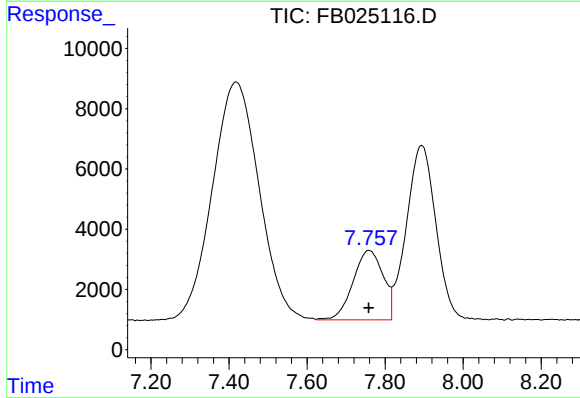


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 123214
Conc: 4.01 ng/ml

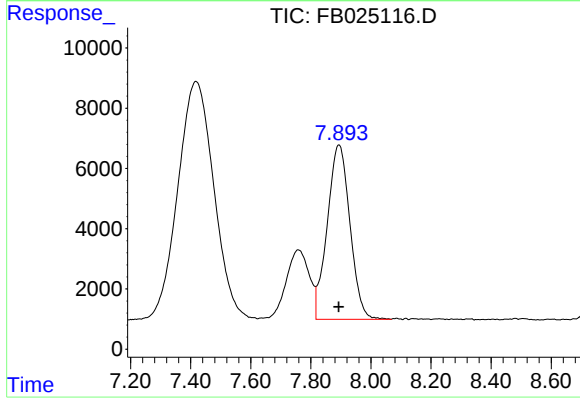


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.001 min
Response: 303953
Conc: 8.09 ng/ml

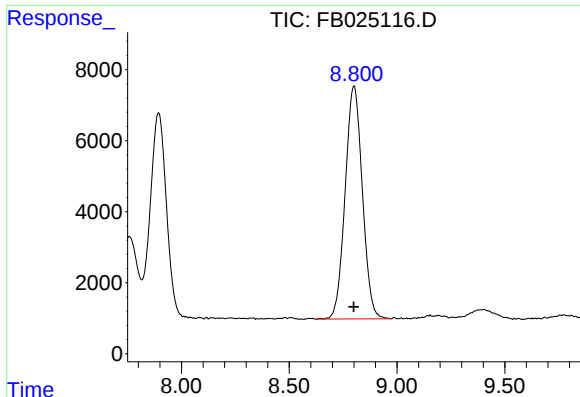


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.001 min
Response: 364793
Conc: 17.09 ng/ml

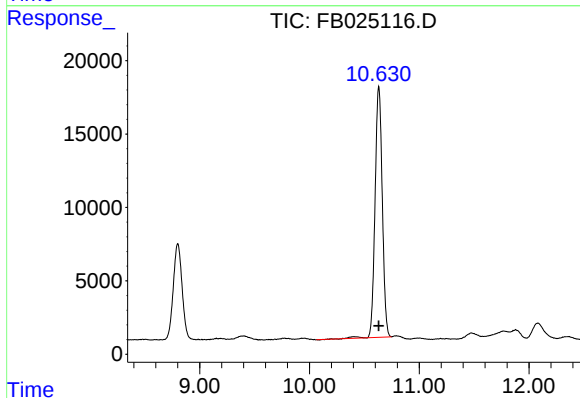


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 784475
Conc: 22.01 ng/ml

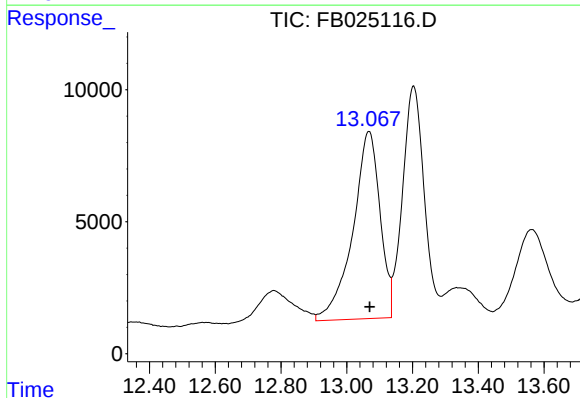


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 407568
Conc: 12.52 ng/ml

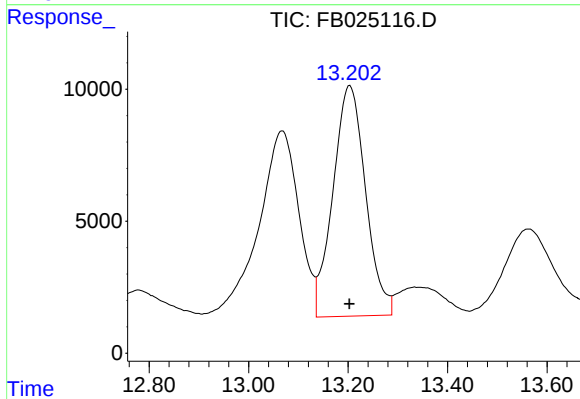


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 398251
Conc: 12.42 ng/ml

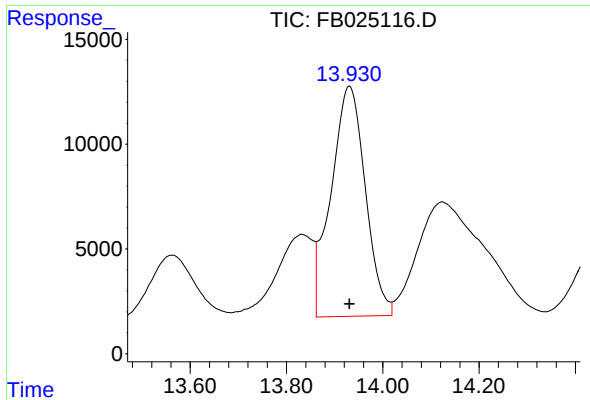

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 543952
Conc: 17.65 ng/ml

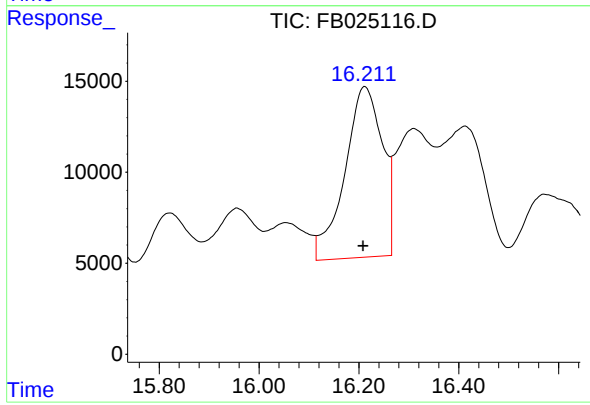

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.004 min
Response: 489287
Conc: 18.74 ng/ml