

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028659.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 15:11
Operator : AJ/MA
Sample : N5193-05
Misc : 4.88G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-SS-03-01-03

Integration File: Calibration.e
Quant Time: Oct 21 03:50:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	32822	2.537 ng/ml
Target Compounds			
7) t Ethylbenzene	13.021	12615	0.636 ng/ml
9) t O-Xylene	13.931	15784	0.811 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	38970	2.013 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028659.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 15:11
Operator : AJ/MA
Sample : N5193-05
Misc : 4.88G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-SS-03-01-03

Integration File: Calibration.e
Quant Time: Oct 21 03:50:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

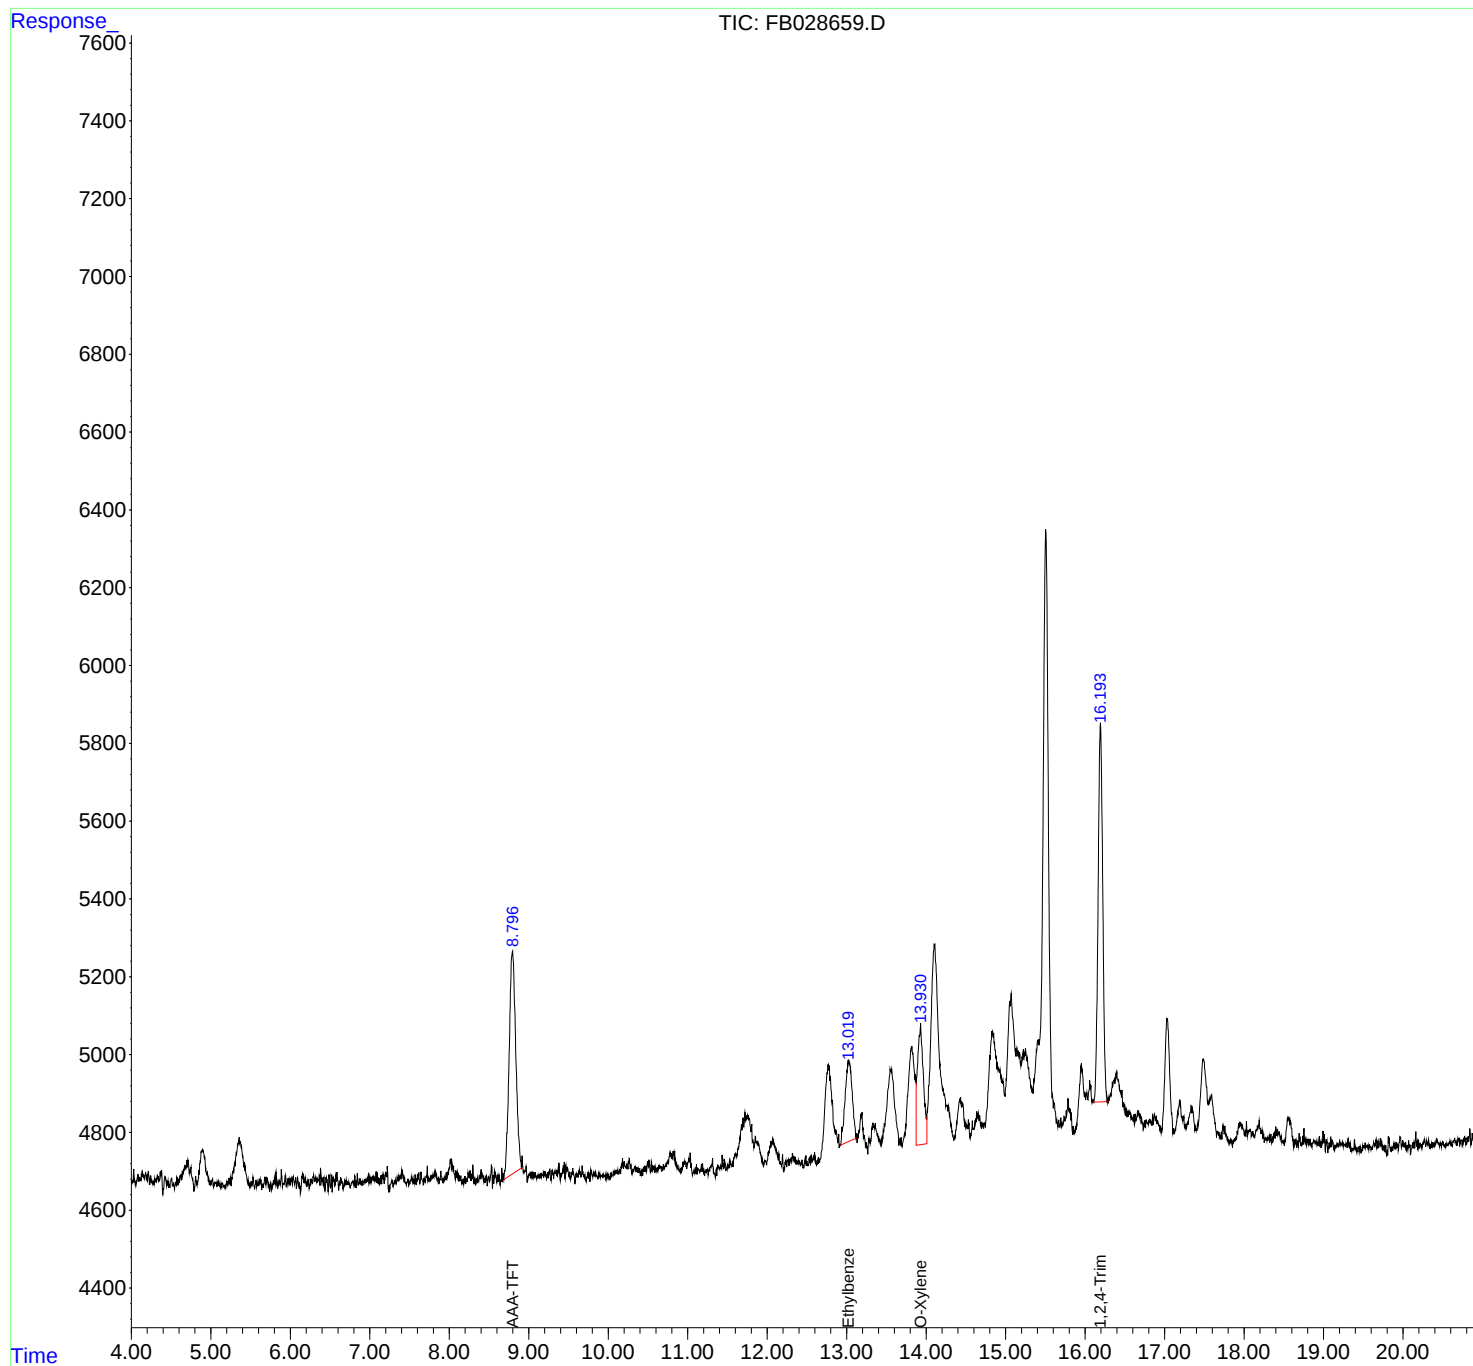


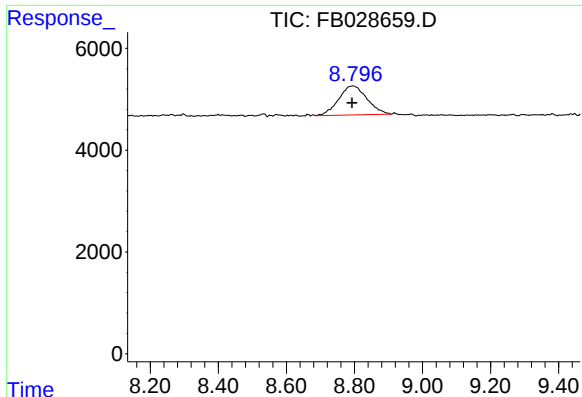

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.004 min
Response: 32822
Conc: 2.54 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-03-01-03

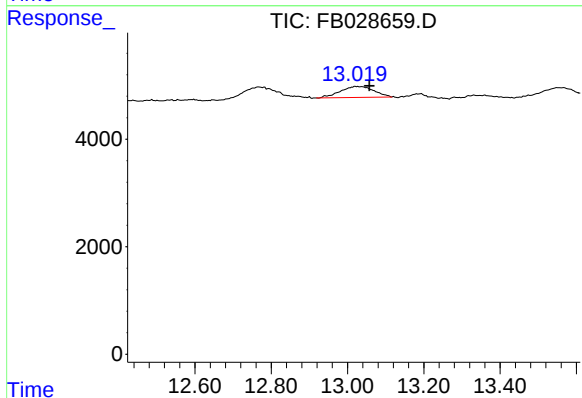


#7 Ethylbenzene

R.T.: 13.021 min
Delta R.T.: -0.037 min
Response: 12615
Conc: 0.64 ng/ml

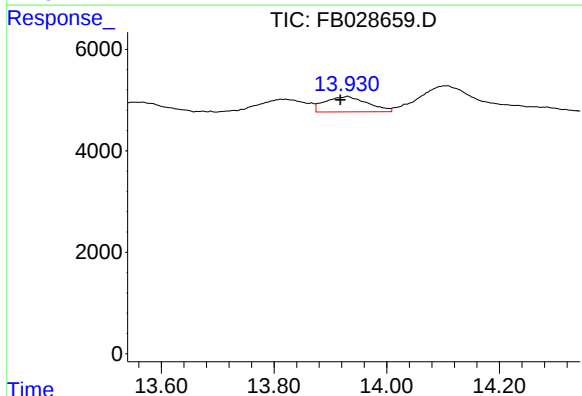

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.014 min
Response: 15784
Conc: 0.81 ng/ml

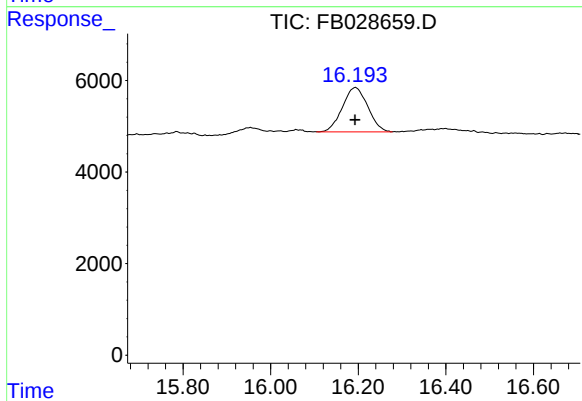

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.001 min
Response: 38970
Conc: 2.01 ng/ml