

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
 Data File : FB028654.D
 Signal(s) : FID2B.CH
 Acq On : 20 Oct 2022 11:53
 Operator : AJ/MA
 Sample : BSF1020S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1020S1

Integration File: Calibration.e
 Quant Time: Oct 21 03:50:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	255001	19.711 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	479001	29.281 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	497246	27.515 ng/ml
3) t n-Heptane	7.747	165591	9.776 ng/ml
4) t Benzene	7.884	202472	9.218 ng/ml
6) t Toluene	10.618	570050	27.197 ng/ml
7) t Ethylbenzene	13.056	179164	9.028 ng/ml
8) t m-Xylene	13.189	353032	17.920 ng/ml
9) t O-Xylene	13.916	352160	18.102 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	345915	17.868 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028654.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 11:53
Operator : AJ/MA
Sample : BSF1020S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1020S1

Integration File: Calibration.e
Quant Time: Oct 21 03:50:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

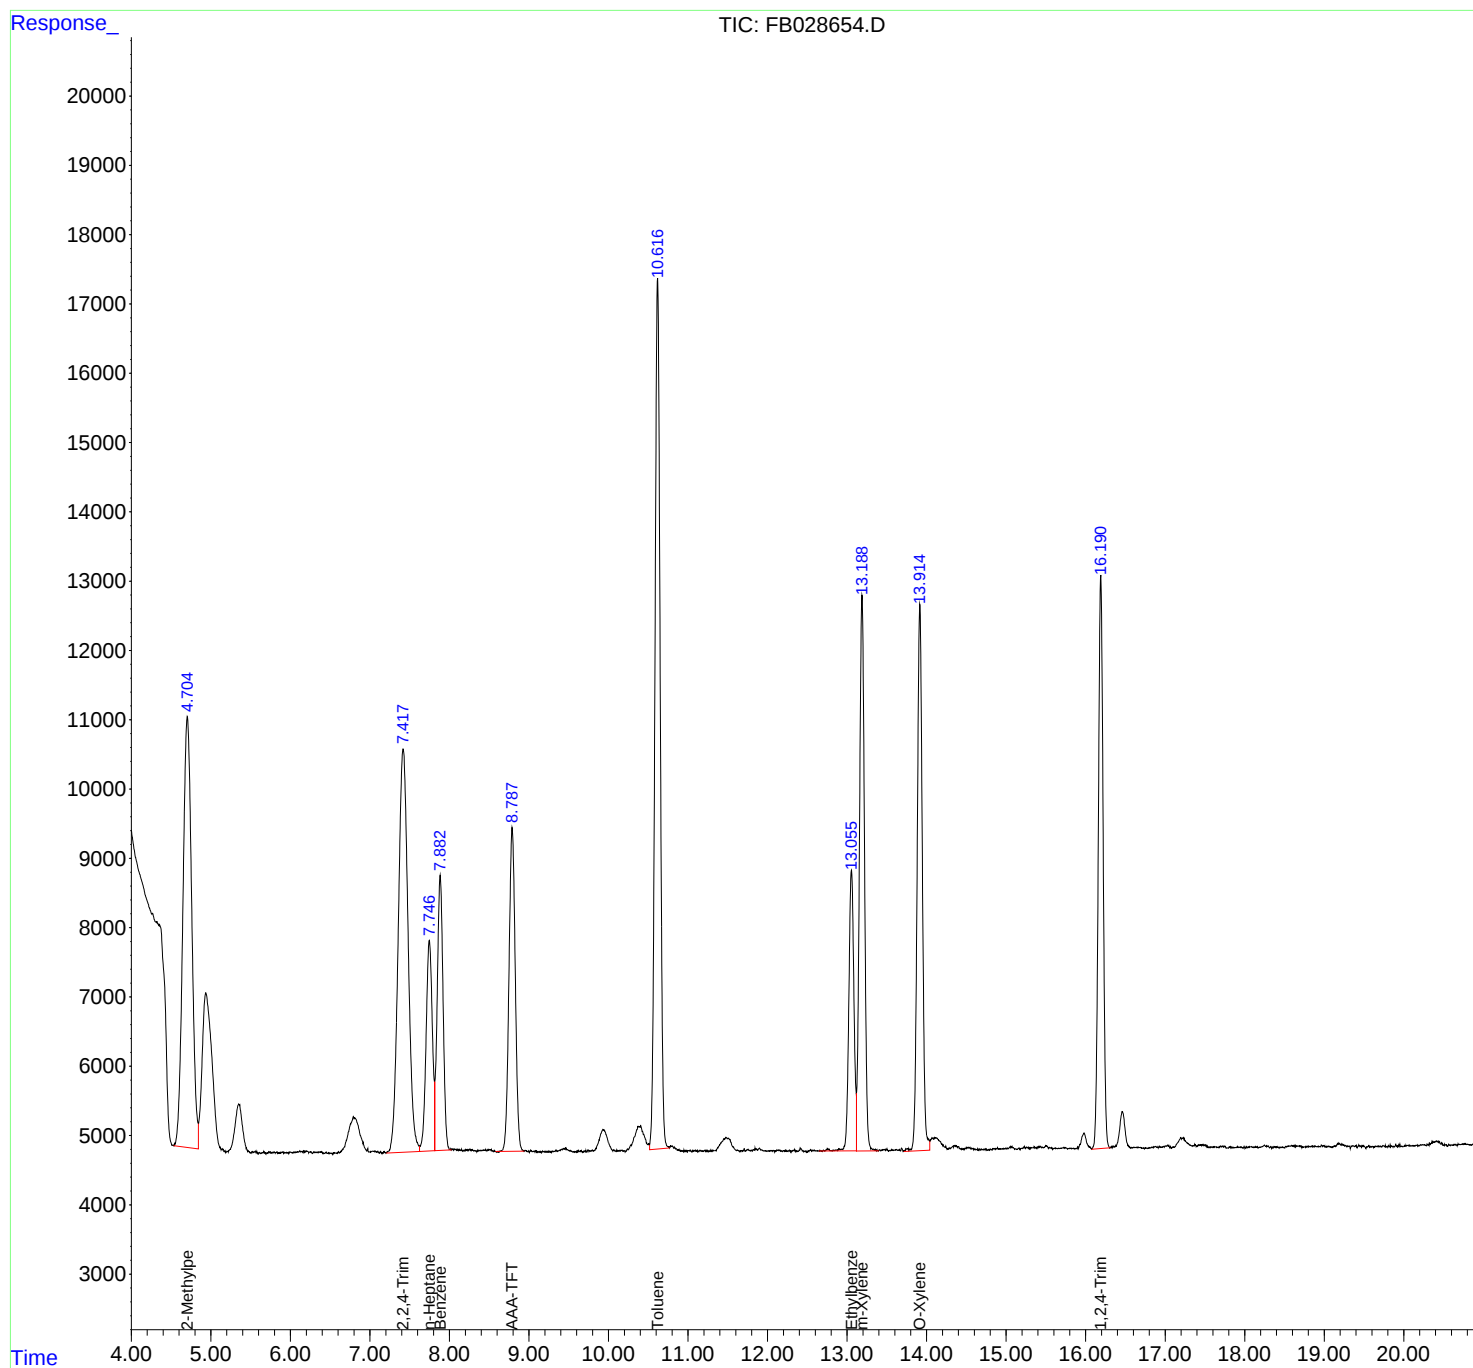


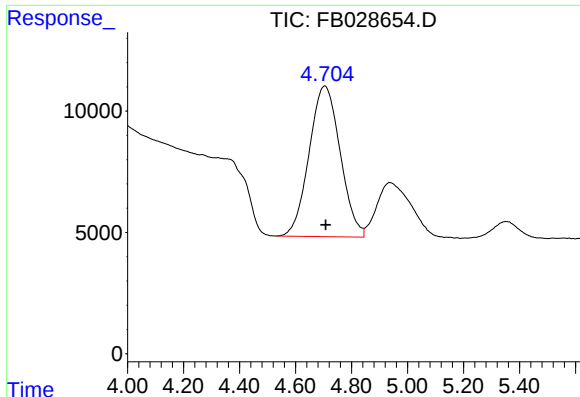

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 479001
Conc: 29.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S1

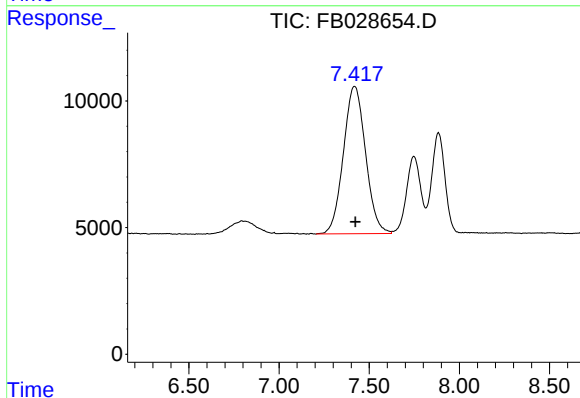


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.005 min
Response: 497246
Conc: 27.51 ng/ml

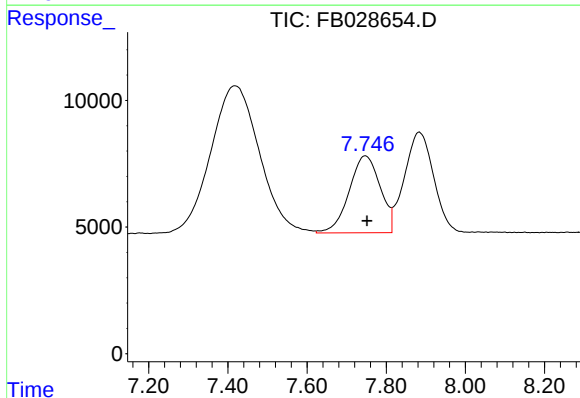


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 165591
Conc: 9.78 ng/ml

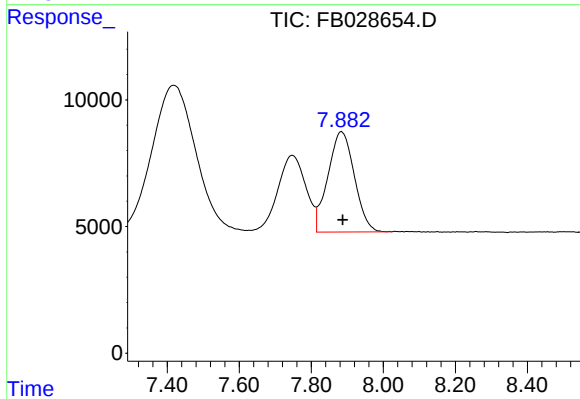

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.004 min
Response: 202472
Conc: 9.22 ng/ml

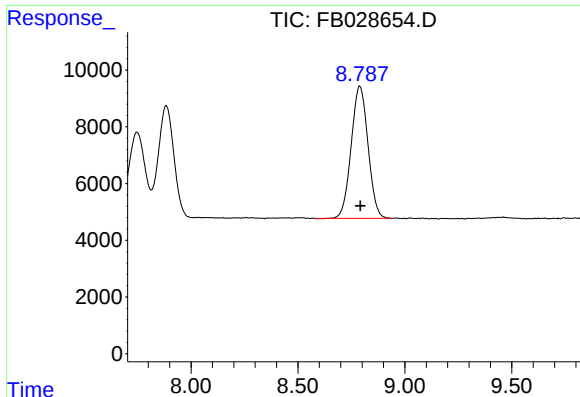

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 255001
Conc: 19.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S1

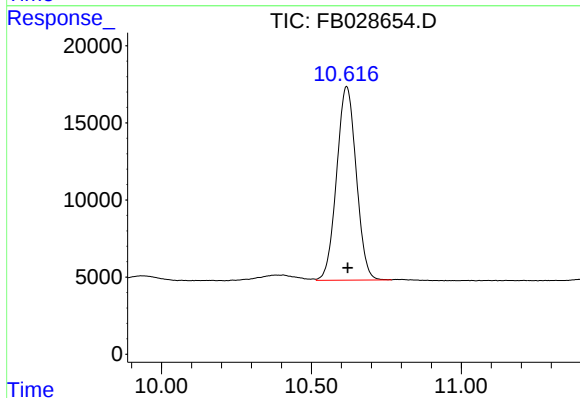


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 570050
Conc: 27.20 ng/ml

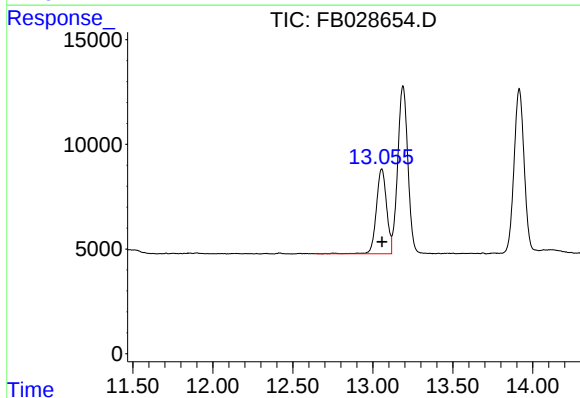


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 179164
Conc: 9.03 ng/ml

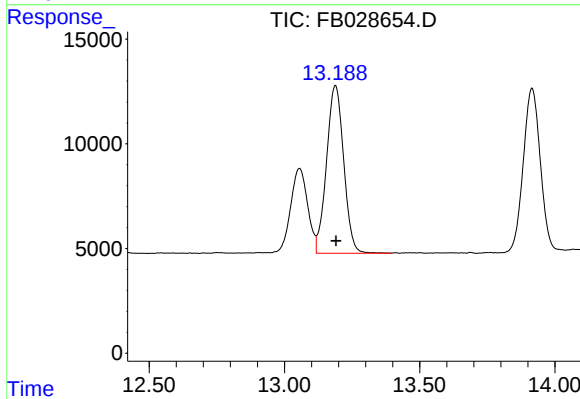

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.002 min
Response: 353032
Conc: 17.92 ng/ml

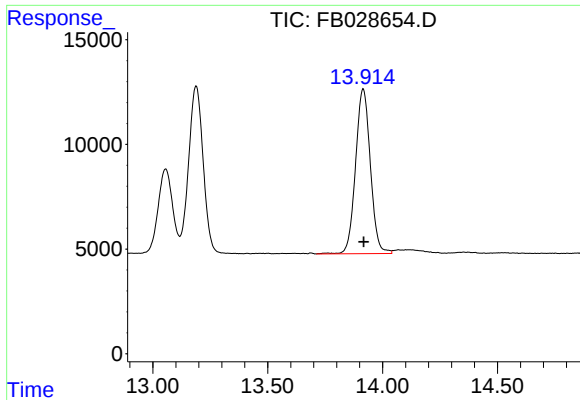

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.002 min
Response: 352160
Conc: 18.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S1

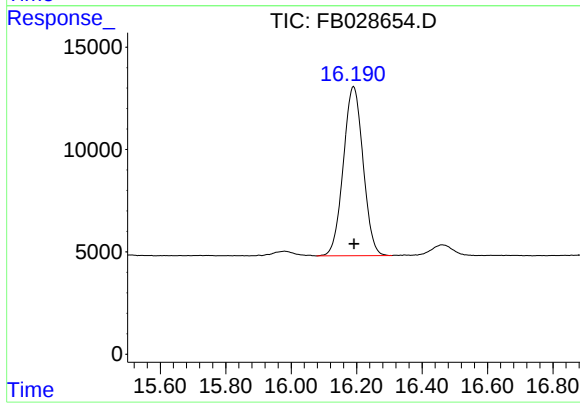

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.002 min
Response: 345915
Conc: 17.87 ng/ml