

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028656.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 13:13
Operator : AJ/MA
Sample : N5193-02
Misc : 4.10G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-DS-01-09-11

Integration File: Calibration.e
Quant Time: Oct 21 03:50:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	7996	0.618 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028656.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 13:13
Operator : AJ/MA
Sample : N5193-02
Misc : 4.10G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-DS-01-09-11

Integration File: Calibration.e
Quant Time: Oct 21 03:50:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

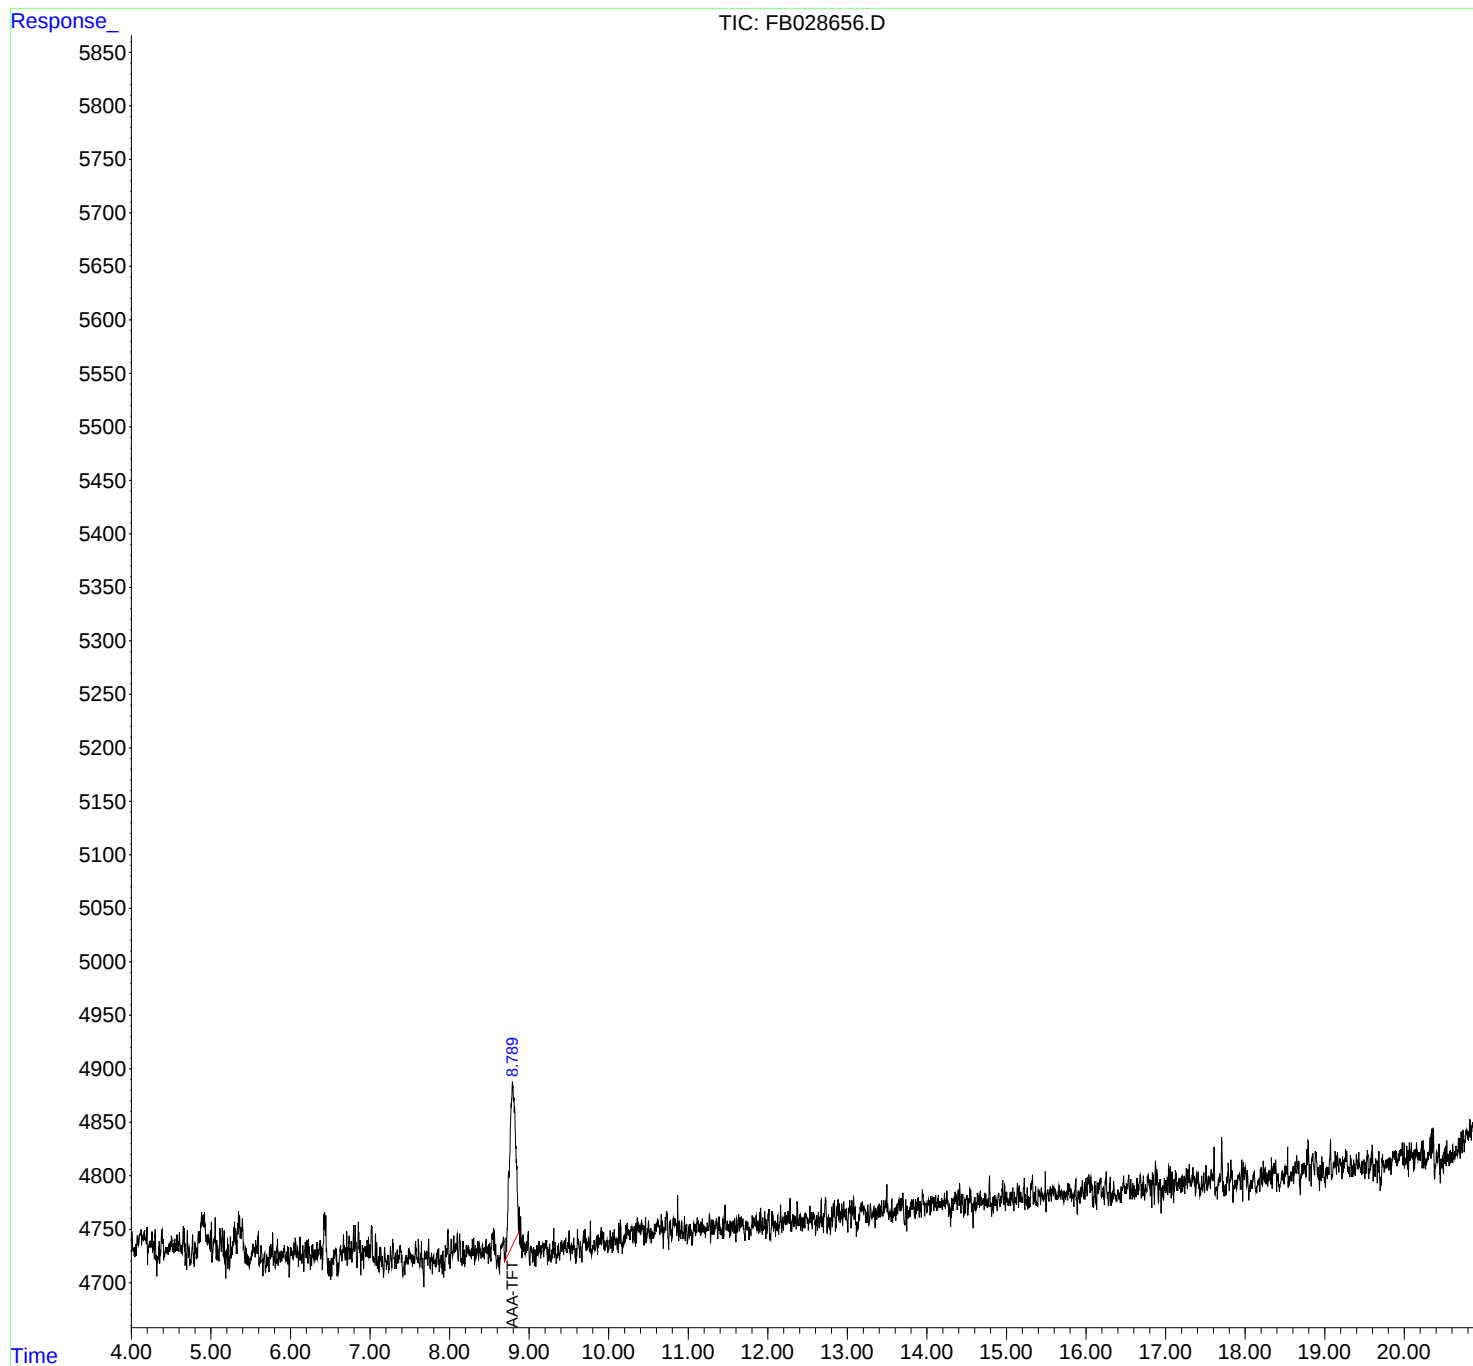

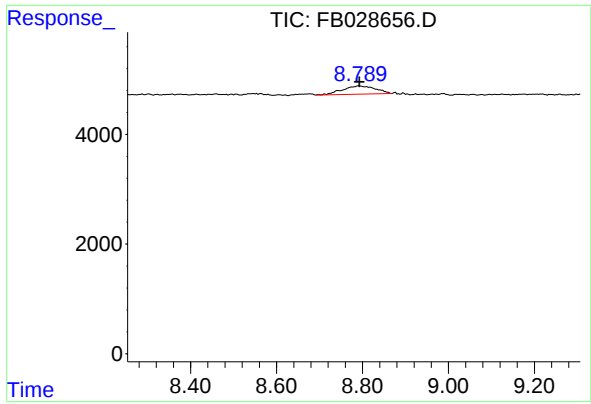

#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 7996
Conc: 0.62 ng/ml

Instrument :

FID_B

ClientSampleId :

LSP-DS-01-09-11