

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
 Data File : FB028660.D
 Signal(s) : FID2B.CH
 Acq On : 20 Oct 2022 15:50
 Operator : AJ/MA
 Sample : BSF1020S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1020S2

Integration File: Calibration.e
 Quant Time: Oct 21 03:50:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	246516	19.055 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	513215	31.372 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	568012	31.430 ng/ml
3) t n-Heptane	7.752	174707	10.314 ng/ml
4) t Benzene	7.888	210825	9.598 ng/ml
6) t Toluene	10.622	600148	28.633 ng/ml
7) t Ethylbenzene	13.059	189497	9.548 ng/ml
8) t m-Xylene	13.191	376790	19.126 ng/ml
9) t O-Xylene	13.918	378059	19.433 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	382595	19.763 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102022\
Data File : FB028660.D
Signal(s) : FID2B.CH
Acq On : 20 Oct 2022 15:50
Operator : AJ/MA
Sample : BSF1020S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1020S2

Integration File: Calibration.e
Quant Time: Oct 21 03:50:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

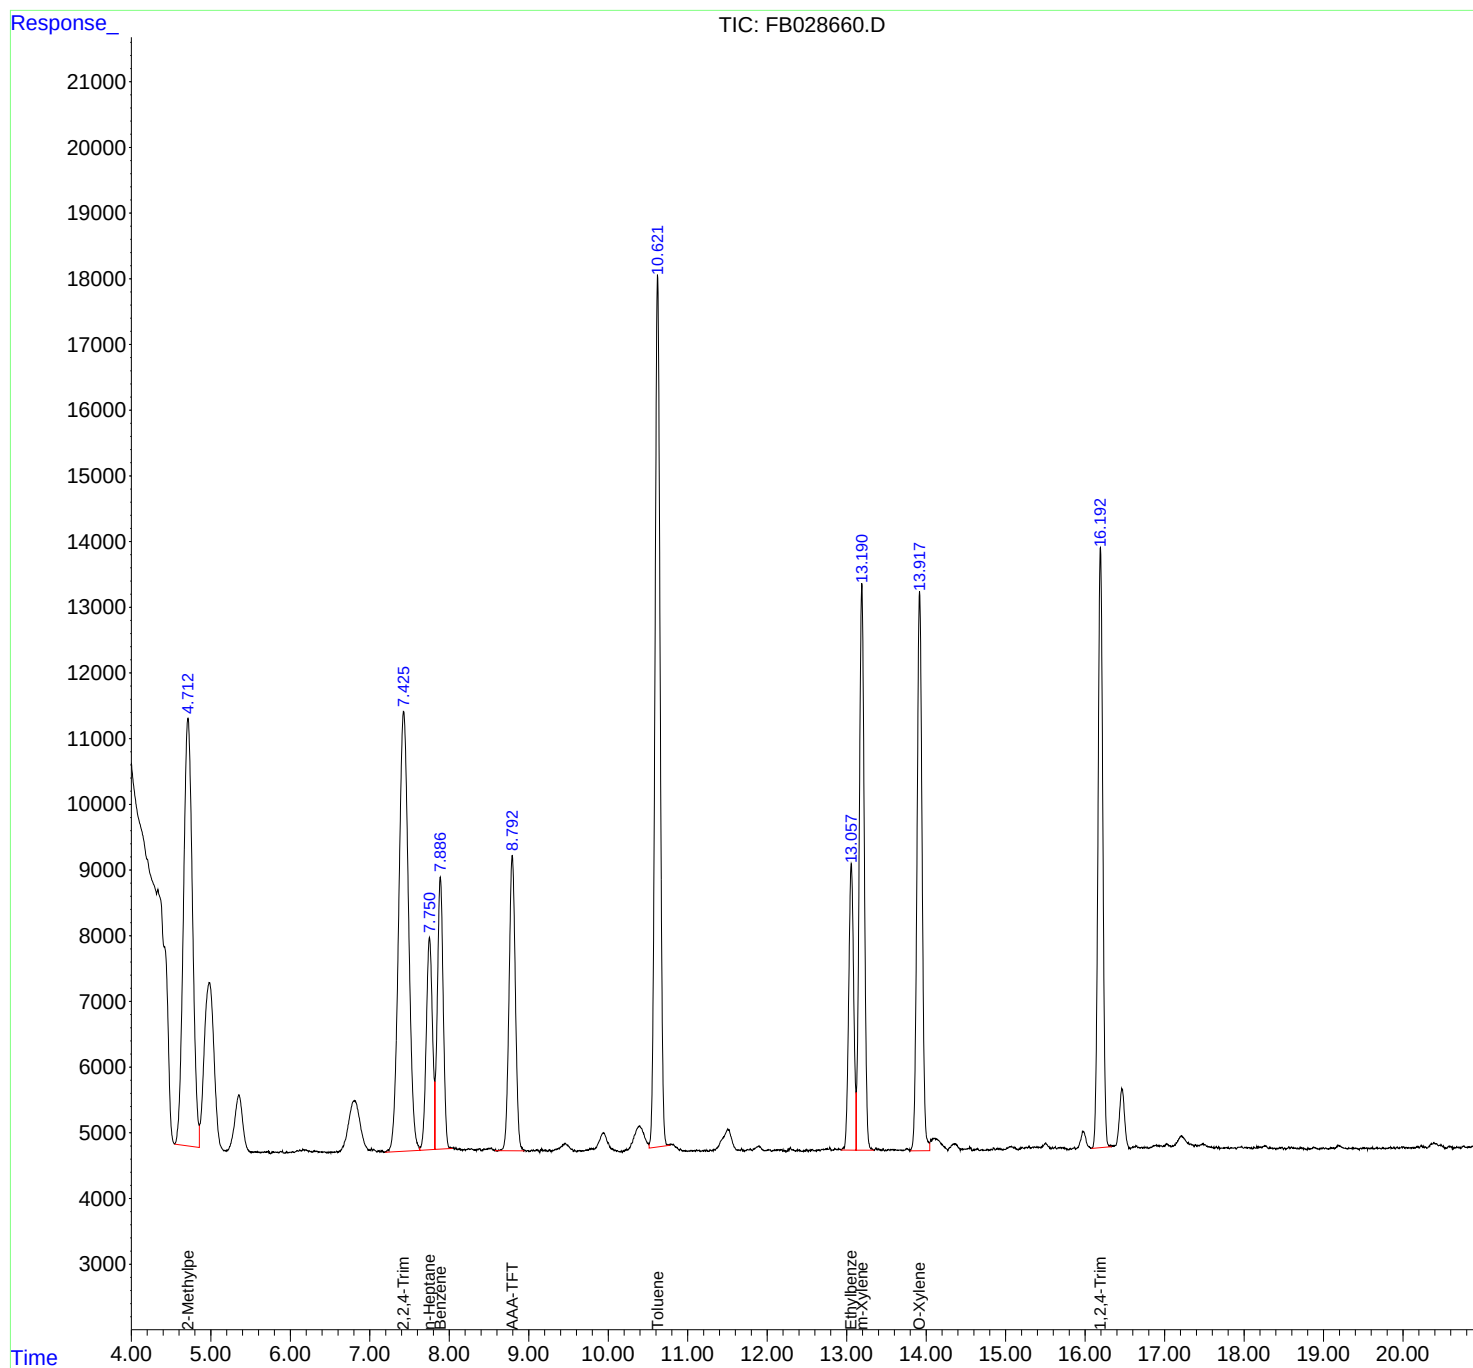


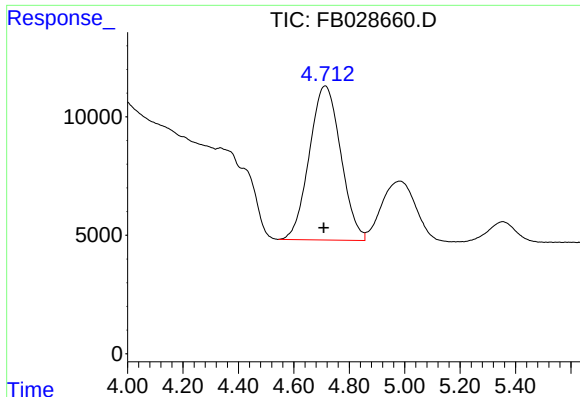

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.006 min
Response: 513215
Conc: 31.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S2

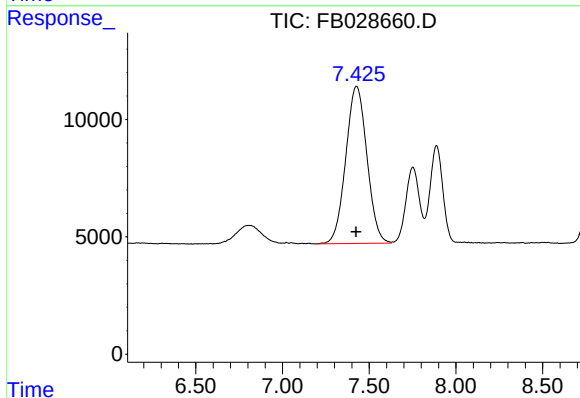


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.003 min
Response: 568012
Conc: 31.43 ng/ml

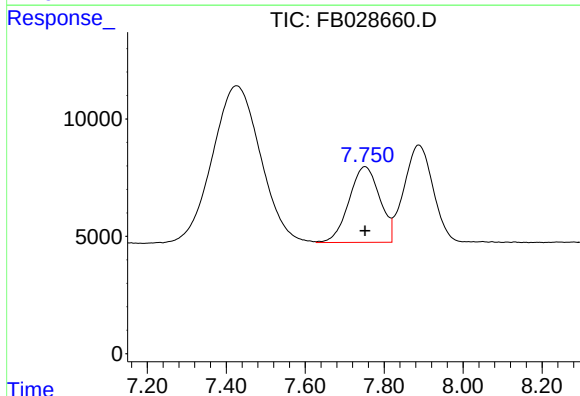


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 174707
Conc: 10.31 ng/ml

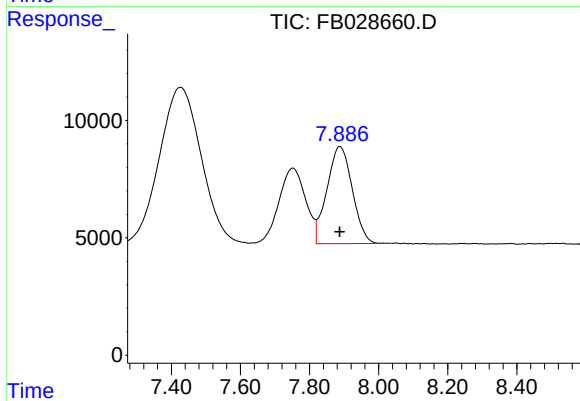

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 210825
Conc: 9.60 ng/ml

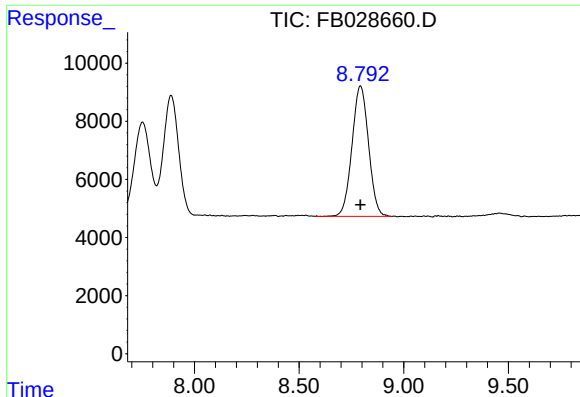

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 246516
Conc: 19.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S2

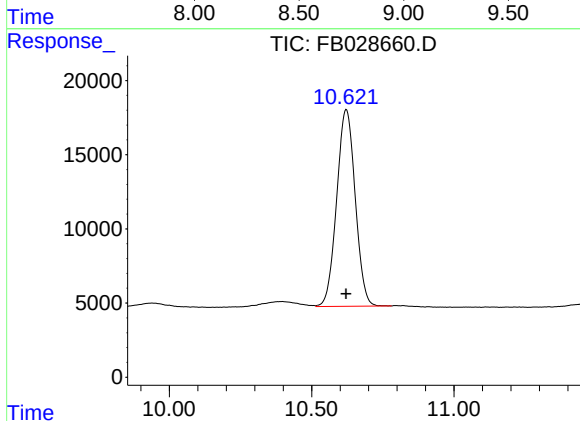


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 600148
Conc: 28.63 ng/ml

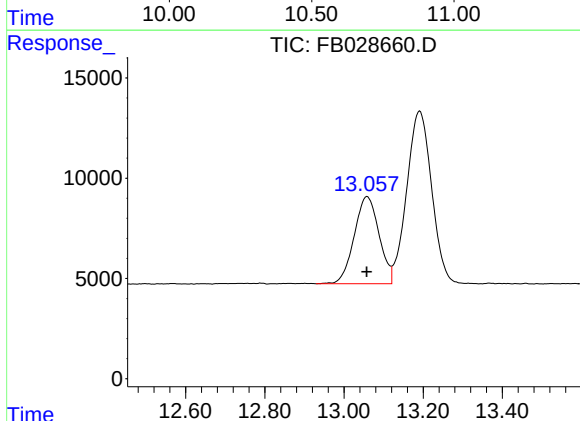


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 189497
Conc: 9.55 ng/ml

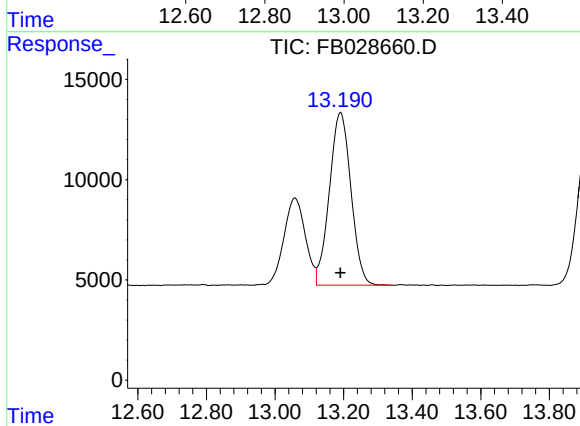

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 376790
Conc: 19.13 ng/ml

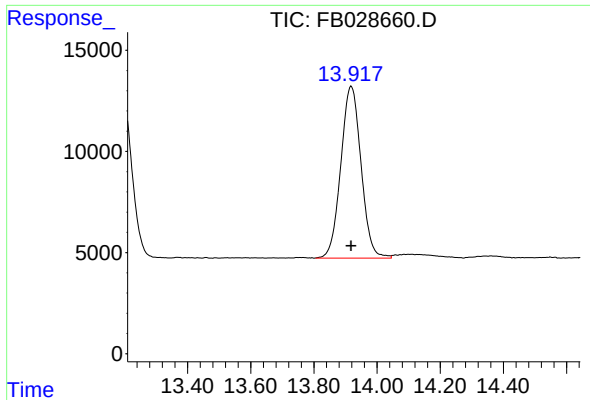

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 378059
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1020S2

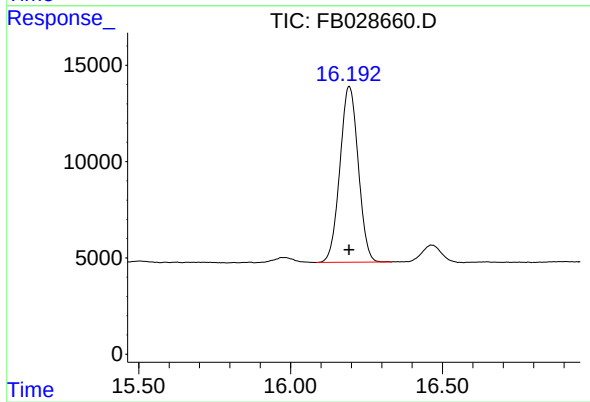

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 382595
Conc: 19.76 ng/ml