

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102119\
 Data File : FB022793.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2019 15:59
 Operator : DD/AJ
 Sample : K5448-03MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 22 03:04:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	490262	19.375 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	934639	27.502 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1056014	29.021 ng/ml
3) t n-Heptane	7.756	347263	9.517 ng/ml
4) t Benzene	7.890	410102	9.288 ng/ml
6) t Toluene	10.628	1186606	27.531 ng/ml
7) t Ethylbenzene	13.068	372691	9.176 ng/ml
8) t m-Xylene	13.201	699233	18.173 ng/ml
9) t O-Xylene	13.929	665377	18.269 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	522471	18.335 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102119\
Data File : FB022793.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2019 15:59
Operator : DD/AJ
Sample : K5448-03MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 03:04:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

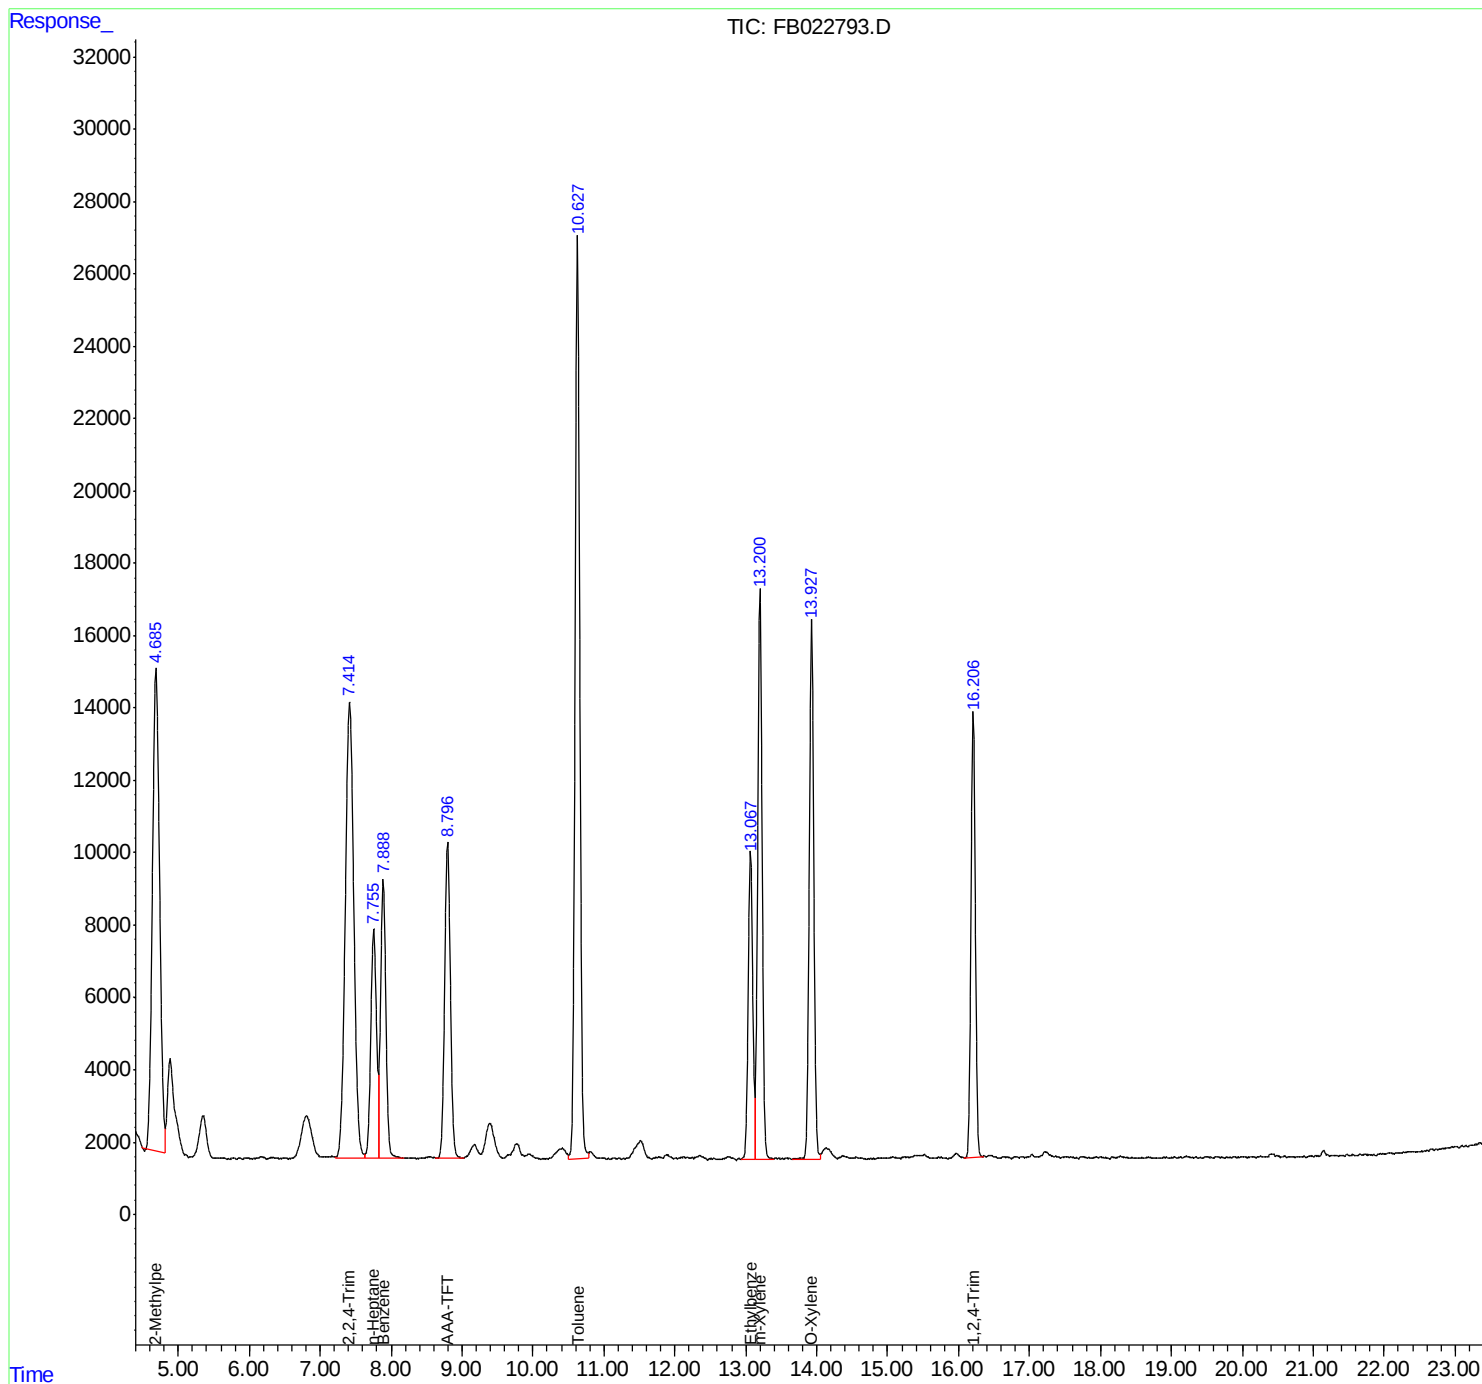

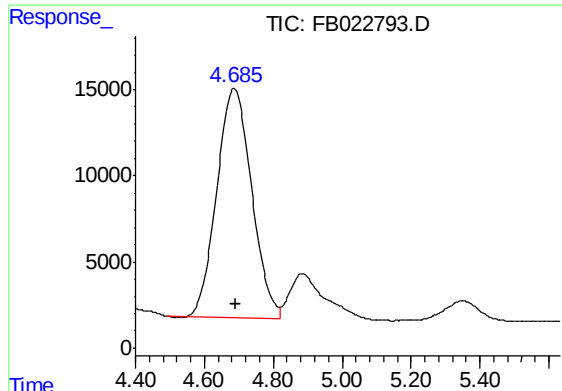


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.004 min
Response: 934639
Conc: 27.50 ng/ml

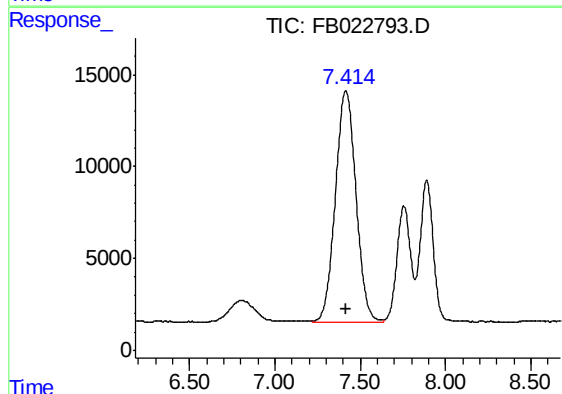


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 1056014
Conc: 29.02 ng/ml

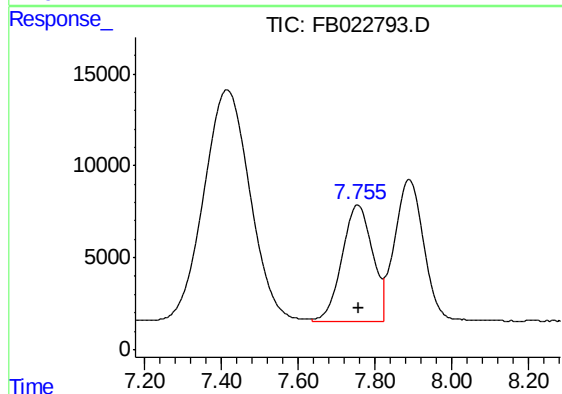


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 347263
Conc: 9.52 ng/ml

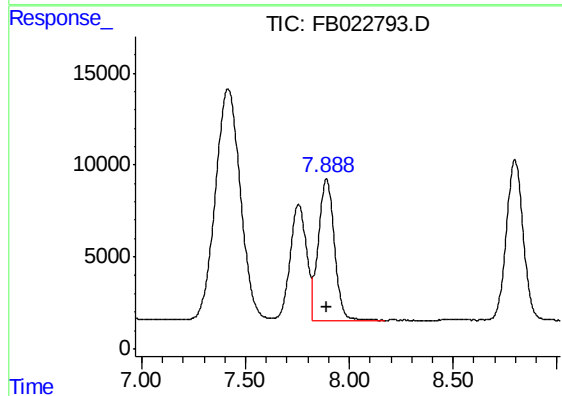


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 410102
Conc: 9.29 ng/ml

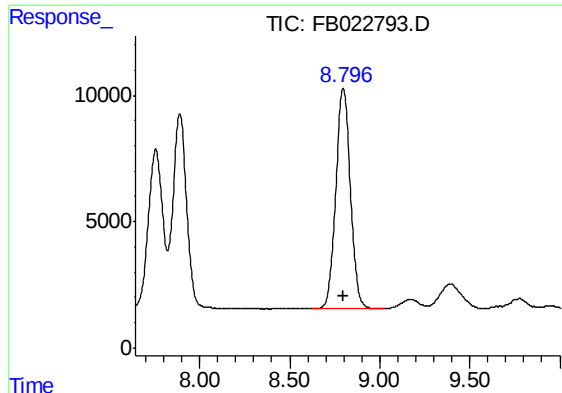


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 490262
Conc: 19.37 ng/ml

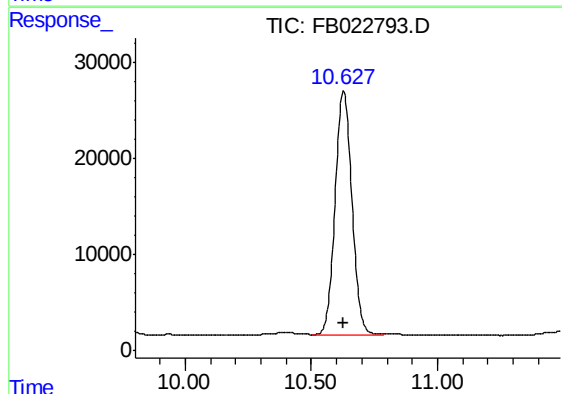


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.001 min
Response: 1186606
Conc: 27.53 ng/ml

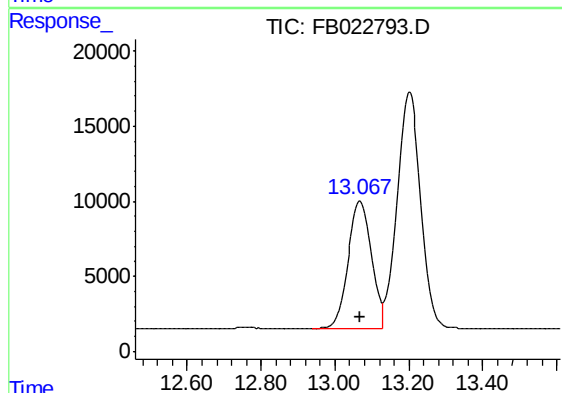


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.001 min
Response: 372691
Conc: 9.18 ng/ml

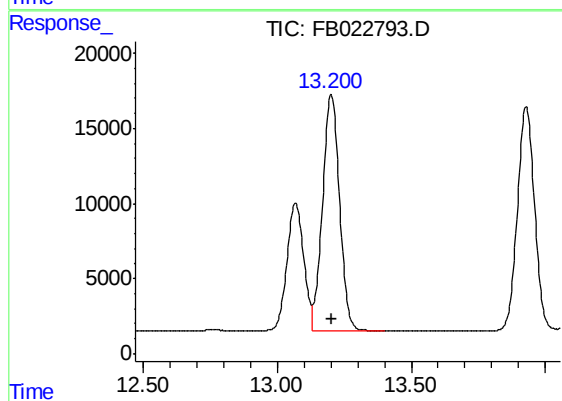


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.001 min
Response: 699233
Conc: 18.17 ng/ml

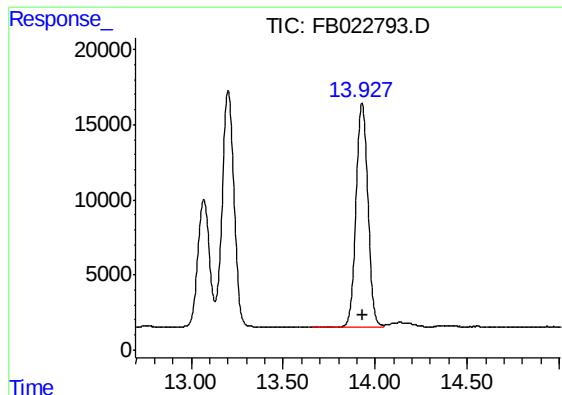

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 665377
Conc: 18.27 ng/ml

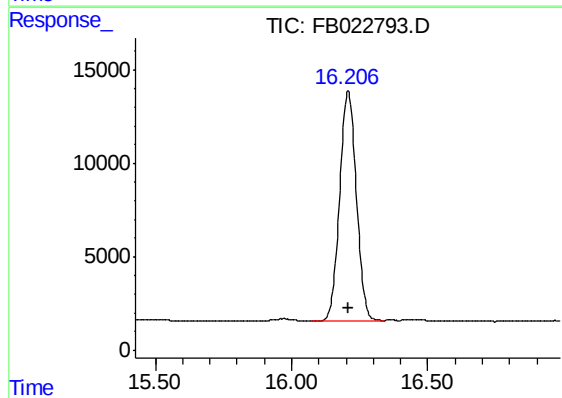

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 522471
Conc: 18.34 ng/ml