

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
Data File : FB025122.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2020 11:03
Operator : DD/AJ
Sample : L4221-11
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 00:36:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	412176	19.307 ng/ml
Target Compounds			
6) t Toluene	10.632	25315826	710.345 ng/ml
7) t Ethylbenzene	13.070	74345	2.284 ng/ml
8) t m-Xylene	13.200	483542	15.077 ng/ml
9) t O-Xylene	13.930	153374	4.975 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
Data File : FB025122.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2020 11:03
Operator : DD/AJ
Sample : L4221-11
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 00:36:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

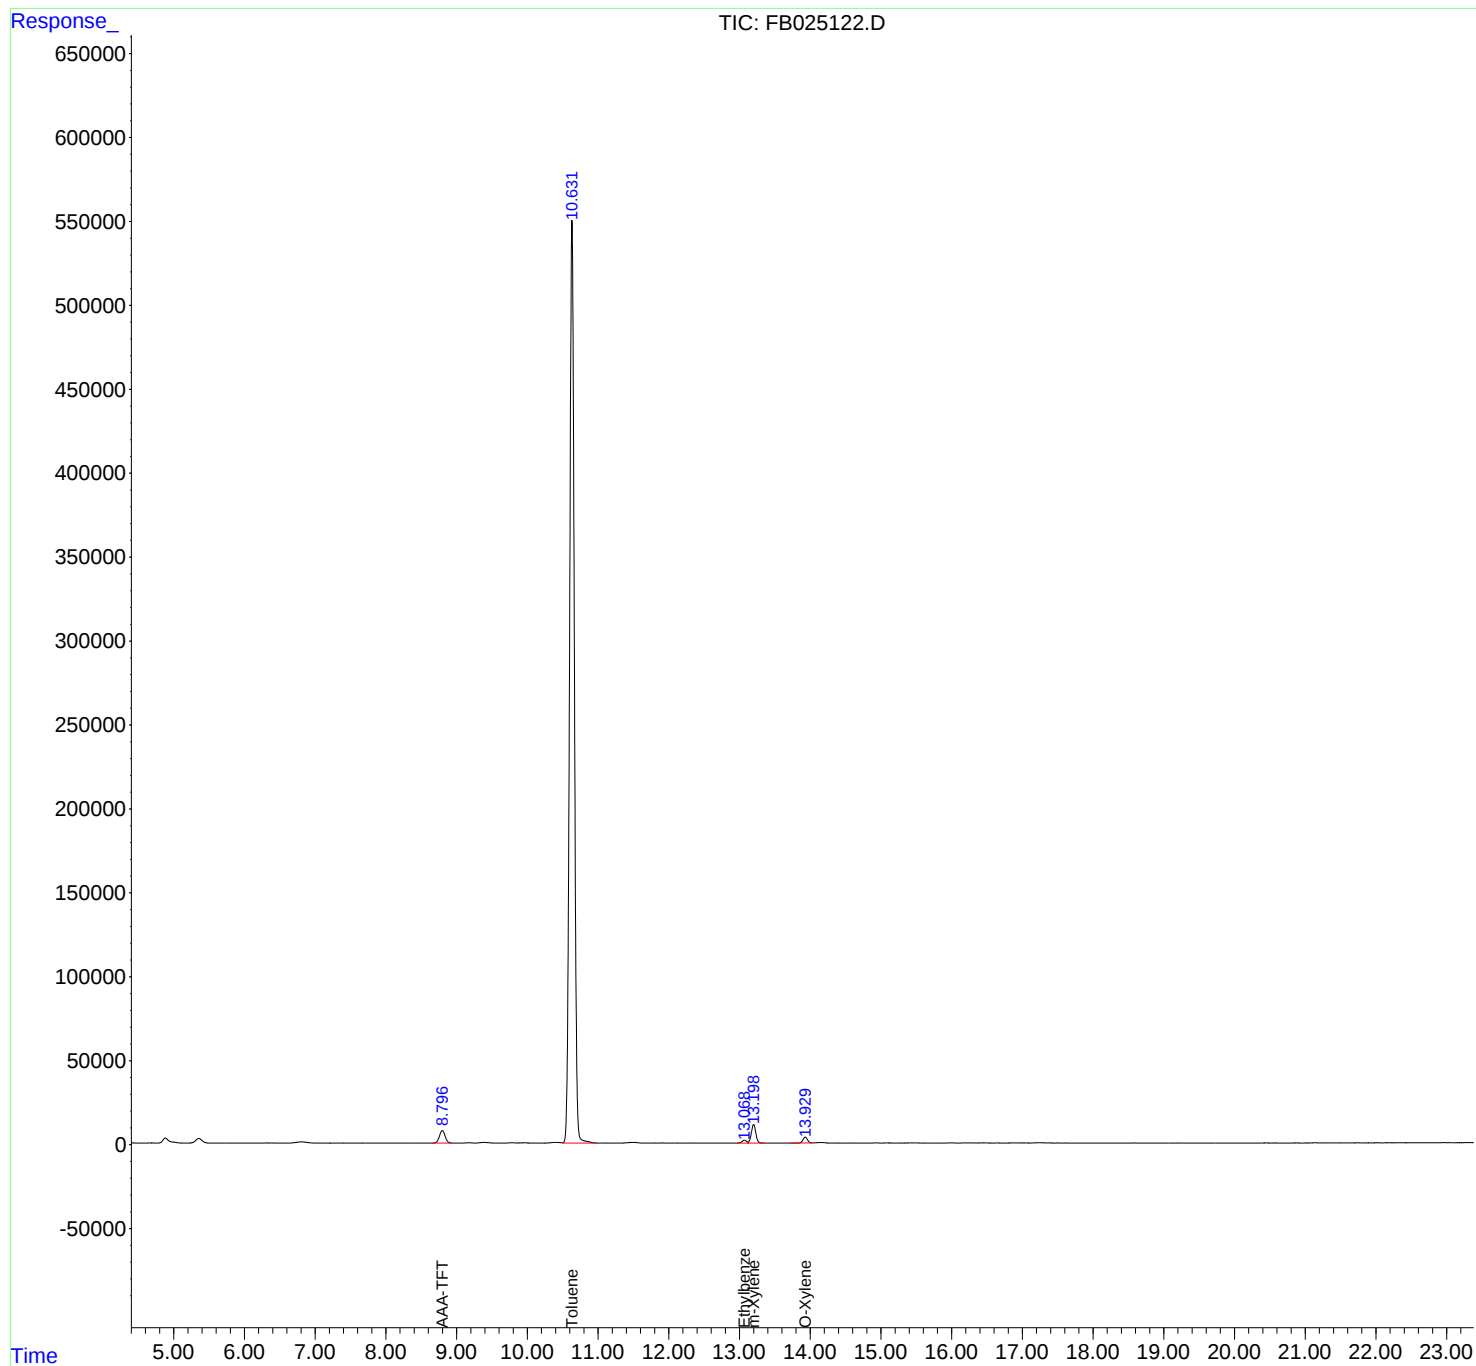

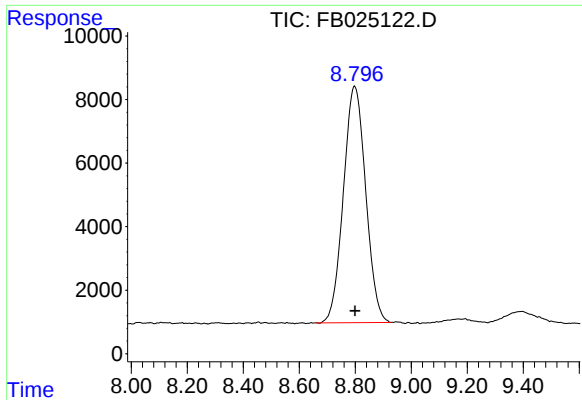


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 412176
Conc: 19.31 ng/ml

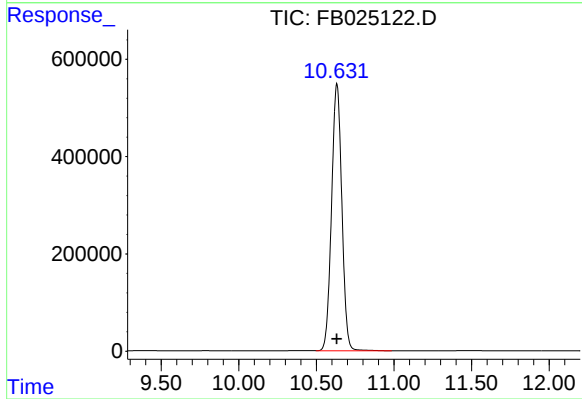


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 25315826
Conc: 710.34 ng/ml

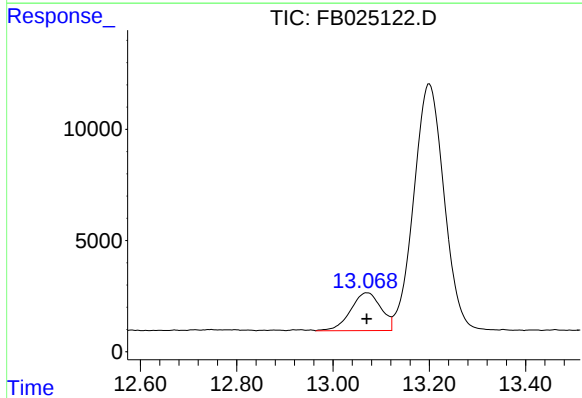


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 74345
Conc: 2.28 ng/ml

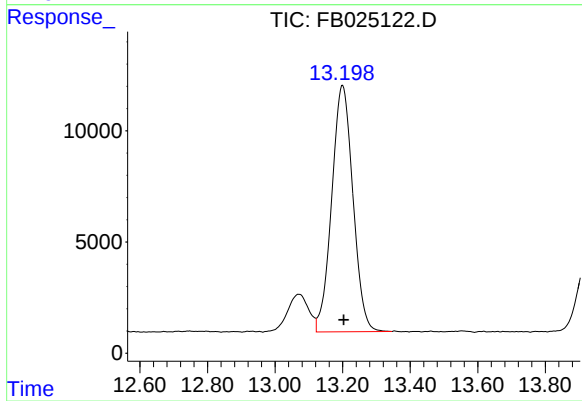

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 483542
Conc: 15.08 ng/ml

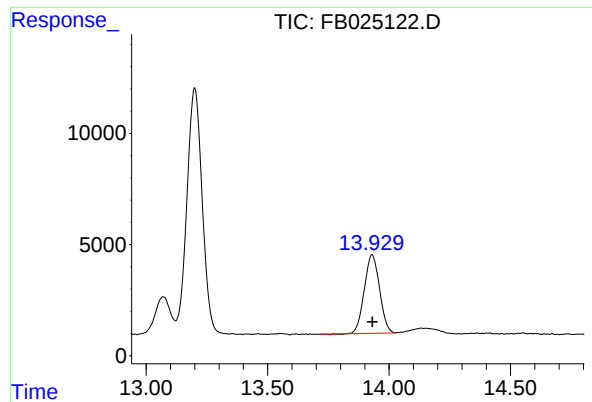

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 153374
Conc: 4.98 ng/ml