

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
 Data File : FB025121.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2020 10:15
 Operator : DD/AJ
 Sample : BSF1021S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 22 00:36:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	393198	18.418 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	884431	29.079 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	934280	29.991 ng/ml
3) t n-Heptane	7.757	305319	9.930 ng/ml
4) t Benzene	7.891	370329	9.854 ng/ml
6) t Toluene	10.630	1036907	29.095 ng/ml
7) t Ethylbenzene	13.069	322697	9.913 ng/ml
8) t m-Xylene	13.202	642412	20.031 ng/ml
9) t O-Xylene	13.929	622266	20.186 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	517901	19.836 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
Data File : FB025121.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2020 10:15
Operator : DD/AJ
Sample : BSF1021S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 00:36:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

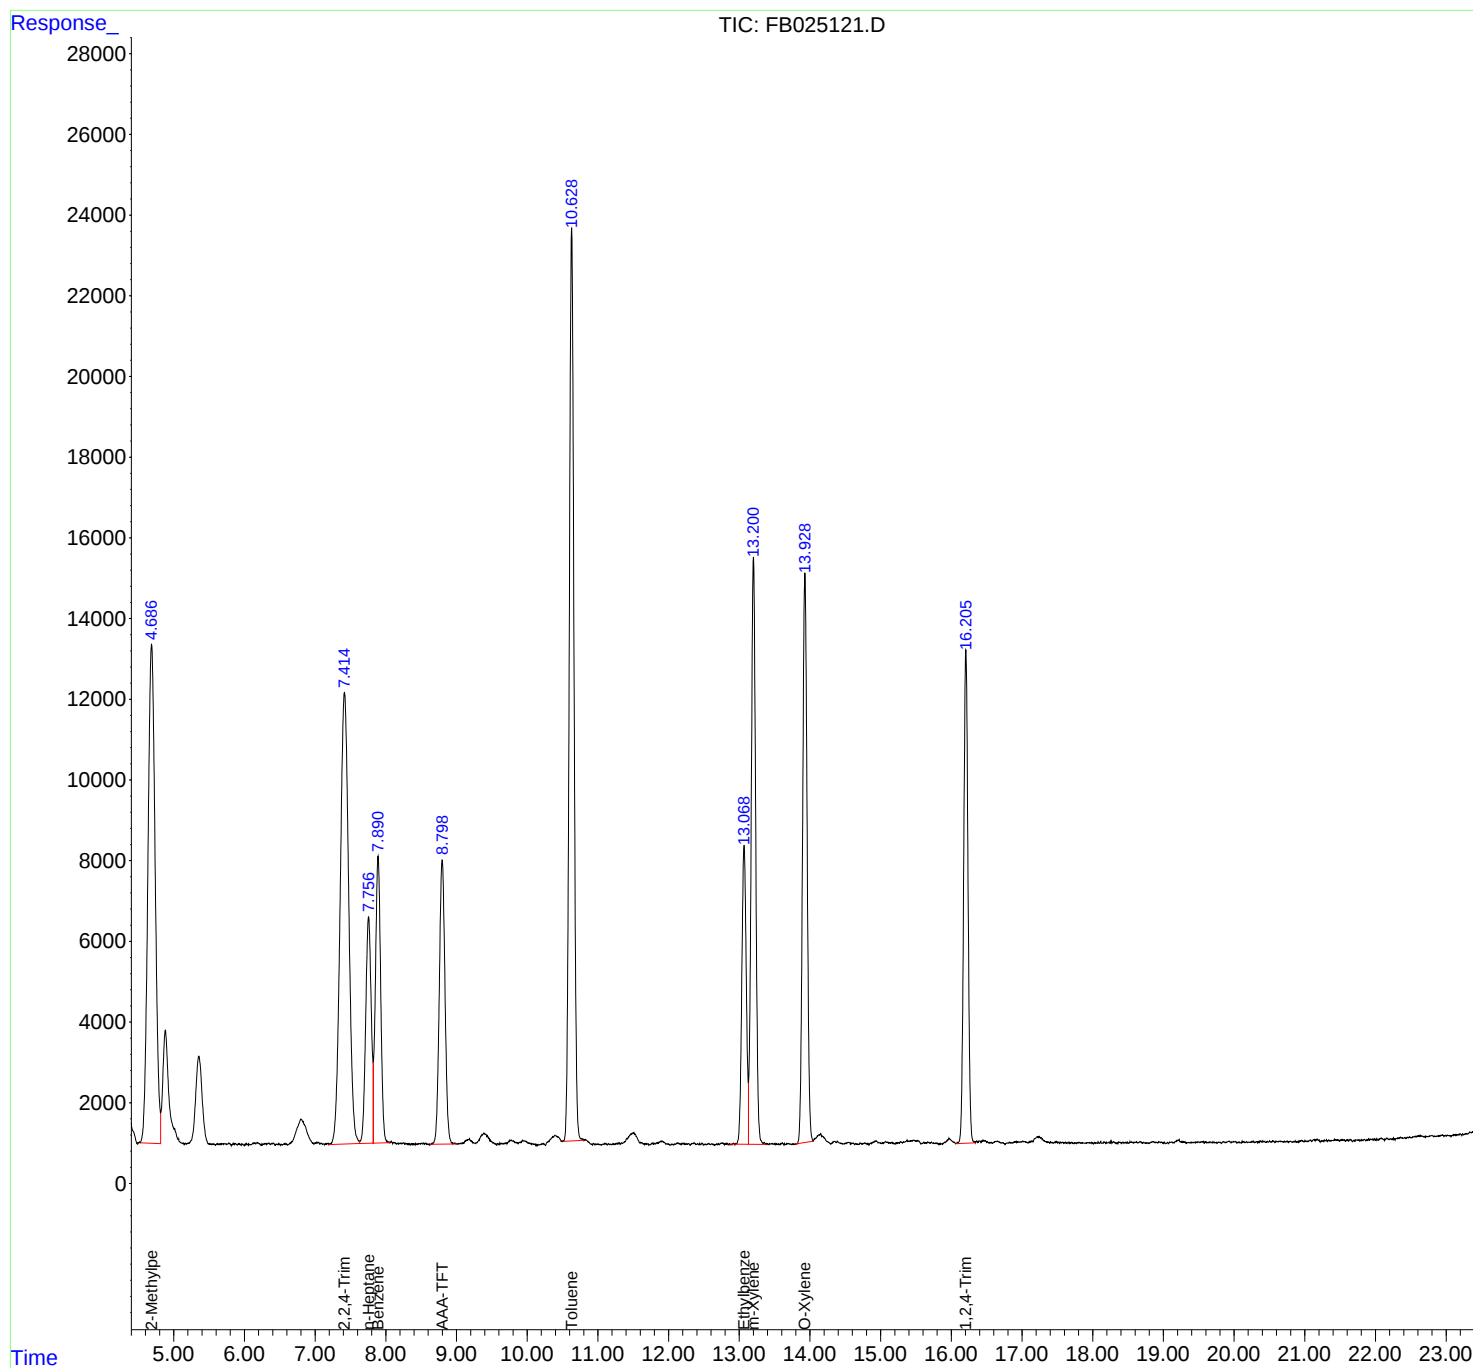

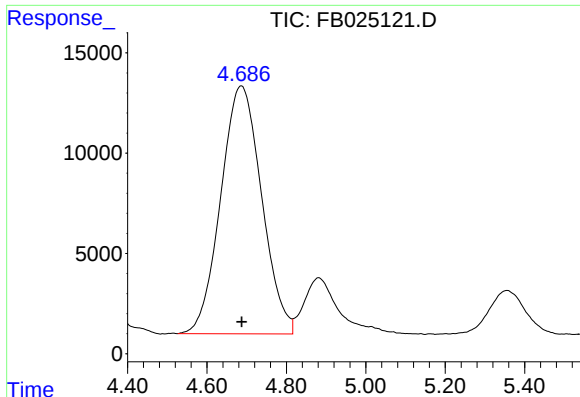


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 884431
Conc: 29.08 ng/ml

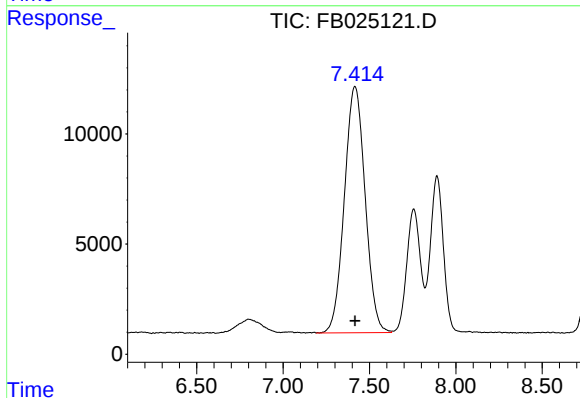


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 934280
Conc: 29.99 ng/ml

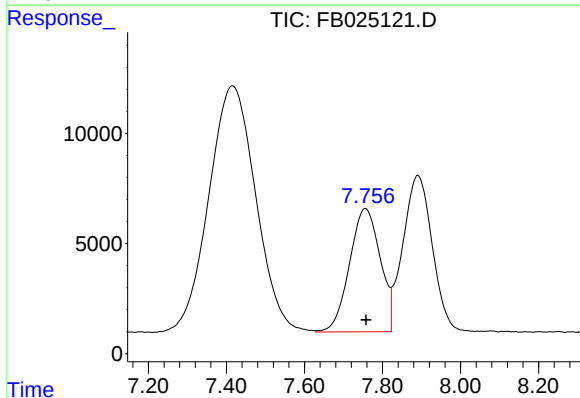


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 305319
Conc: 9.93 ng/ml

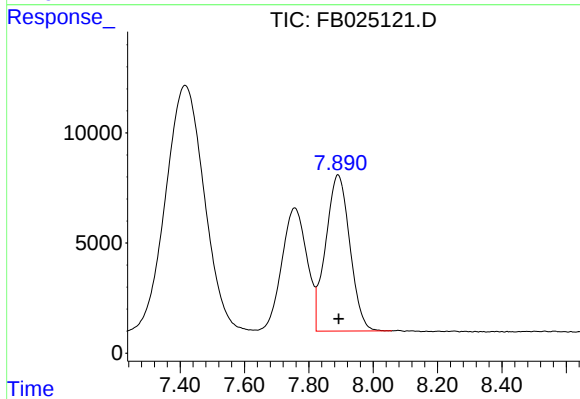


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 370329
Conc: 9.85 ng/ml

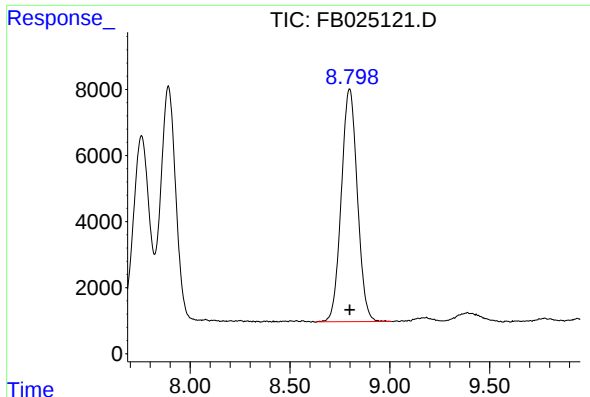


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 393198
Conc: 18.42 ng/ml

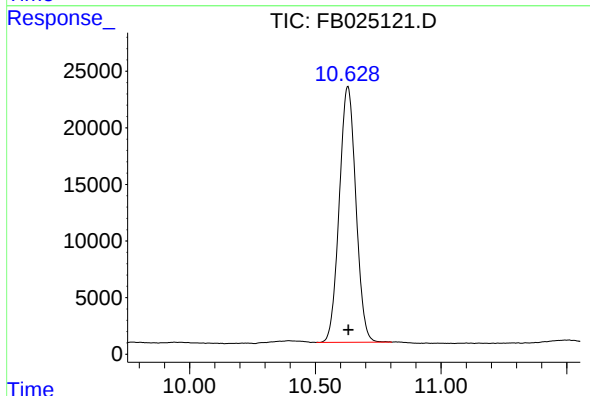


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 1036907
Conc: 29.09 ng/ml

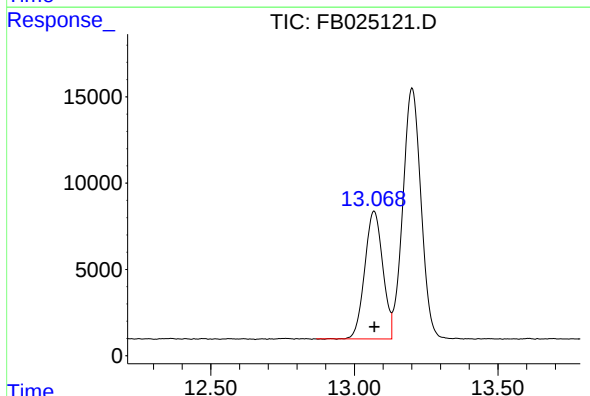


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 322697
Conc: 9.91 ng/ml

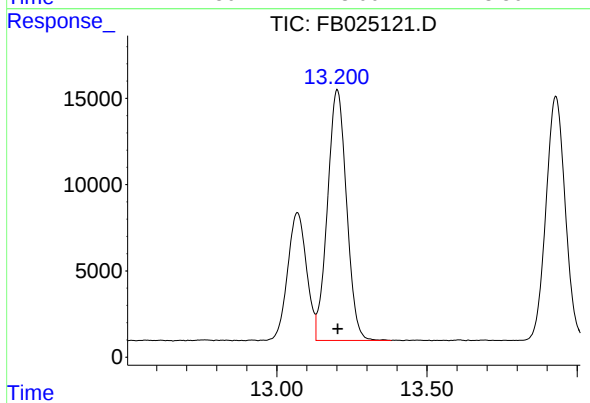


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 642412
Conc: 20.03 ng/ml

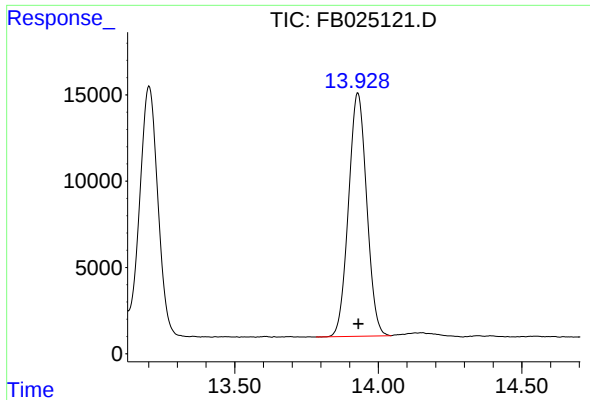

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 622266
Conc: 20.19 ng/ml

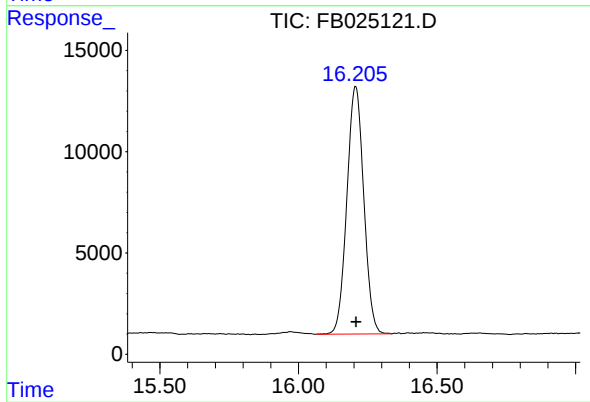

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.002 min
Response: 517901
Conc: 19.84 ng/ml