

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
 Data File : FB025123.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2020 11:34
 Operator : DD/AJ
 Sample : L4221-11MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 22 00:36:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	379355	17.770 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	747930	24.591 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	740838	23.781 ng/ml
3) t n-Heptane	7.758	243071	7.906 ng/ml
4) t Benzene	7.893	334278	8.894 ng/ml
6) t Toluene	10.632	14241461	399.606 ng/ml
7) t Ethylbenzene	13.071	321619	9.880 ng/ml
8) t m-Xylene	13.202	829409	25.862 ng/ml
9) t O-Xylene	13.931	632022	20.502 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	455899	17.462 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
Data File : FB025123.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2020 11:34
Operator : DD/AJ
Sample : L4221-11MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 00:36:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

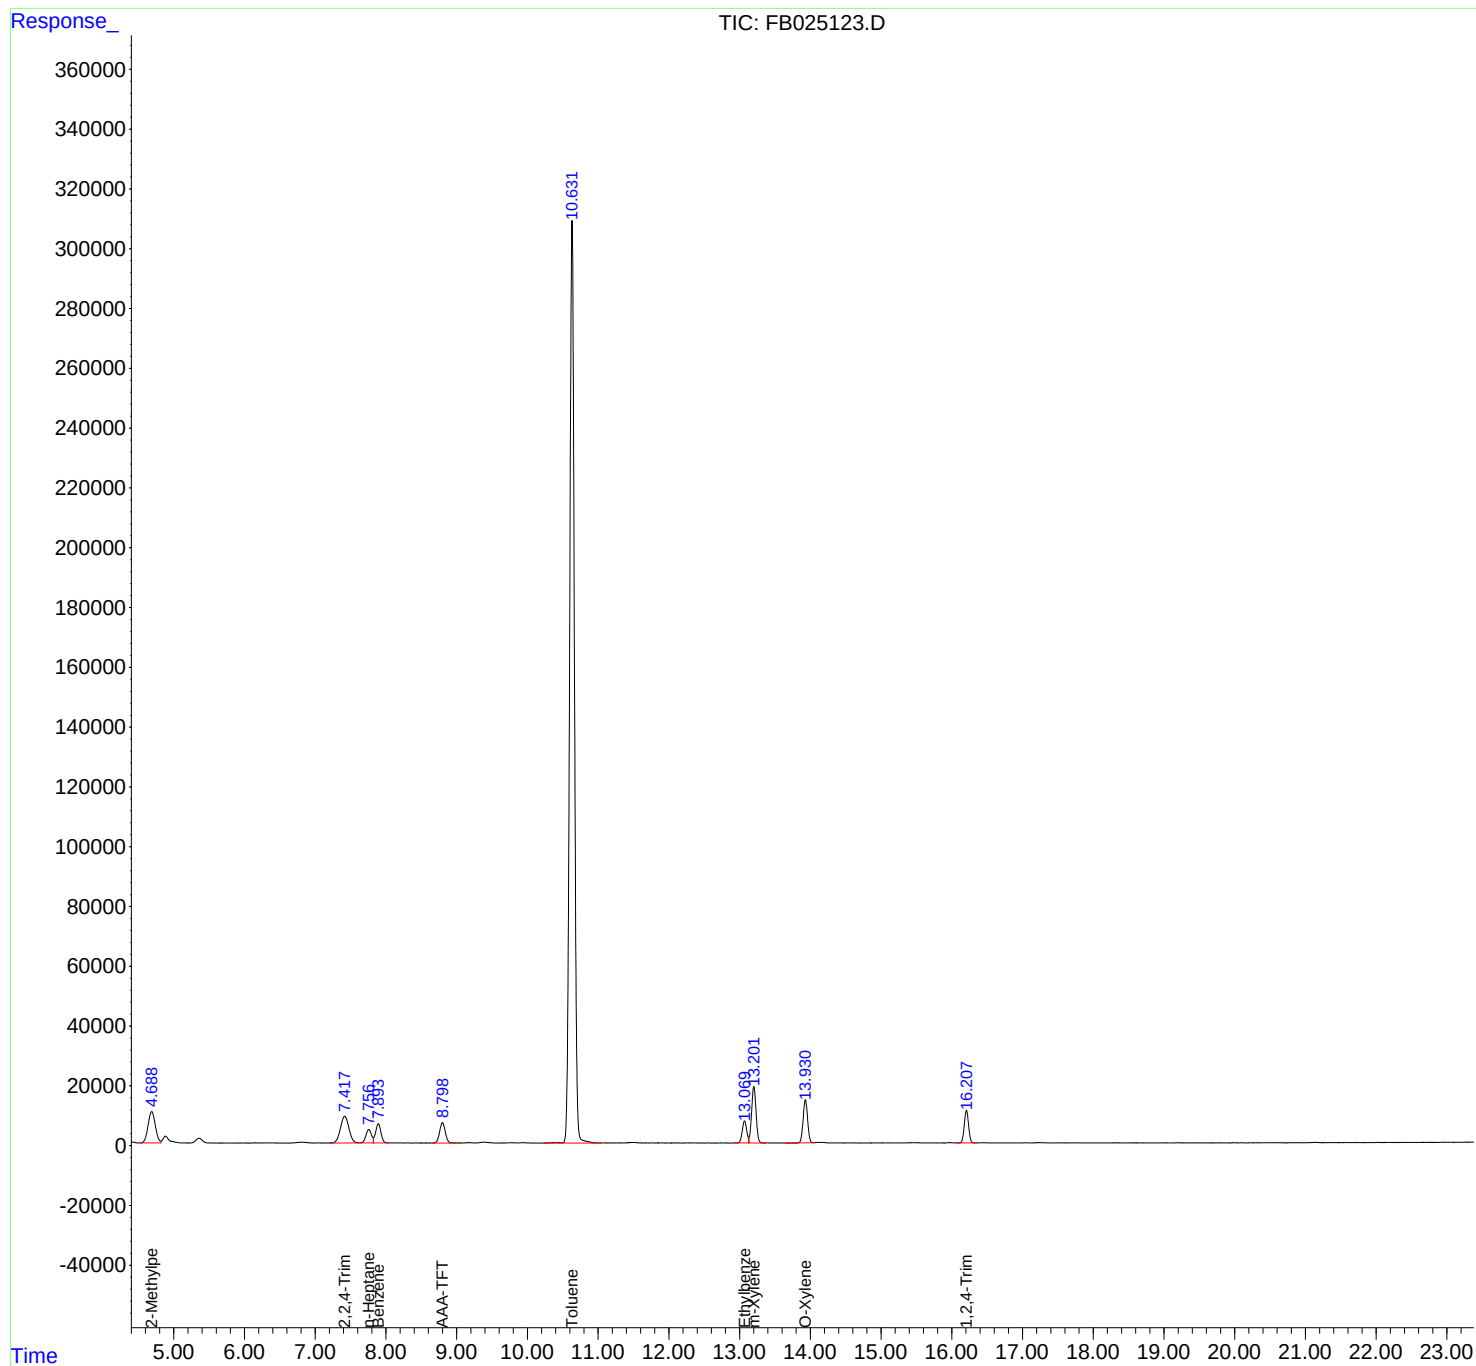

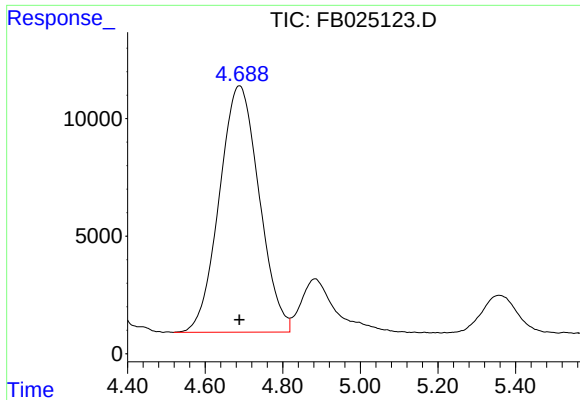


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.001 min
Response: 747930
Conc: 24.59 ng/ml

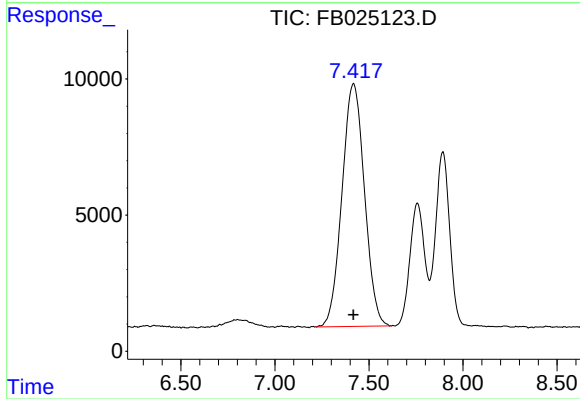


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 740838
Conc: 23.78 ng/ml

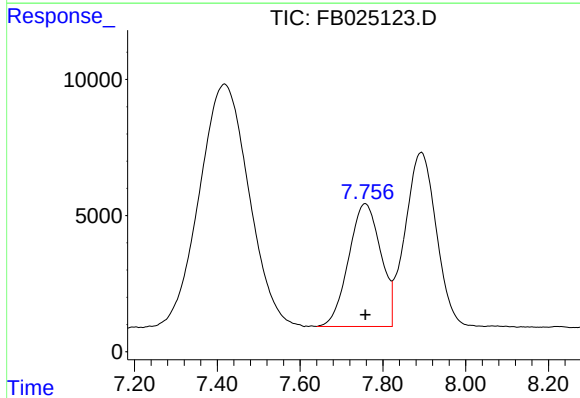


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 243071
Conc: 7.91 ng/ml

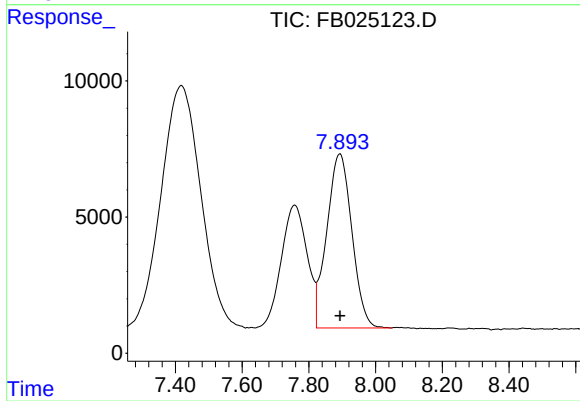


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 334278
Conc: 8.89 ng/ml

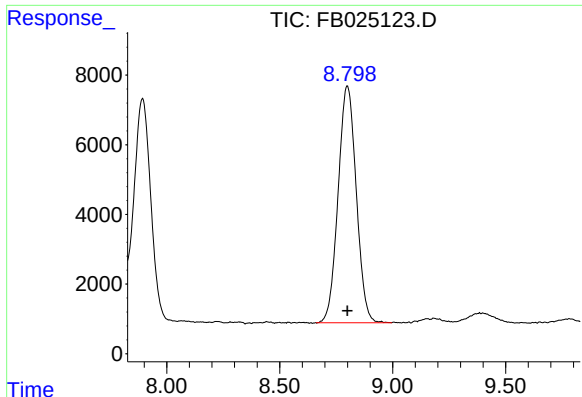


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 379355
Conc: 17.77 ng/ml

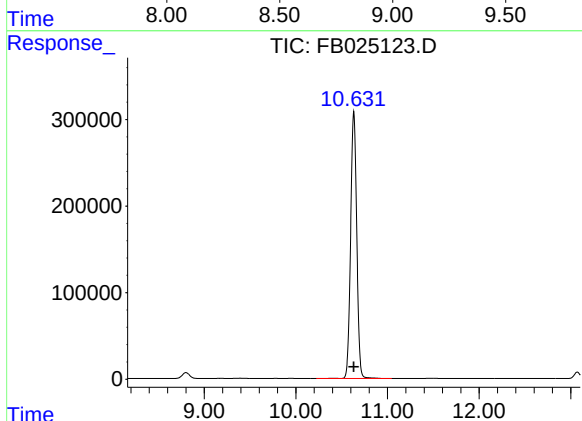


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 14241461
Conc: 399.61 ng/ml

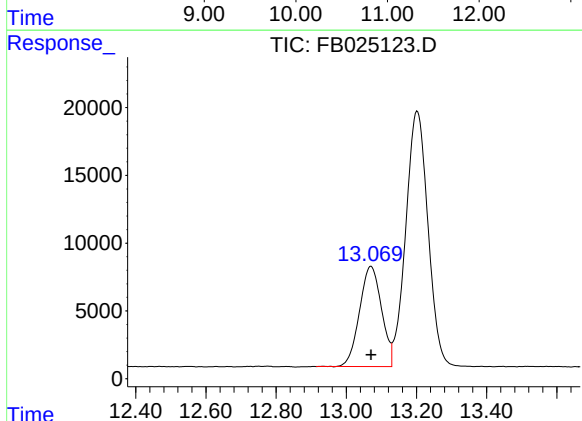


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 321619
Conc: 9.88 ng/ml

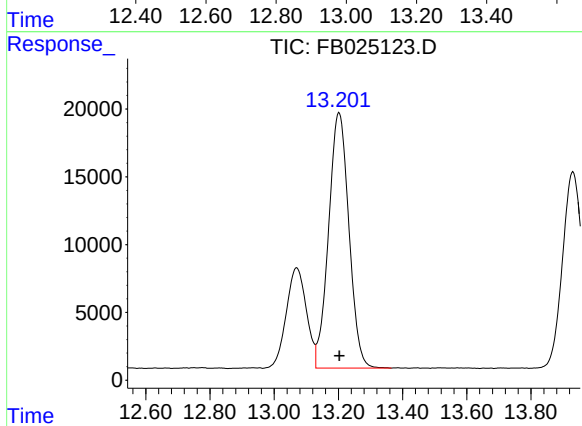


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 829409
Conc: 25.86 ng/ml

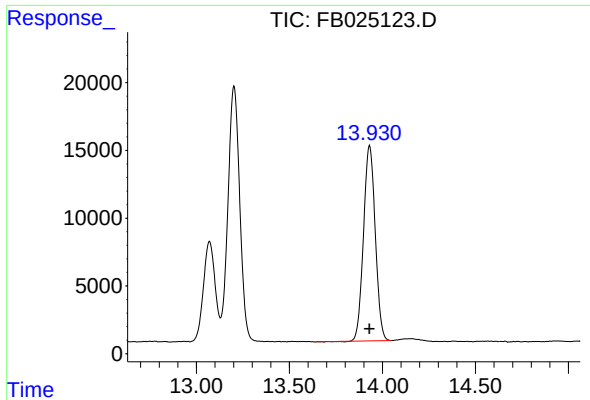

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 632022
Conc: 20.50 ng/ml

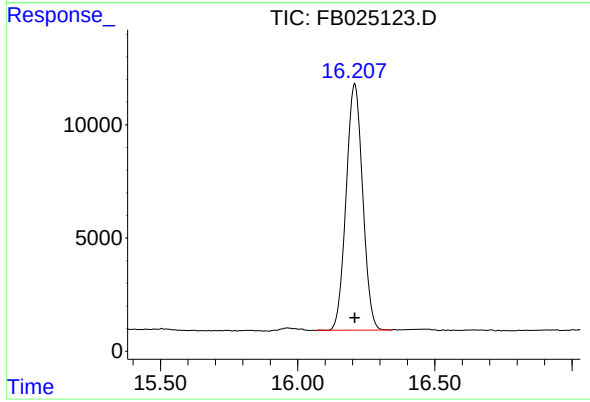

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 455899
Conc: 17.46 ng/ml