

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
 Data File : FB025124.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2020 12:05
 Operator : DD/AJ
 Sample : L4221-11MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 22 00:37:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	374384	17.537 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	731265	24.043 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	710423	22.805 ng/ml
3) t n-Heptane	7.758	236451	7.691 ng/ml
4) t Benzene	7.893	339691	9.038 ng/ml
6) t Toluene	10.632	17393369	488.046 ng/ml
7) t Ethylbenzene	13.070	330659	10.158 ng/ml
8) t m-Xylene	13.203	830761	25.904 ng/ml
9) t O-Xylene	13.931	649392	21.066 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	455937	17.463 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102120\
Data File : FB025124.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2020 12:05
Operator : DD/AJ
Sample : L4221-11MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 22 00:37:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

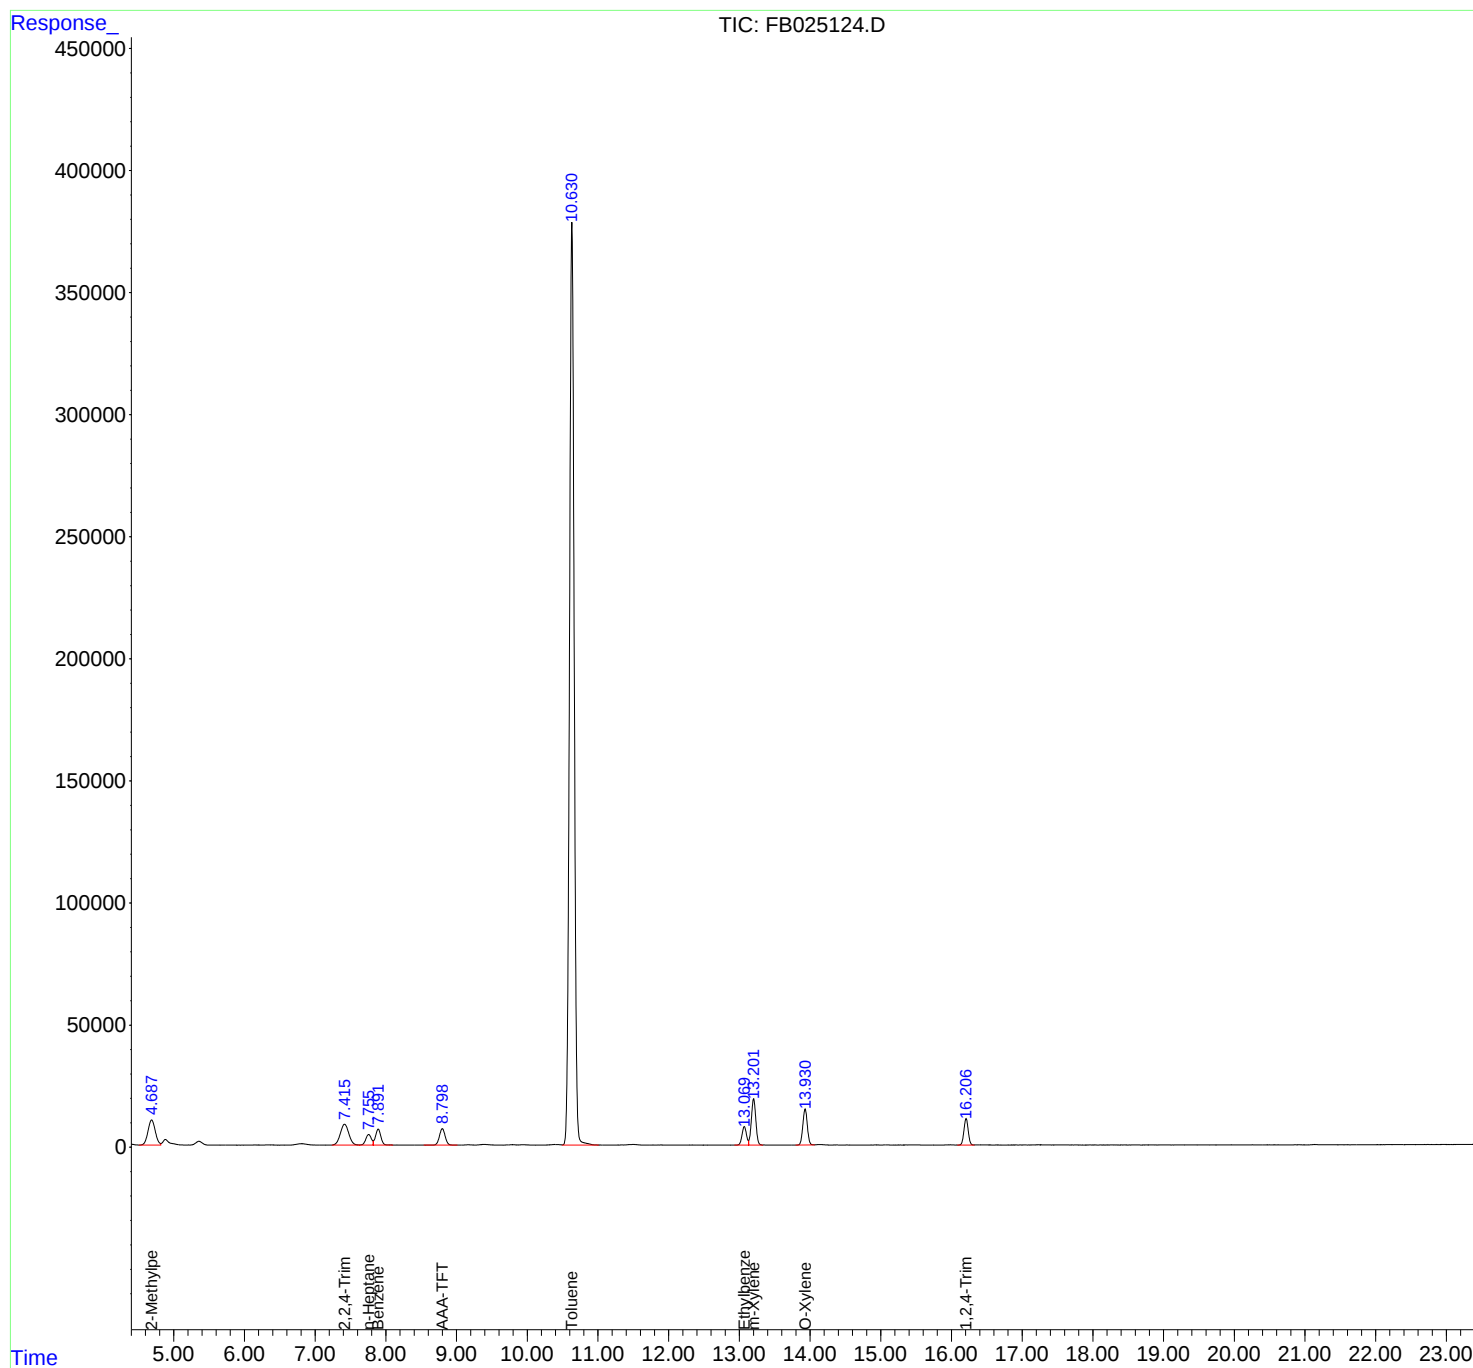

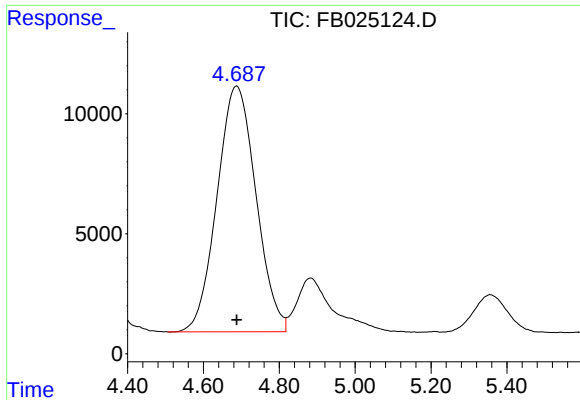


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 731265
Conc: 24.04 ng/ml

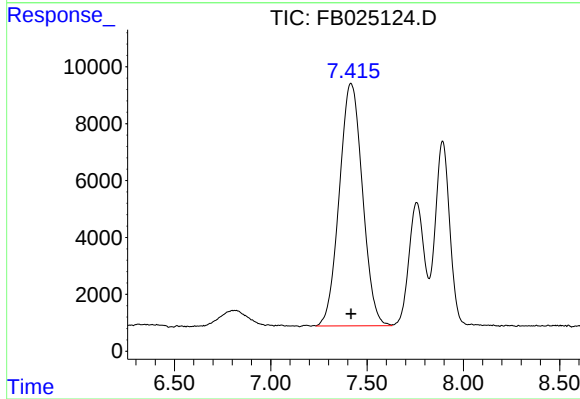


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 710423
Conc: 22.81 ng/ml

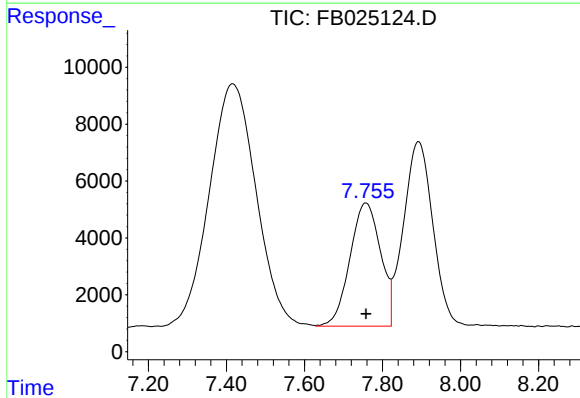


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 236451
Conc: 7.69 ng/ml

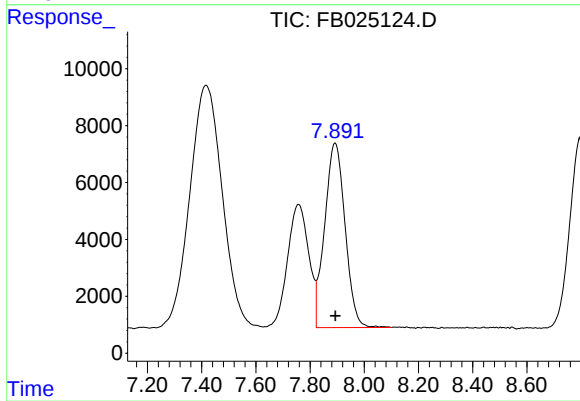


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 339691
Conc: 9.04 ng/ml

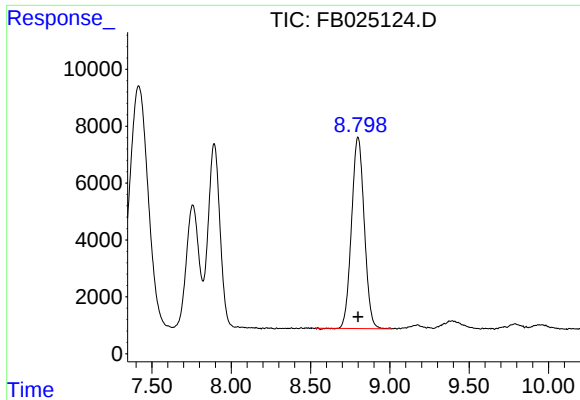


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 374384
Conc: 17.54 ng/ml

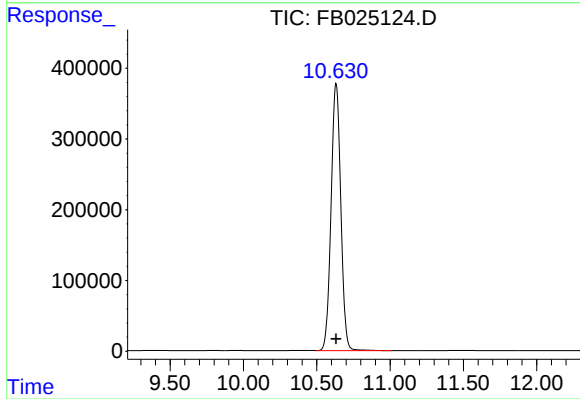


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 17393369
Conc: 488.05 ng/ml

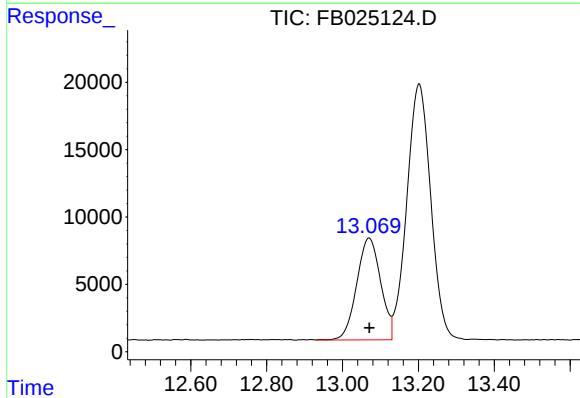


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 330659
Conc: 10.16 ng/ml

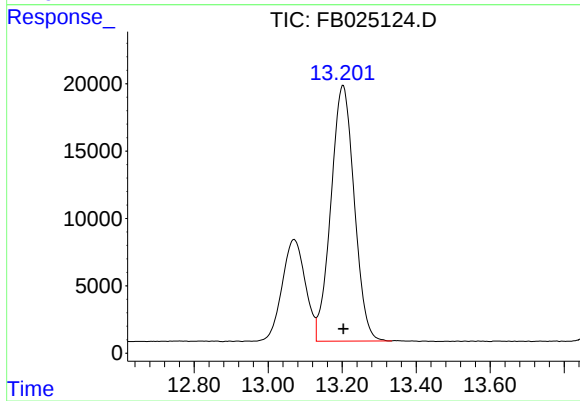


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 830761
Conc: 25.90 ng/ml

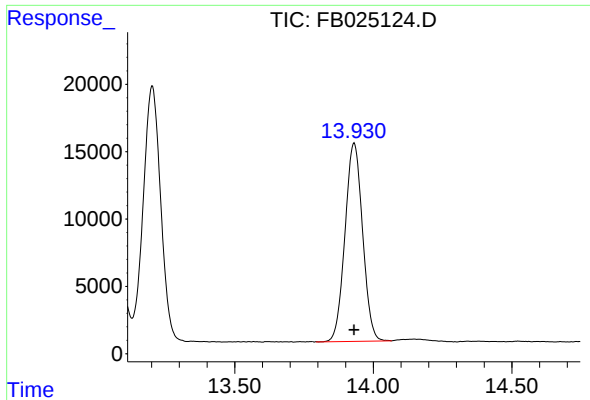

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 649392
Conc: 21.07 ng/ml

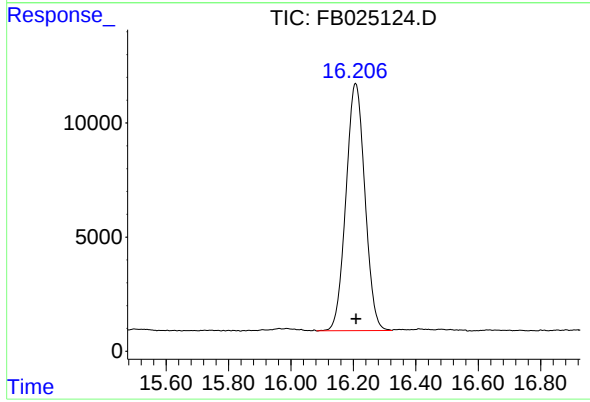

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 455937
Conc: 17.46 ng/ml