

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
 Data File : FB028670.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2022 13:02
 Operator : AJ/MA
 Sample : N5193-10
 Misc : 5.49G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 21 17:18:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.855	28256	2.184 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	7216	0.441 ng/ml
2) t 2,2,4-Trimethylpentane	7.400	1819	0.101 ng/ml
3) t n-Heptane	7.759	1386	0.082 ng/ml
4) t Benzene	7.886	21231	0.967 ng/ml
6) t Toluene	10.630	13654	0.651 ng/ml
7) t Ethylbenzene	13.022	23734	1.196 ng/ml
8) t m-Xylene	13.188	6077	0.308 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
Data File : FB028670.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2022 13:02
Operator : AJ/MA
Sample : N5193-10
Misc : 5.49G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 21 17:18:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

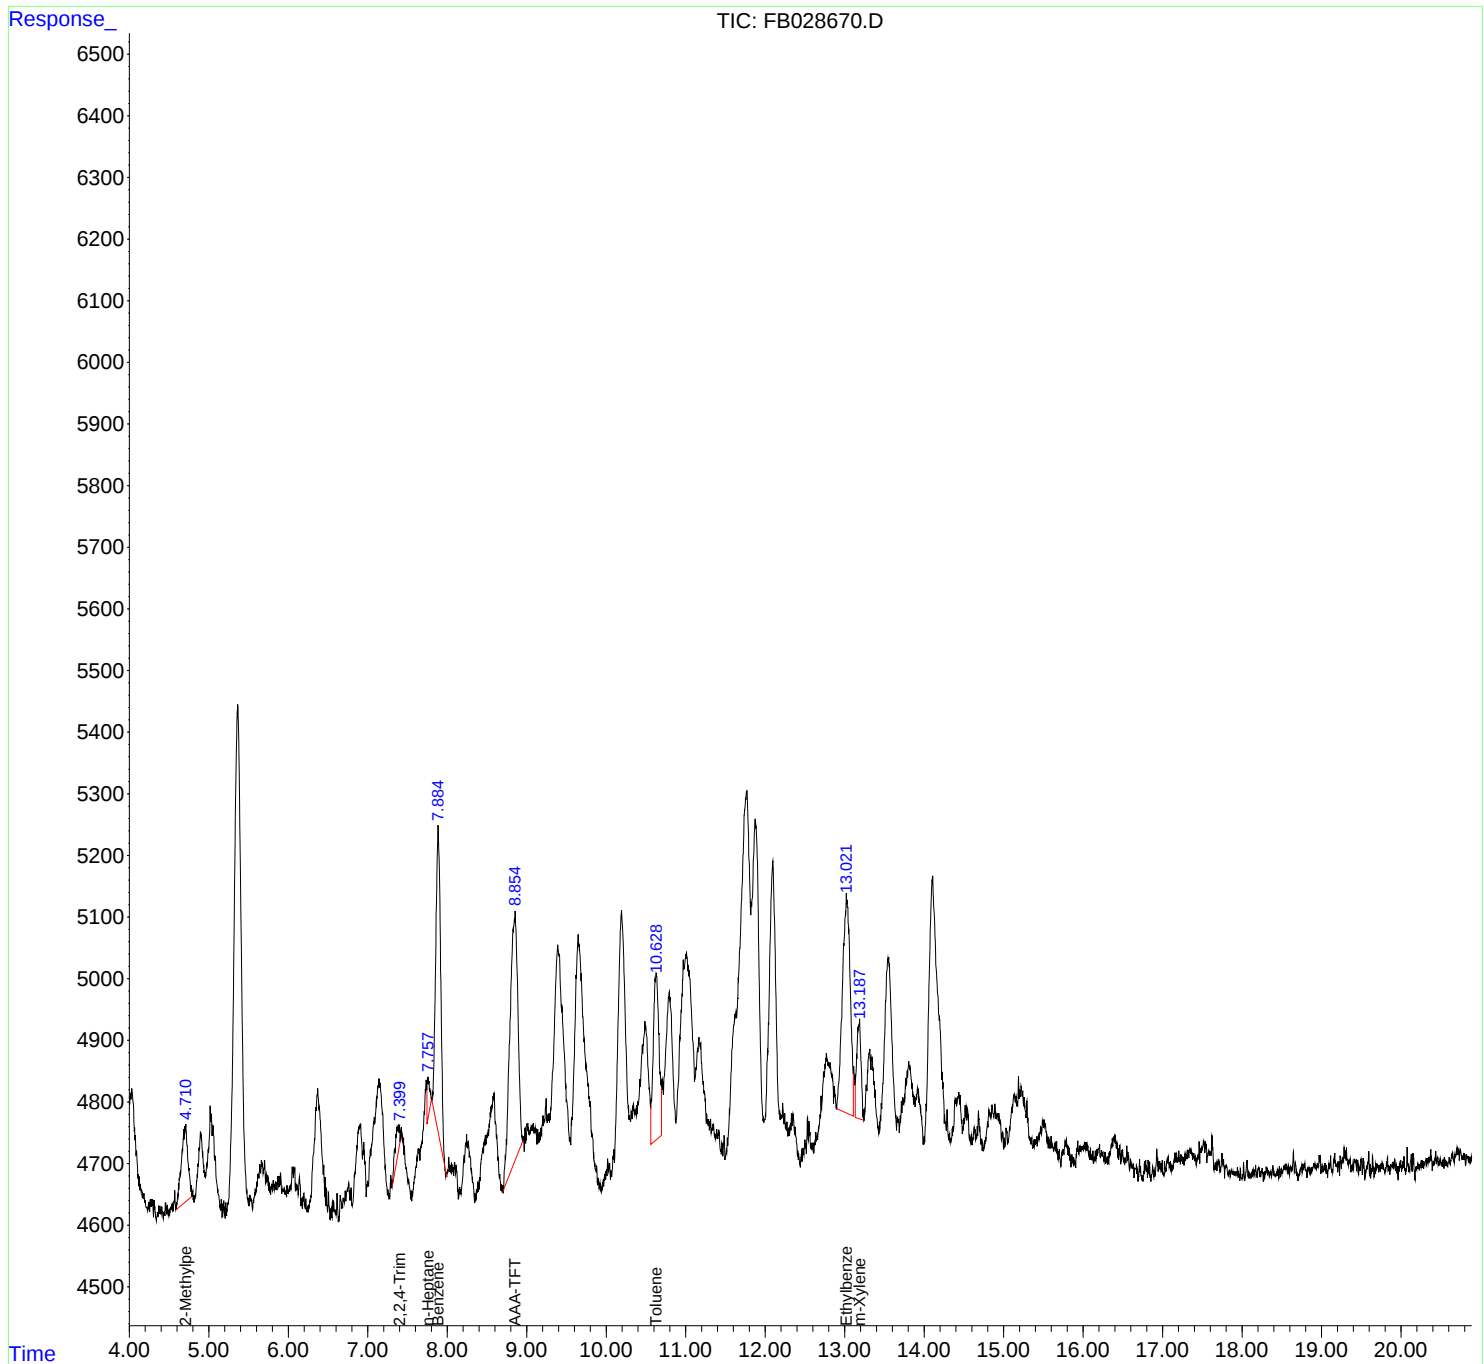


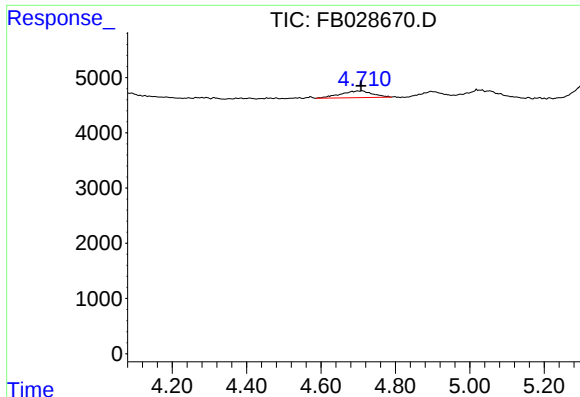

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 7216
Conc: 0.44 ng/ml

Instrument :
FID_B
ClientSampleId :

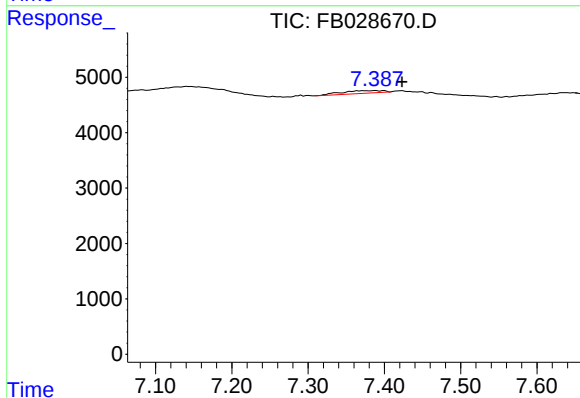


#2 2,2,4-Trimethylpentane

R.T.: 7.400 min
Delta R.T.: -0.023 min
Response: 1819
Conc: 0.10 ng/ml

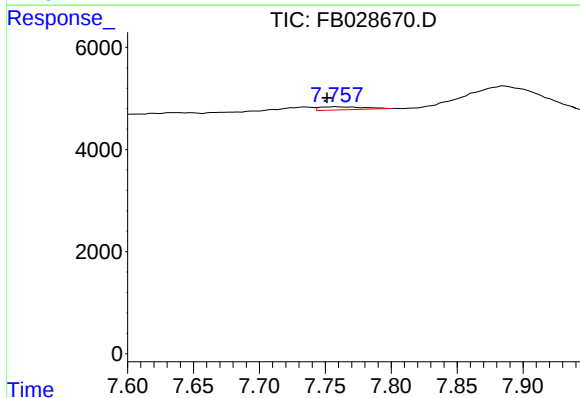


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.007 min
Response: 1386
Conc: 0.08 ng/ml

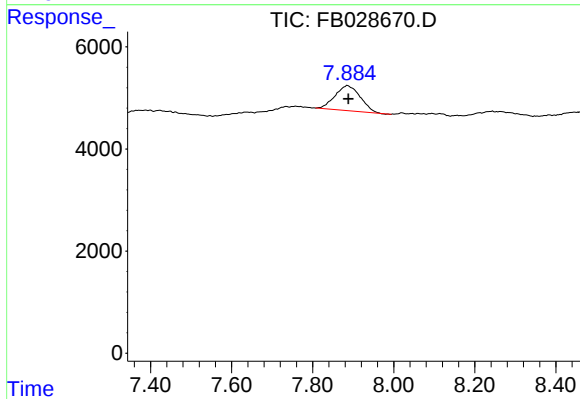

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 21231
Conc: 0.97 ng/ml

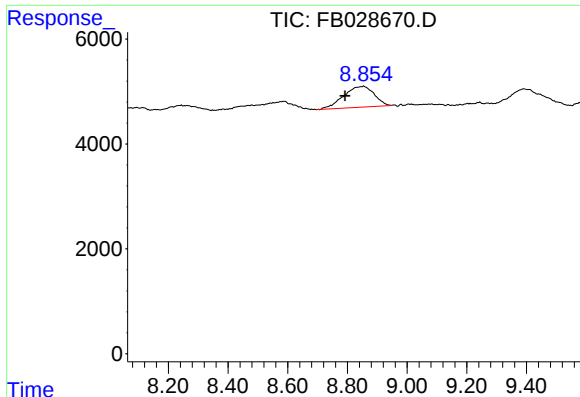

#5 AAA-TFT


R.T.: 8.855 min
Delta R.T.: 0.063 min
Response: 28256
Conc: 2.18 ng/ml

Instrument :
FID_B
ClientSampleId :

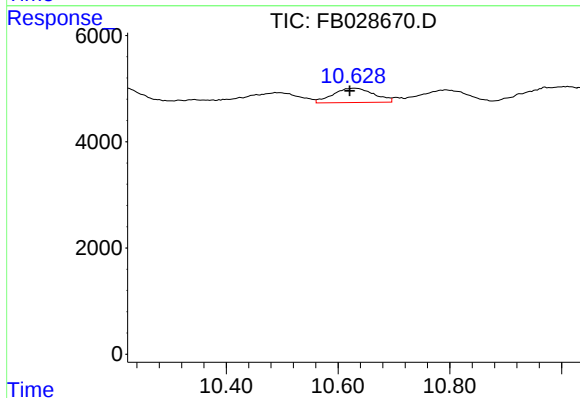


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.009 min
Response: 13654
Conc: 0.65 ng/ml

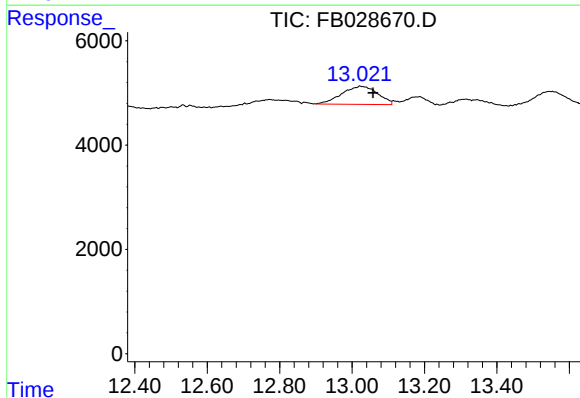

#7 Ethylbenzene

R.T.: 13.022 min
Delta R.T.: -0.036 min
Response: 23734
Conc: 1.20 ng/ml

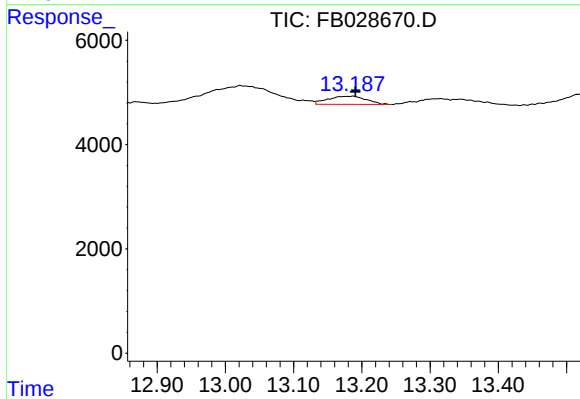

#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.002 min
Response: 6077
Conc: 0.31 ng/ml