

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
Data File : FB028672.D  
Signal(s) : FID2B.CH  
Acq On : 21 Oct 2022 14:21  
Operator : AJ/MA  
Sample : N5193-12  
Misc : 5.49G/5.00 ML DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 21 17:19:02 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units  |
|------------------------------|--------|----------|-------------|
| -----                        |        |          |             |
| System Monitoring Compounds  |        |          |             |
| 5) s AAA-TFT                 | 8.796  | 49558    | 3.831 ng/ml |
| Target Compounds             |        |          |             |
| 3) t n-Heptane               | 7.765  | 6351     | 0.375 ng/ml |
| 7) t Ethylbenzene            | 13.025 | 6664     | 0.336 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.208 | 1453     | 0.075 ng/ml |
| -----                        |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
Data File : FB028672.D  
Signal(s) : FID2B.CH  
Acq On : 21 Oct 2022 14:21  
Operator : AJ/MA  
Sample : N5193-12  
Misc : 5.49G/5.00 ML DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 21 17:19:02 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

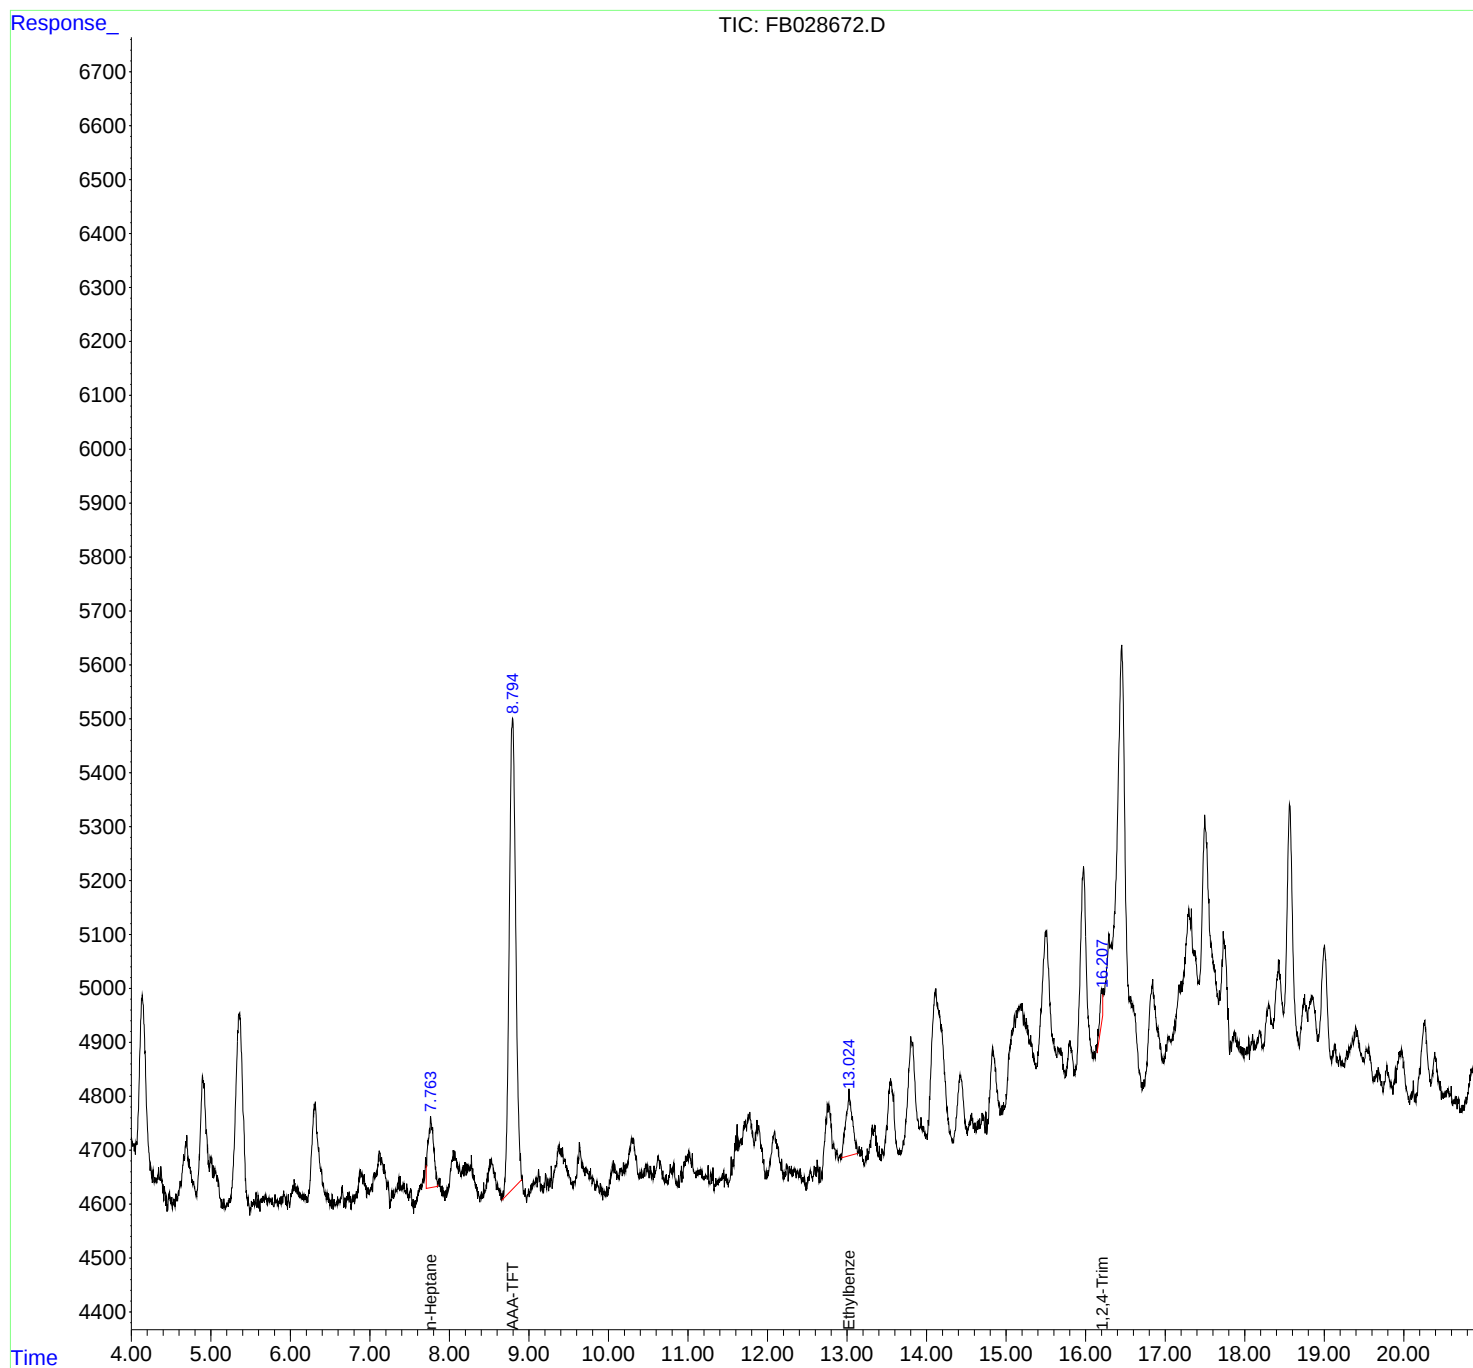


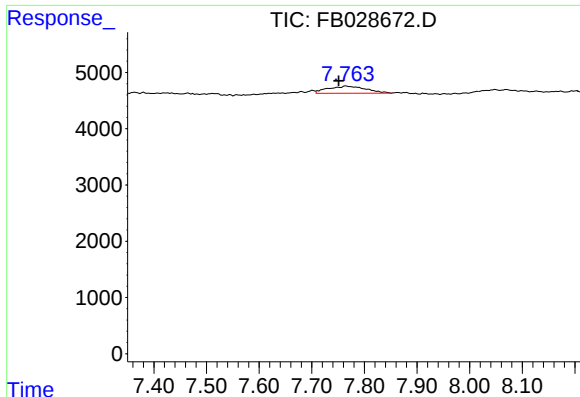

#3 n-Heptane


R.T.: 7.765 min  
Delta R.T.: 0.014 min  
Response: 6351  
Conc: 0.37 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

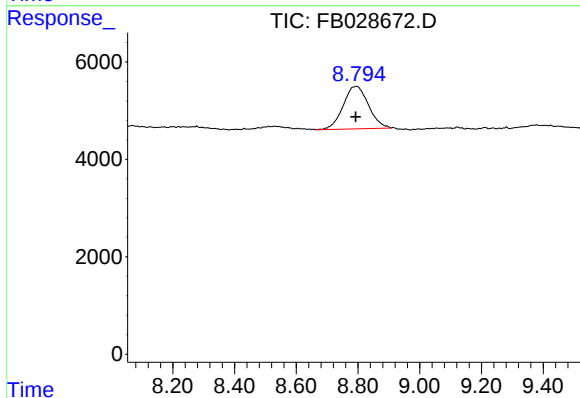


#5 AAA-TFT

R.T.: 8.796 min  
Delta R.T.: 0.003 min  
Response: 49558  
Conc: 3.83 ng/ml

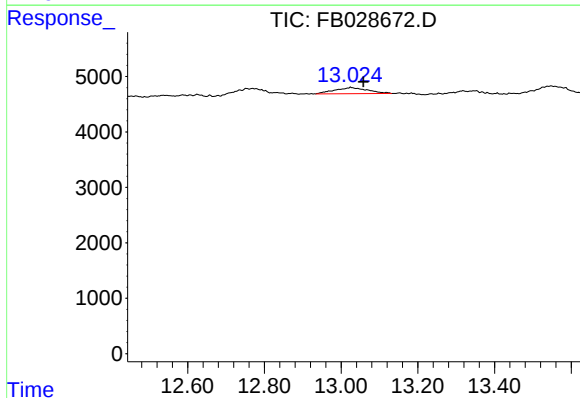

#7 Ethylbenzene

R.T.: 13.025 min  
Delta R.T.: -0.033 min  
Response: 6664  
Conc: 0.34 ng/ml

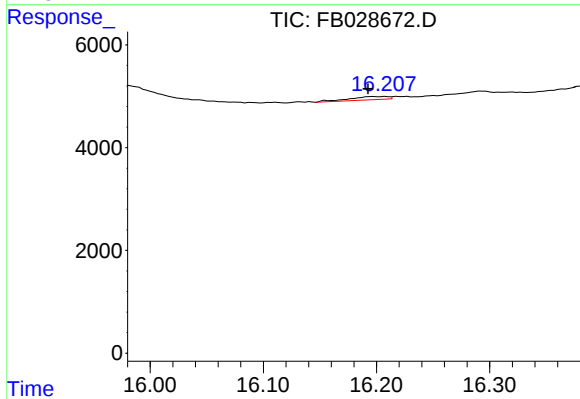

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min  
Delta R.T.: 0.015 min  
Response: 1453  
Conc: 0.08 ng/ml