

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
 Data File : FB028688.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2022 1:32
 Operator : AJ/MA
 Sample : N5193-12
 Misc : 5.79G/5.00 ML DI WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 22 16:41:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	149169	11.530 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	23166	1.416 ng/ml
2) t 2,2,4-Trimethylpentane	7.387	1613	0.089 ng/ml
3) t n-Heptane	7.755	42010	2.480 ng/ml
6) t Toluene	10.633	13238	0.632 ng/ml
7) t Ethylbenzene	13.027	76778	3.869 ng/ml
9) t O-Xylene	13.945	16244	0.835 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	7123	0.368 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
Data File : FB028688.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2022 1:32
Operator : AJ/MA
Sample : N5193-12
Misc : 5.79G/5.00 ML DI WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 22 16:41:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

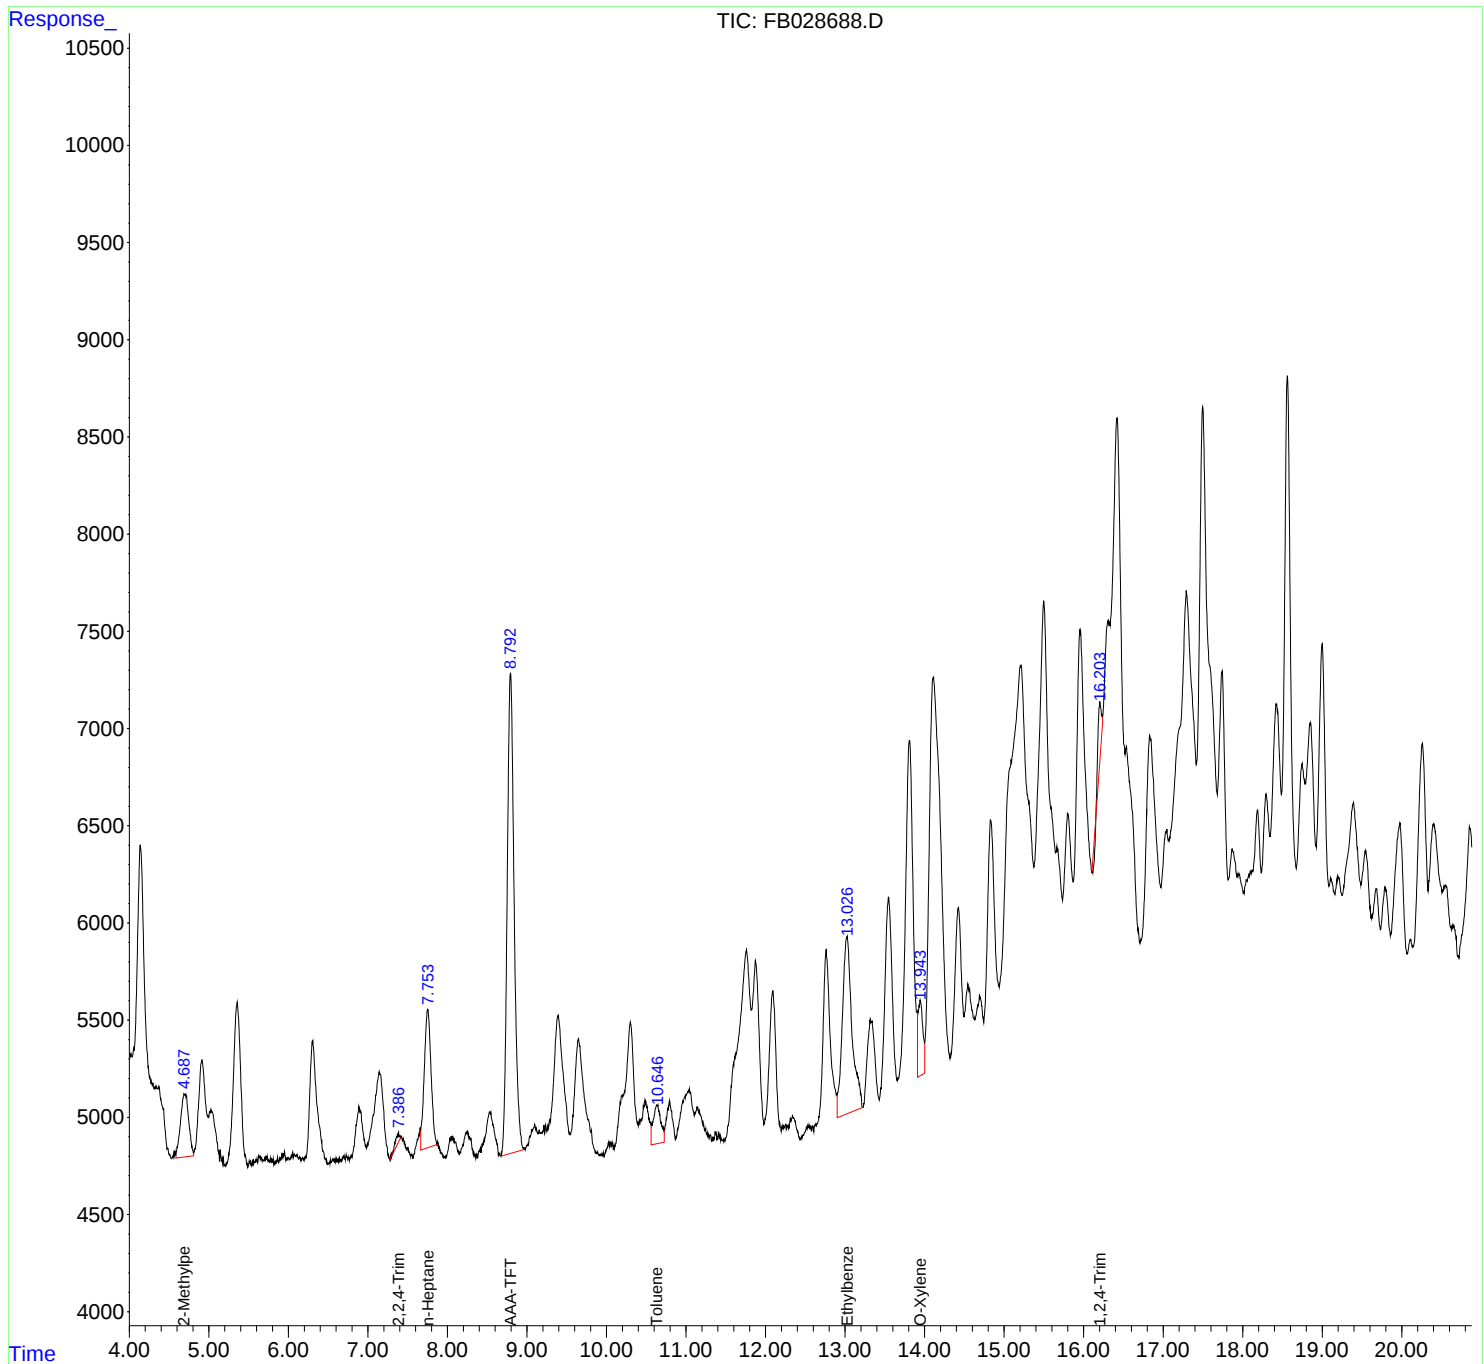


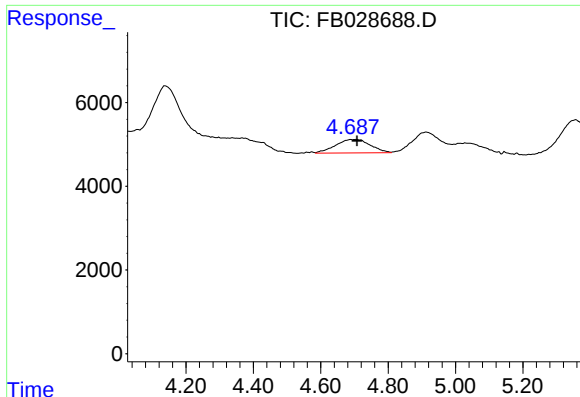

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.019 min
Response: 23166
Conc: 1.42 ng/ml

Instrument :
FID_B
ClientSampleId :

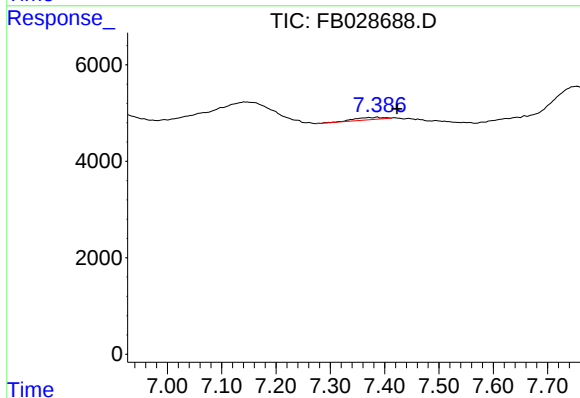


#2 2,2,4-Trimethylpentane

R.T.: 7.387 min
Delta R.T.: -0.036 min
Response: 1613
Conc: 0.09 ng/ml

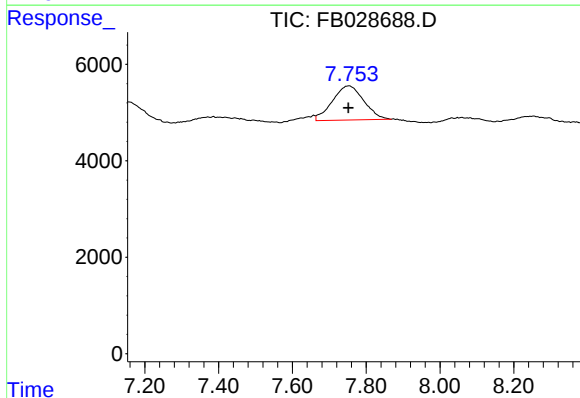


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 42010
Conc: 2.48 ng/ml

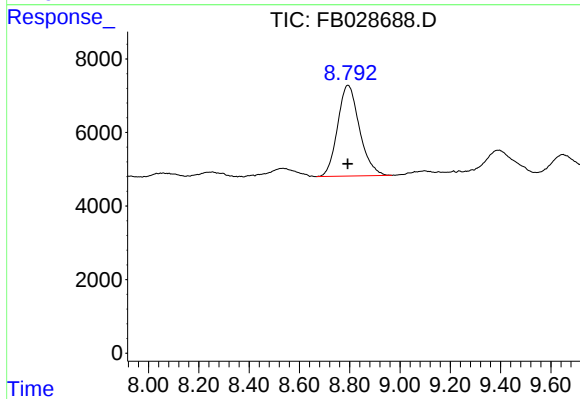

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 149169
Conc: 11.53 ng/ml

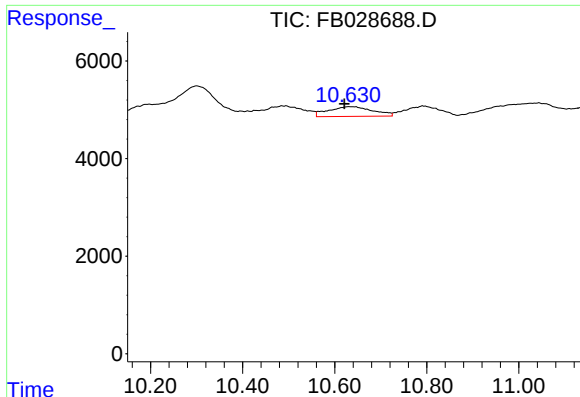

#6 Toluene


R.T.: 10.633 min
Delta R.T.: 0.012 min
Response: 13238
Conc: 0.63 ng/ml

Instrument :
FID_B
ClientSampleId :

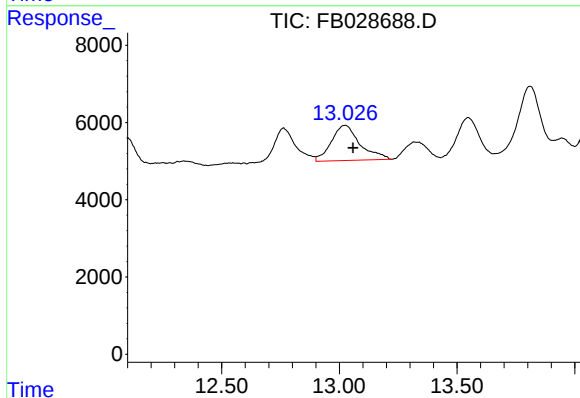


#7 Ethylbenzene

R.T.: 13.027 min
Delta R.T.: -0.031 min
Response: 76778
Conc: 3.87 ng/ml

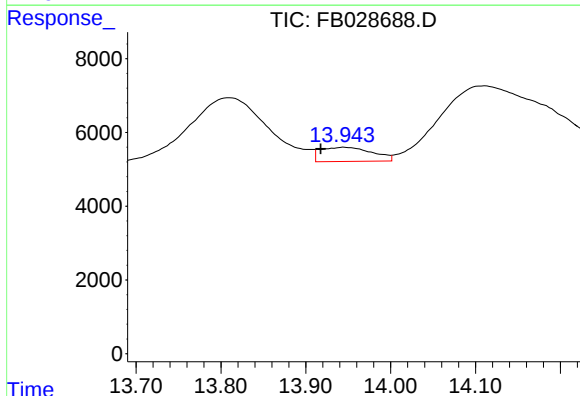

#9 O-Xylene

R.T.: 13.945 min
Delta R.T.: 0.028 min
Response: 16244
Conc: 0.83 ng/ml

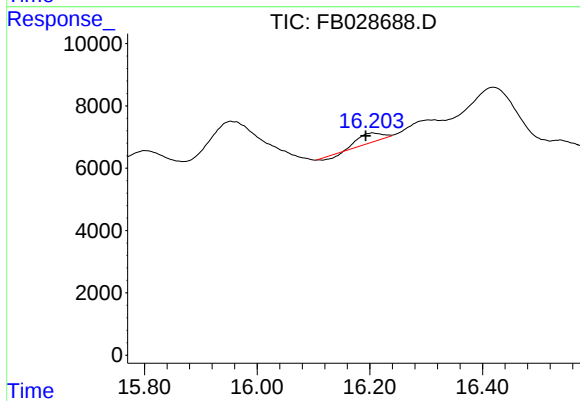

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.013 min
Response: 7123
Conc: 0.37 ng/ml