

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
 Data File : FB028690.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Oct 2022 2:49  
 Operator : AJ/MA  
 Sample : N5193-14  
 Misc : 6.32G/5.00 ML DI WATER  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Oct 22 16:41:55 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
 Quant Title :  
 QLast Update : Wed Oct 05 12:47:25 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.796  | 286961   | 22.181 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.706  | 15724    | 0.961 ng/ml  |
| 2) t 2,2,4-Trimethylpentane  | 7.436  | 688      | 0.038 ng/ml  |
| 3) t n-Heptane               | 7.762  | 4323     | 0.255 ng/ml  |
| 7) t Ethylbenzene            | 13.031 | 431383   | 21.736 ng/ml |
| 9) t O-Xylene                | 13.922 | 129250   | 6.644 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.199 | 14239    | 0.736 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
Data File : FB028690.D  
Signal(s) : FID2B.CH  
Acq On : 22 Oct 2022 2:49  
Operator : AJ/MA  
Sample : N5193-14  
Misc : 6.32G/5.00 ML DI WATER  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 22 16:41:55 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

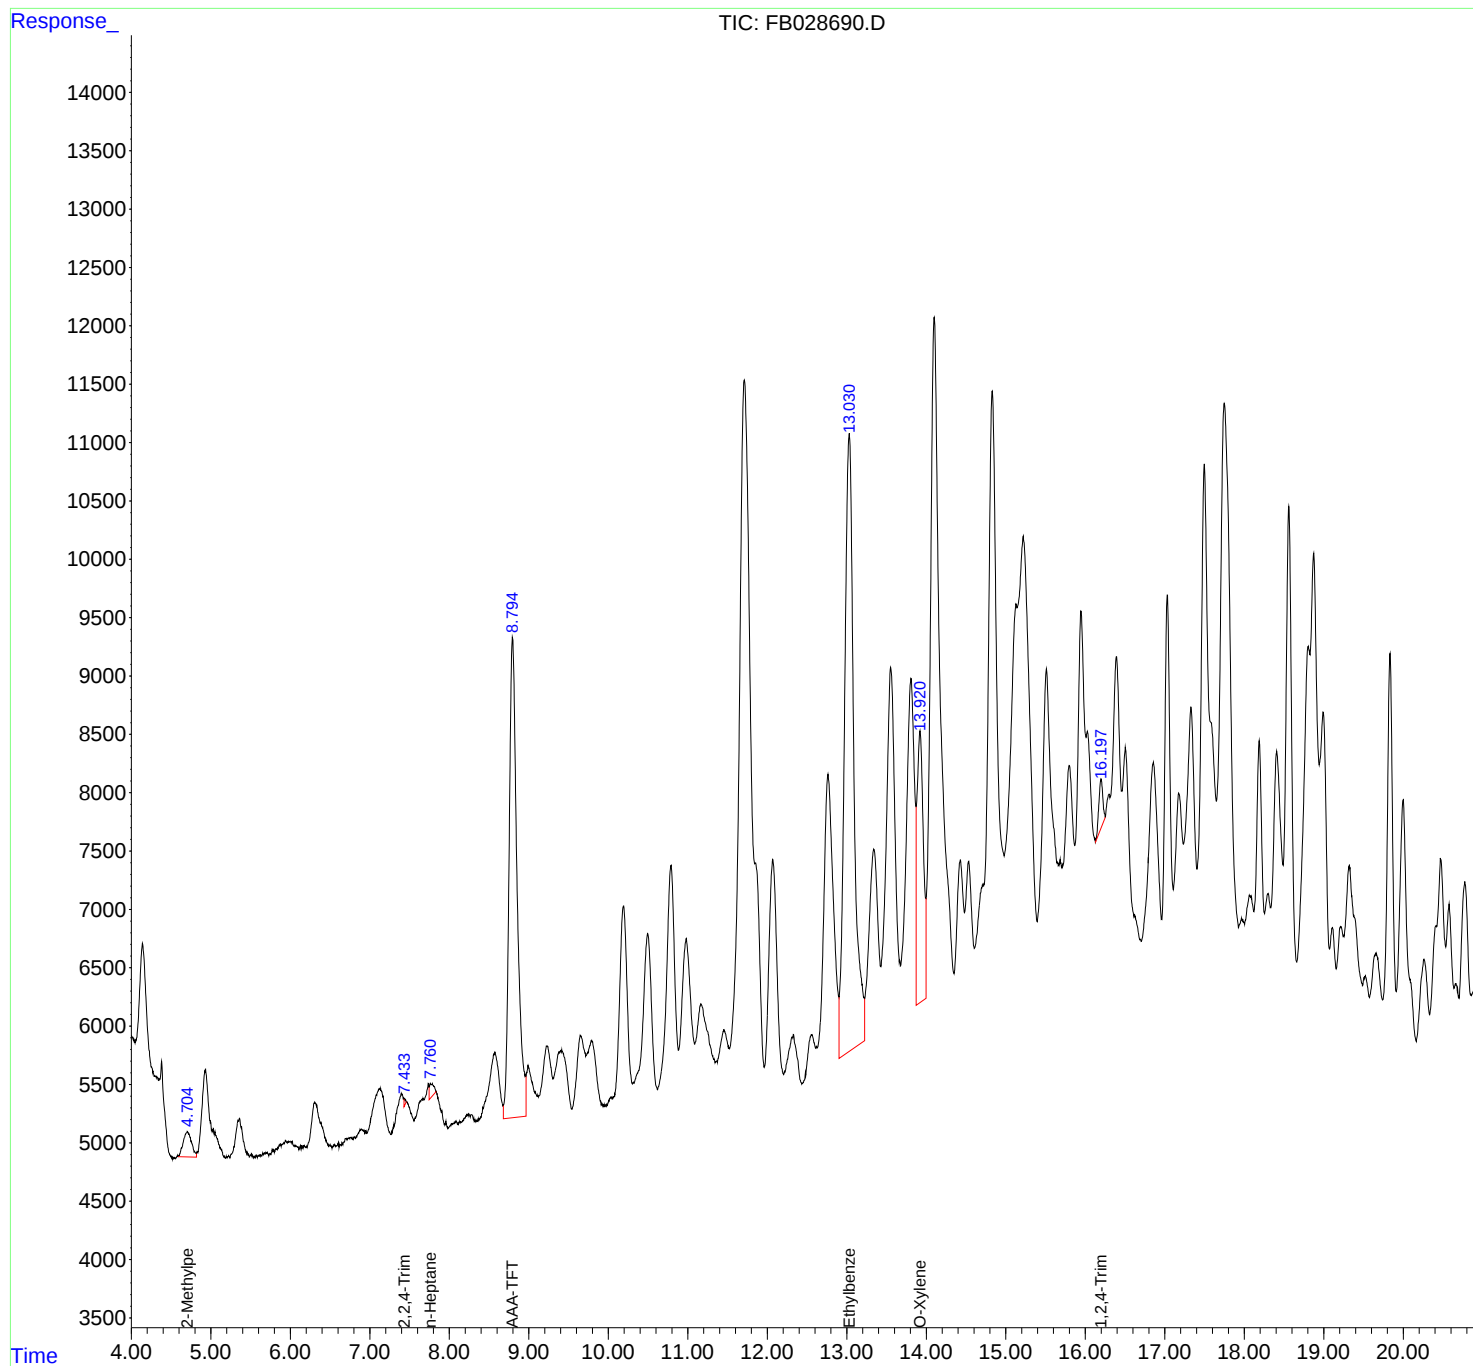


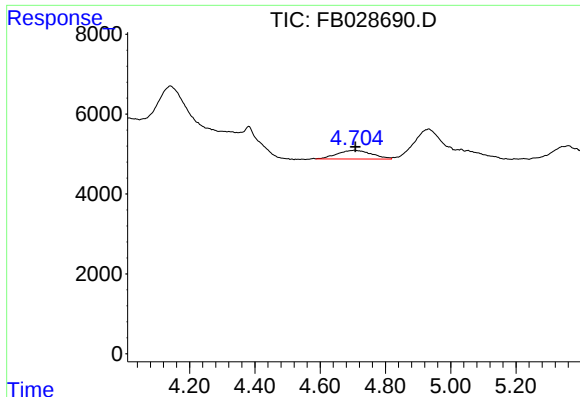

#1 2-Methylpentane


R.T.: 4.706 min  
Delta R.T.: -0.002 min  
Response: 15724  
Conc: 0.96 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

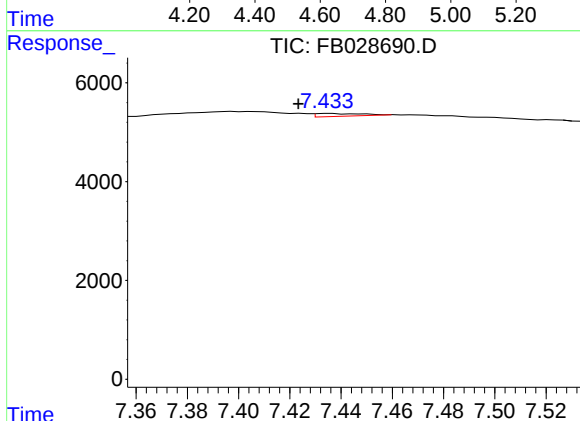


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min  
Delta R.T.: 0.013 min  
Response: 688  
Conc: 0.04 ng/ml

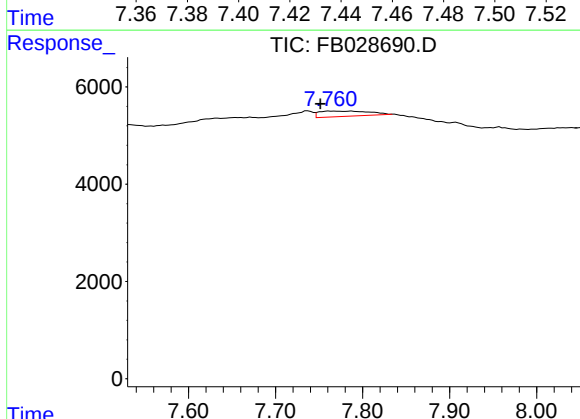


#3 n-Heptane

R.T.: 7.762 min  
Delta R.T.: 0.010 min  
Response: 4323  
Conc: 0.26 ng/ml

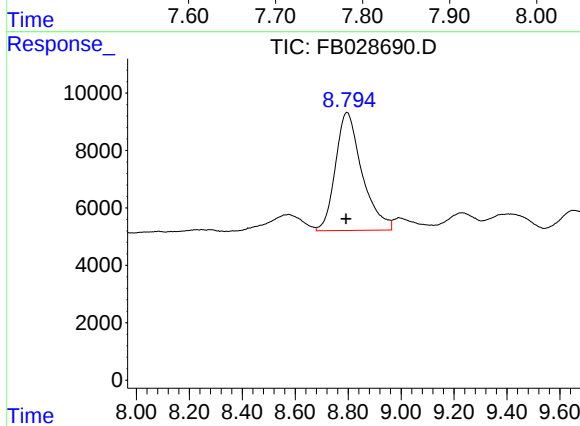

#5 AAA-TFT


R.T.: 8.796 min  
Delta R.T.: 0.003 min  
Response: 286961  
Conc: 22.18 ng/ml

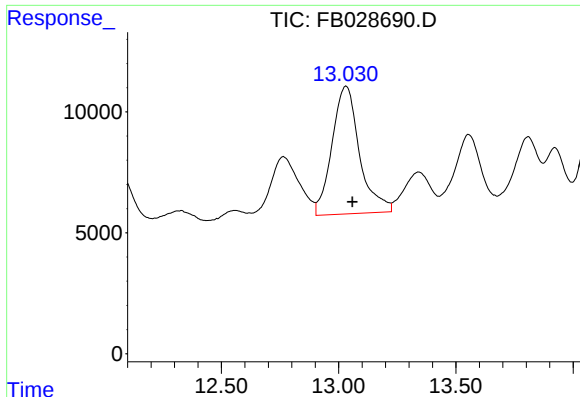

#7 Ethylbenzene


R.T.: 13.031 min  
Delta R.T.: -0.026 min  
Response: 431383  
Conc: 21.74 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

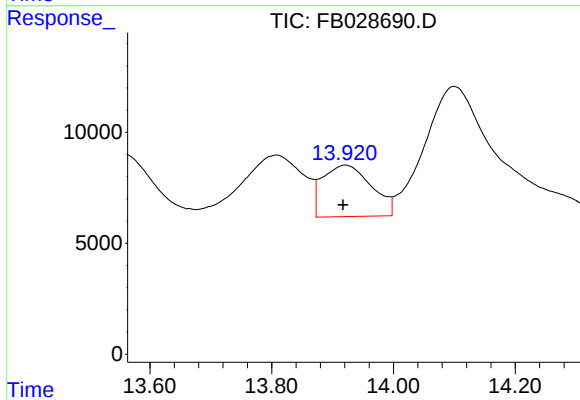

#9 O-Xylene

R.T.: 13.922 min  
Delta R.T.: 0.004 min  
Response: 129250  
Conc: 6.64 ng/ml

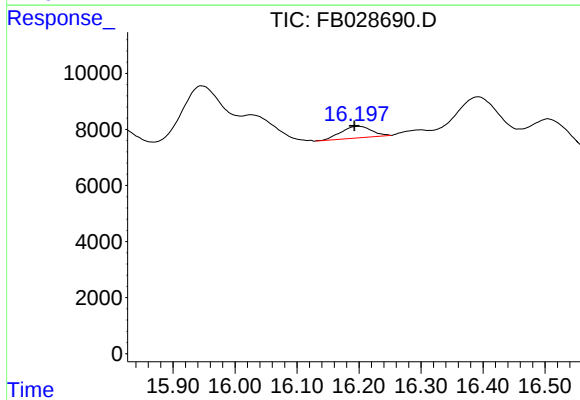

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min  
Delta R.T.: 0.007 min  
Response: 14239  
Conc: 0.74 ng/ml