

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
 Data File : FB028666.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2022 10:26
 Operator : AJ/MA
 Sample : BSF1021S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1021S1

Integration File: Calibration.e
 Quant Time: Oct 21 17:18:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	244290	18.883 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	491902	30.069 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	526375	29.126 ng/ml
3) t n-Heptane	7.748	165574	9.775 ng/ml
4) t Benzene	7.884	205512	9.357 ng/ml
6) t Toluene	10.617	587028	28.007 ng/ml
7) t Ethylbenzene	13.054	188470	9.496 ng/ml
8) t m-Xylene	13.186	372908	18.928 ng/ml
9) t O-Xylene	13.914	376988	19.378 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	386121	19.945 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
Data File : FB028666.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2022 10:26
Operator : AJ/MA
Sample : BSF1021S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1021S1

Integration File: Calibration.e
Quant Time: Oct 21 17:18:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

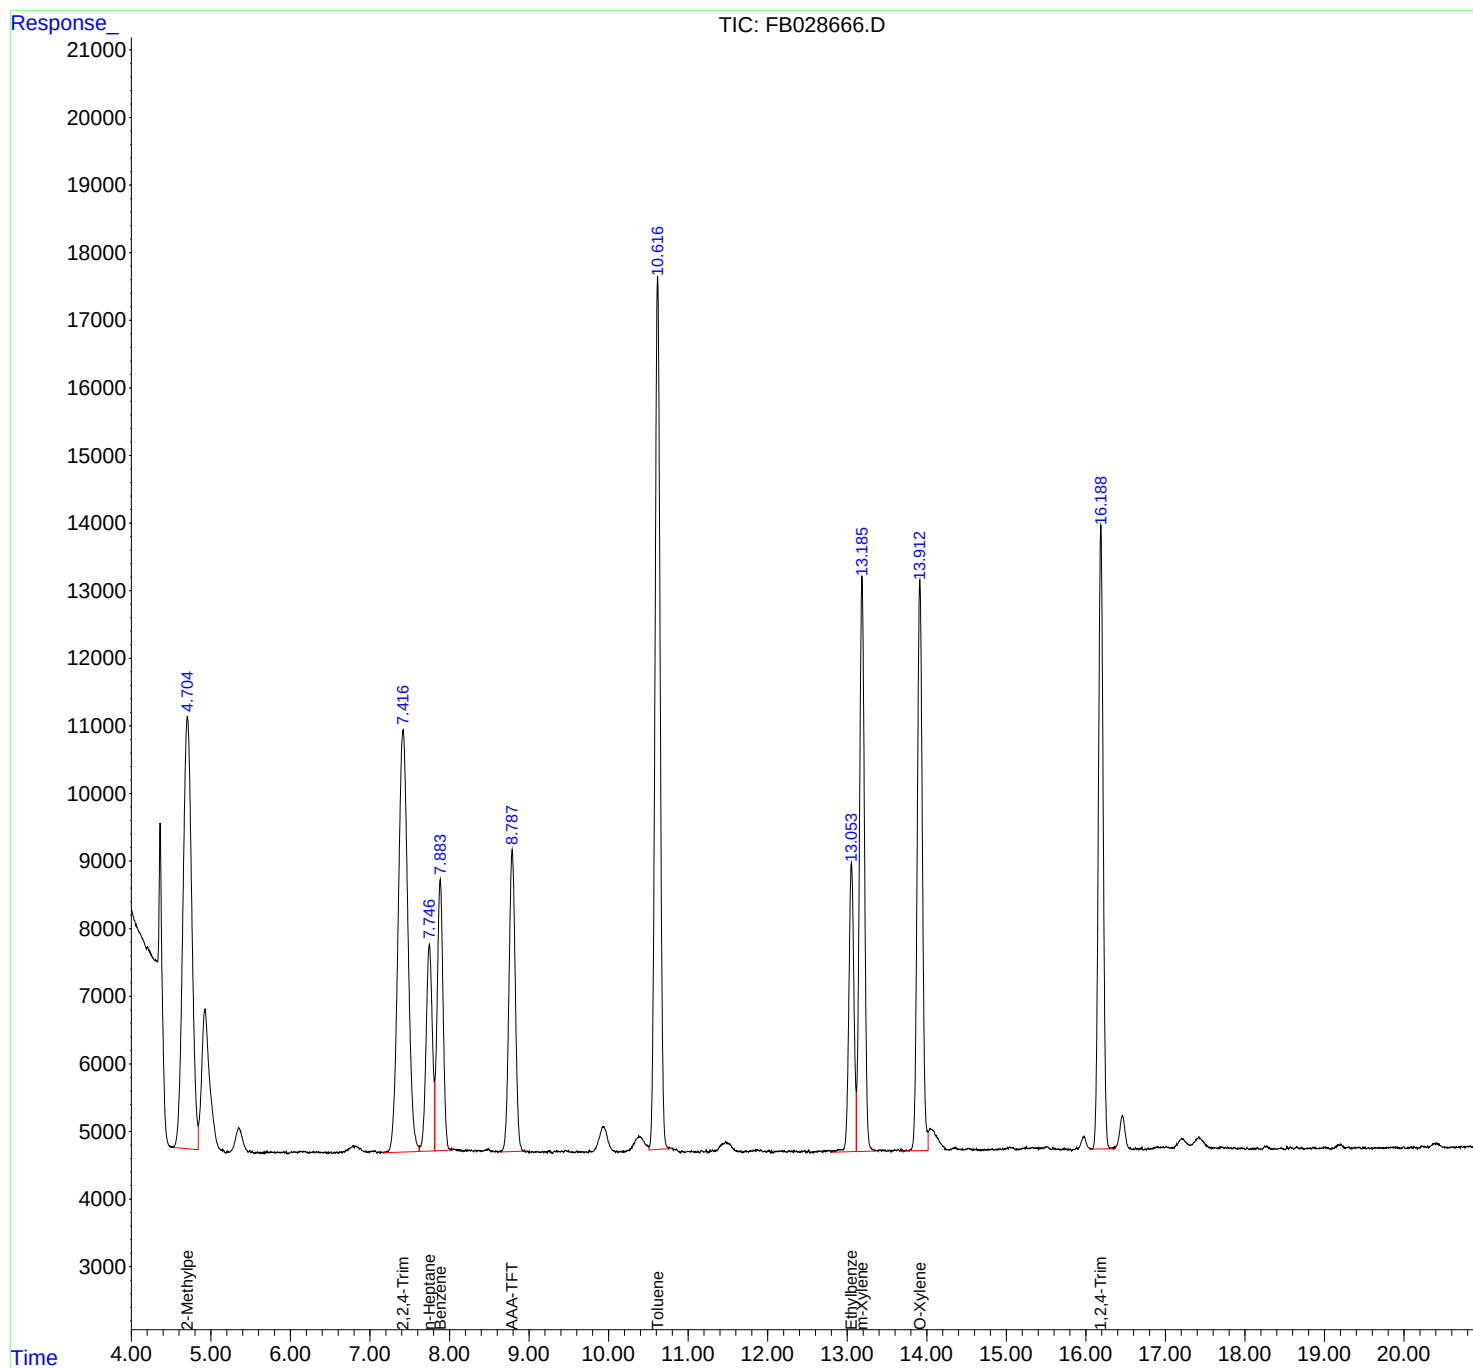


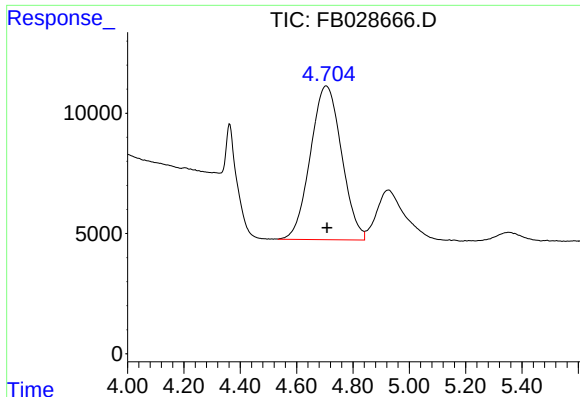

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 491902
Conc: 30.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S1

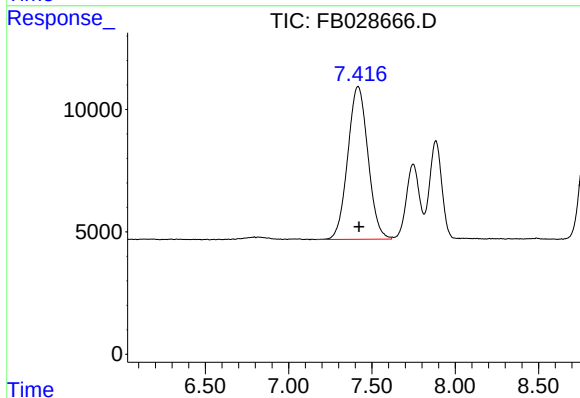


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.006 min
Response: 526375
Conc: 29.13 ng/ml

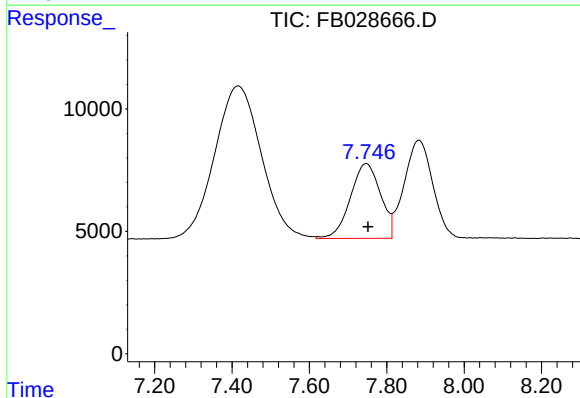


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.004 min
Response: 165574
Conc: 9.78 ng/ml

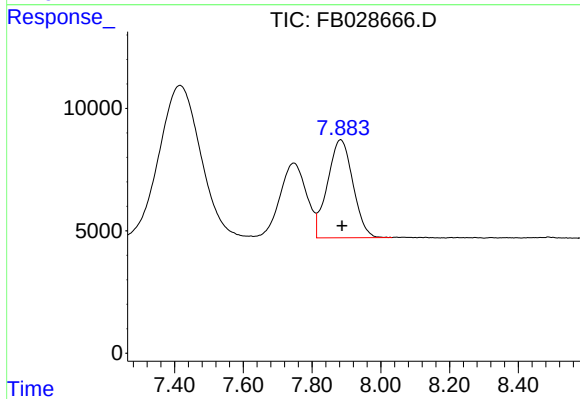

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.004 min
Response: 205512
Conc: 9.36 ng/ml

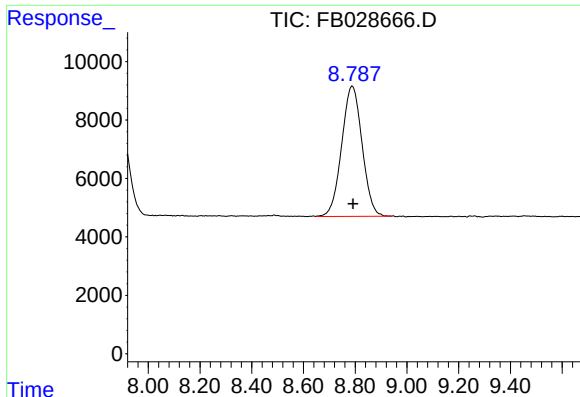

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 244290
Conc: 18.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S1

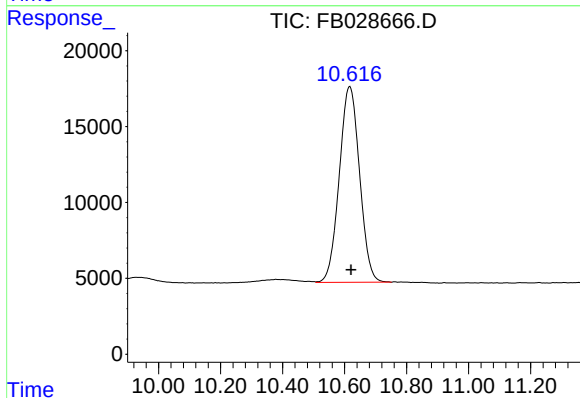


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 587028
Conc: 28.01 ng/ml

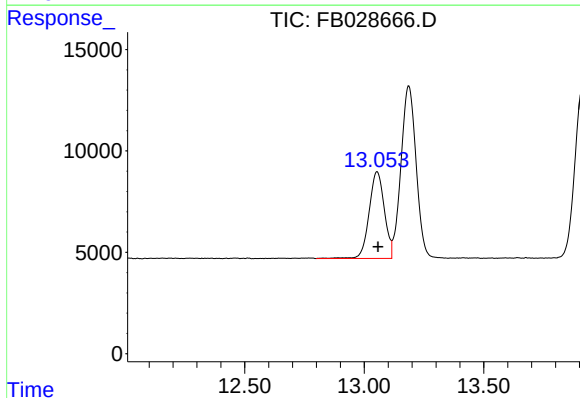


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 188470
Conc: 9.50 ng/ml

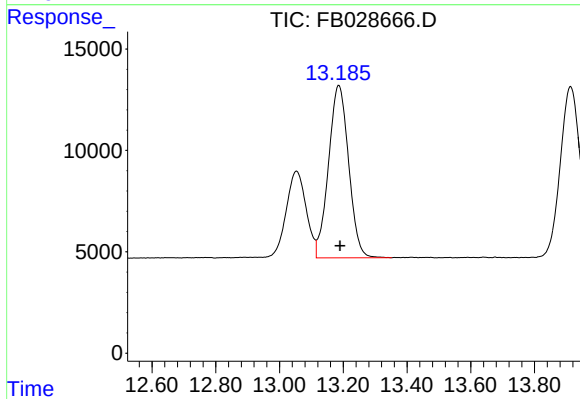

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.004 min
Response: 372908
Conc: 18.93 ng/ml

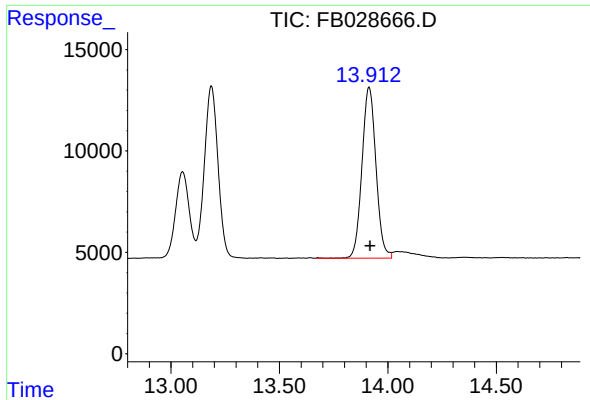

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 376988
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S1

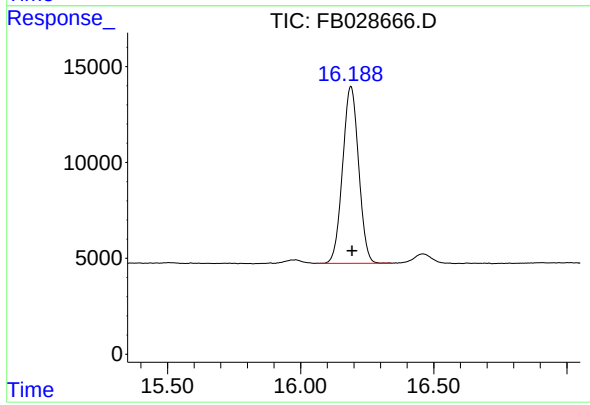

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.004 min
Response: 386121
Conc: 19.95 ng/ml