

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
 Data File : FB028673.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2022 15:00
 Operator : AJ/MA
 Sample : BSF1021S2
 Misc : 5.49G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1021S2

Integration File: Calibration.e
 Quant Time: Oct 21 17:19:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	273206	21.118 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	502067	30.691 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	546695	30.251 ng/ml
3) t n-Heptane	7.751	175007	10.332 ng/ml
4) t Benzene	7.888	216858	9.873 ng/ml
6) t Toluene	10.622	618701	29.518 ng/ml
7) t Ethylbenzene	13.059	195221	9.837 ng/ml
8) t m-Xylene	13.192	384546	19.519 ng/ml
9) t O-Xylene	13.919	378340	19.447 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	363644	18.784 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
Data File : FB028673.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2022 15:00
Operator : AJ/MA
Sample : BSF1021S2
Misc : 5.49G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1021S2

Integration File: Calibration.e
Quant Time: Oct 21 17:19:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

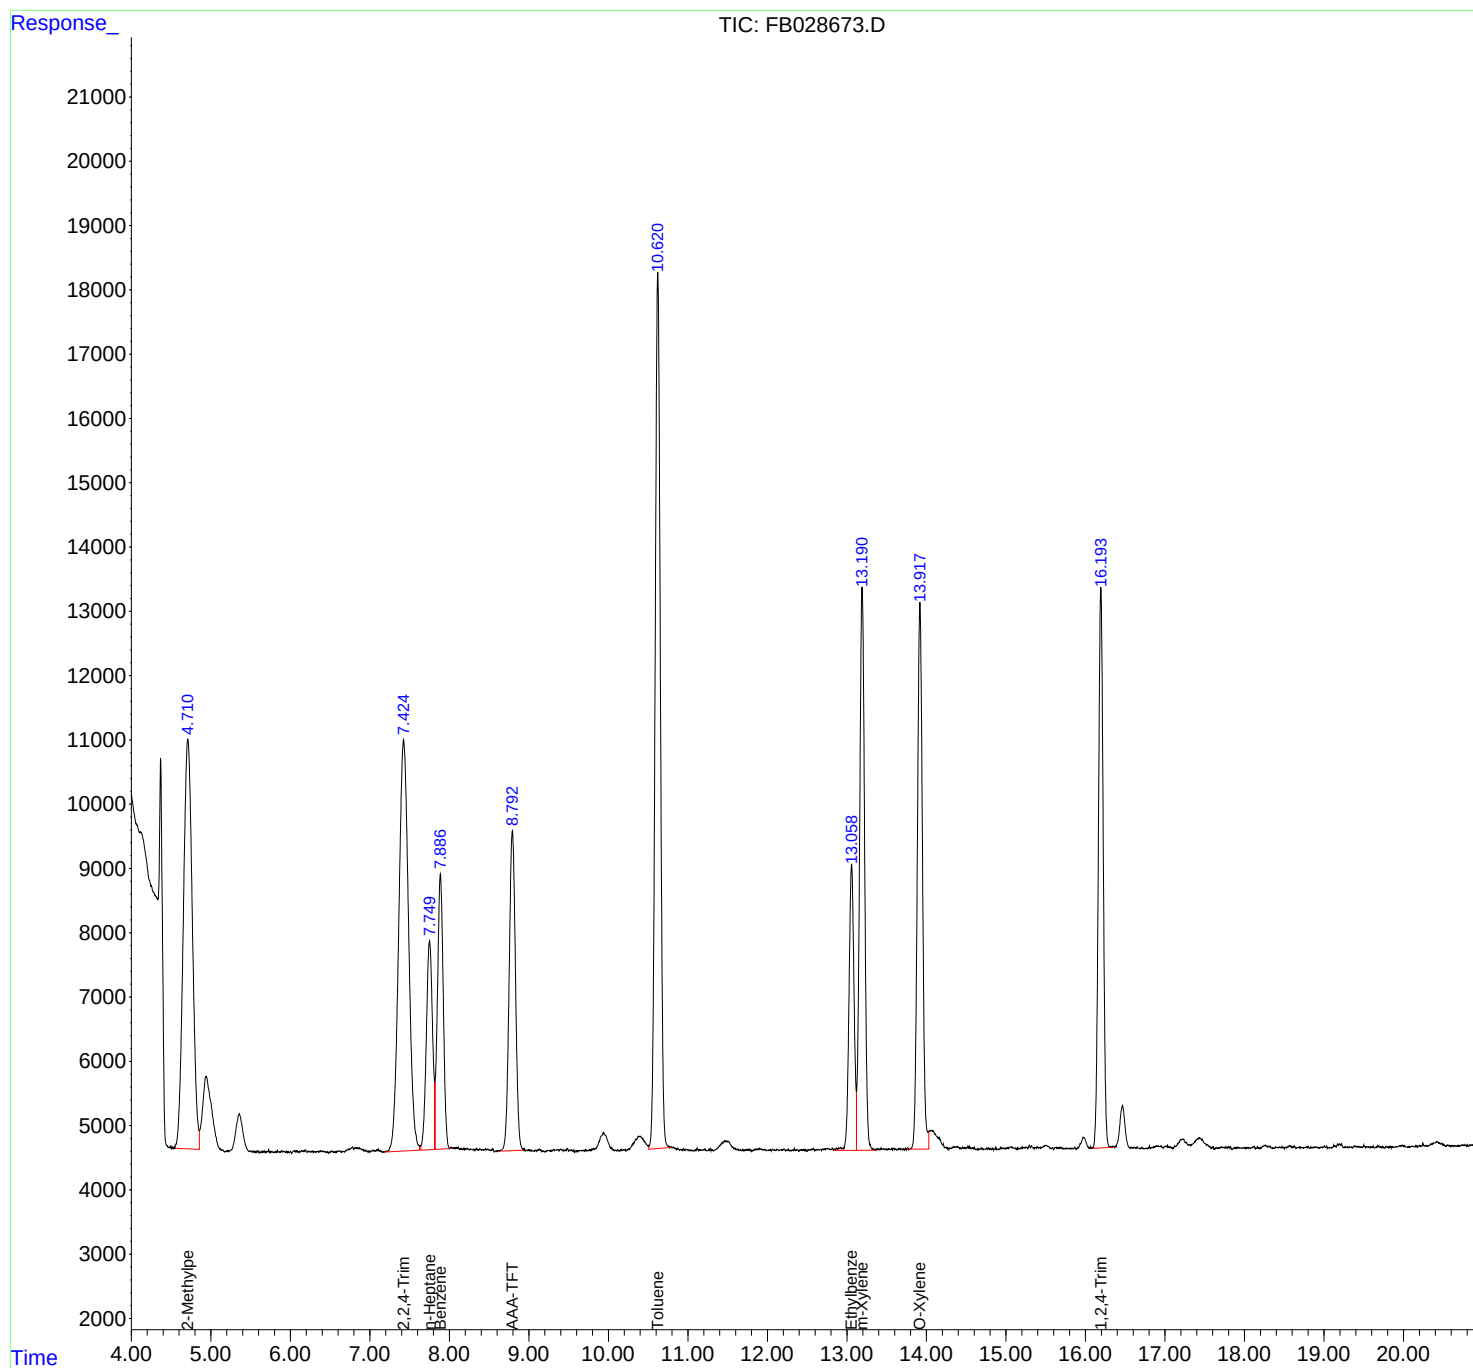


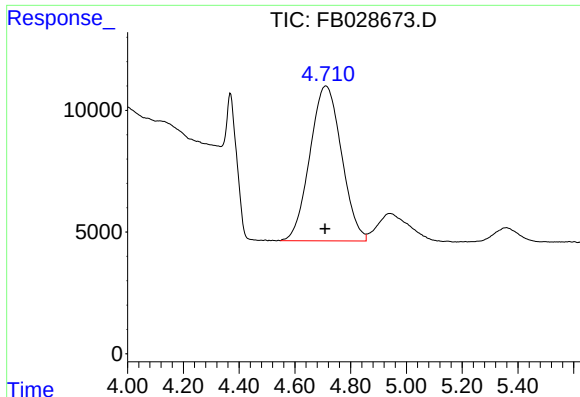

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.003 min
Response: 502067
Conc: 30.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S2

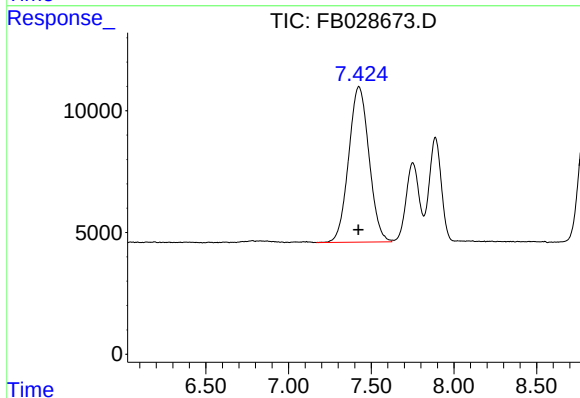


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.002 min
Response: 546695
Conc: 30.25 ng/ml

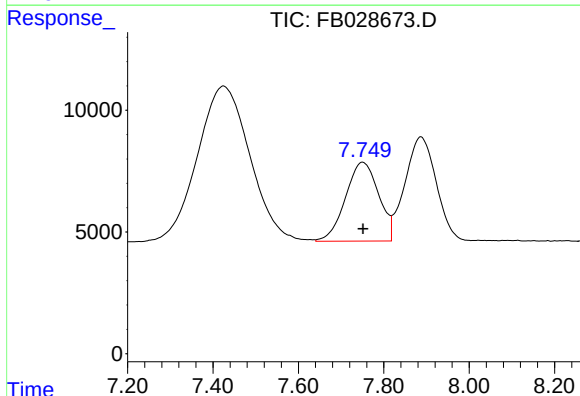


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 175007
Conc: 10.33 ng/ml

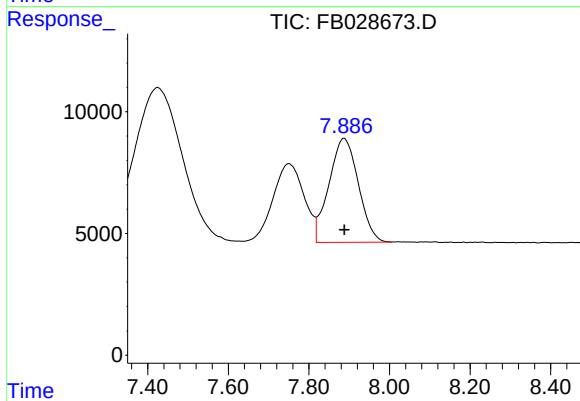

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 216858
Conc: 9.87 ng/ml

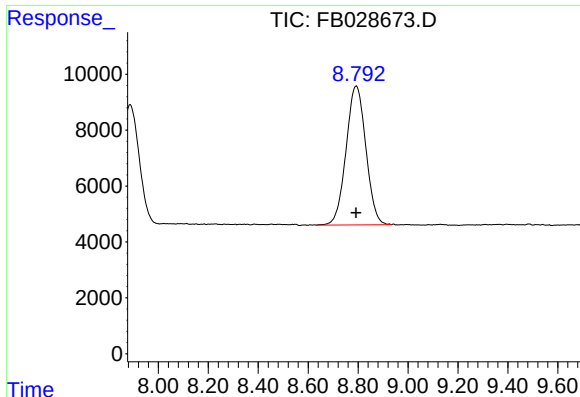

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 273206
Conc: 21.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S2

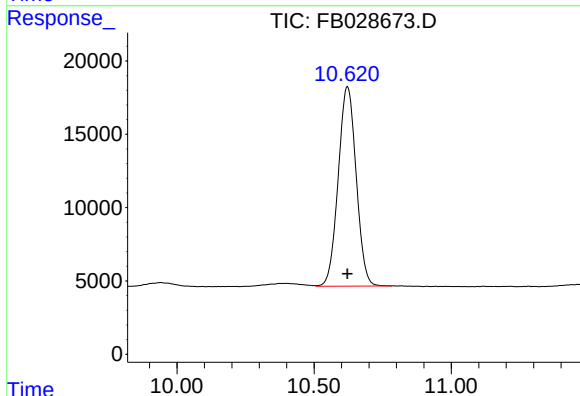


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 618701
Conc: 29.52 ng/ml

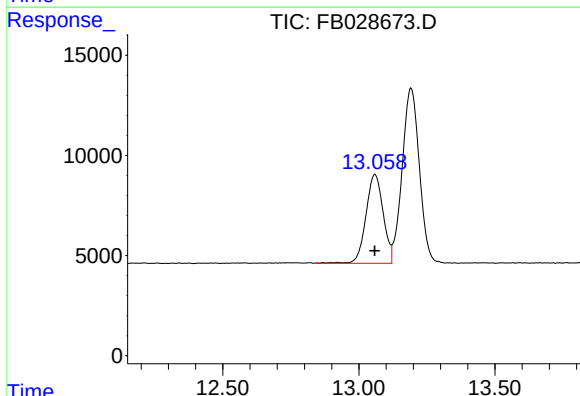


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.001 min
Response: 195221
Conc: 9.84 ng/ml

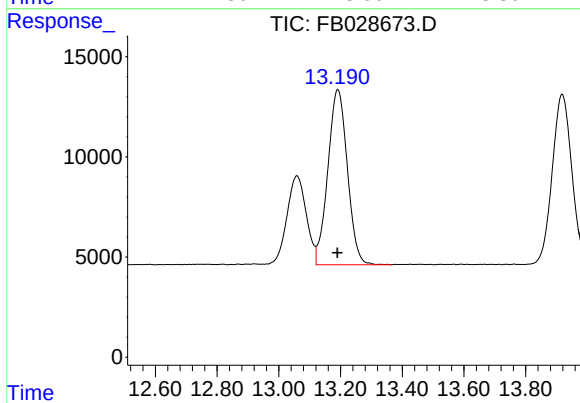

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.001 min
Response: 384546
Conc: 19.52 ng/ml

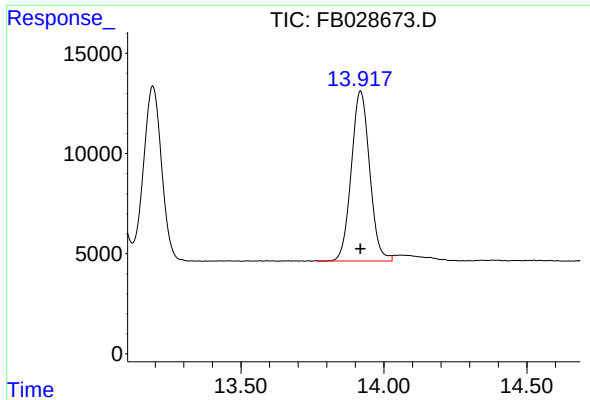

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.001 min
Response: 378340
Conc: 19.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S2

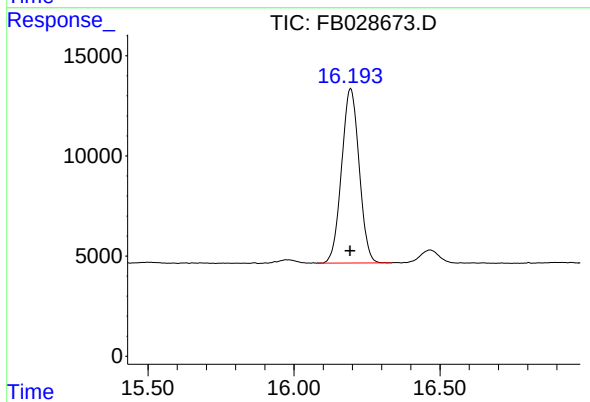

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 363644
Conc: 18.78 ng/ml