

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
Data File : FB028676.D  
Signal(s) : FID2B.CH  
Acq On : 21 Oct 2022 17:39  
Operator : AJ/MA  
Sample : N5193-14  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
LSP-SS-07-20-40

Integration File: Calibration.e  
Quant Time: Oct 22 16:40:51 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 8) t m-Xylene               | 13.228 | 4365     | 0.222 ng/ml |
| 9) t O-Xylene               | 13.861 | 3691     | 0.190 ng/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102122\  
Data File : FB028676.D  
Signal(s) : FID2B.CH  
Acq On : 21 Oct 2022 17:39  
Operator : AJ/MA  
Sample : N5193-14  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
LSP-SS-07-20-40

Integration File: Calibration.e  
Quant Time: Oct 22 16:40:51 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

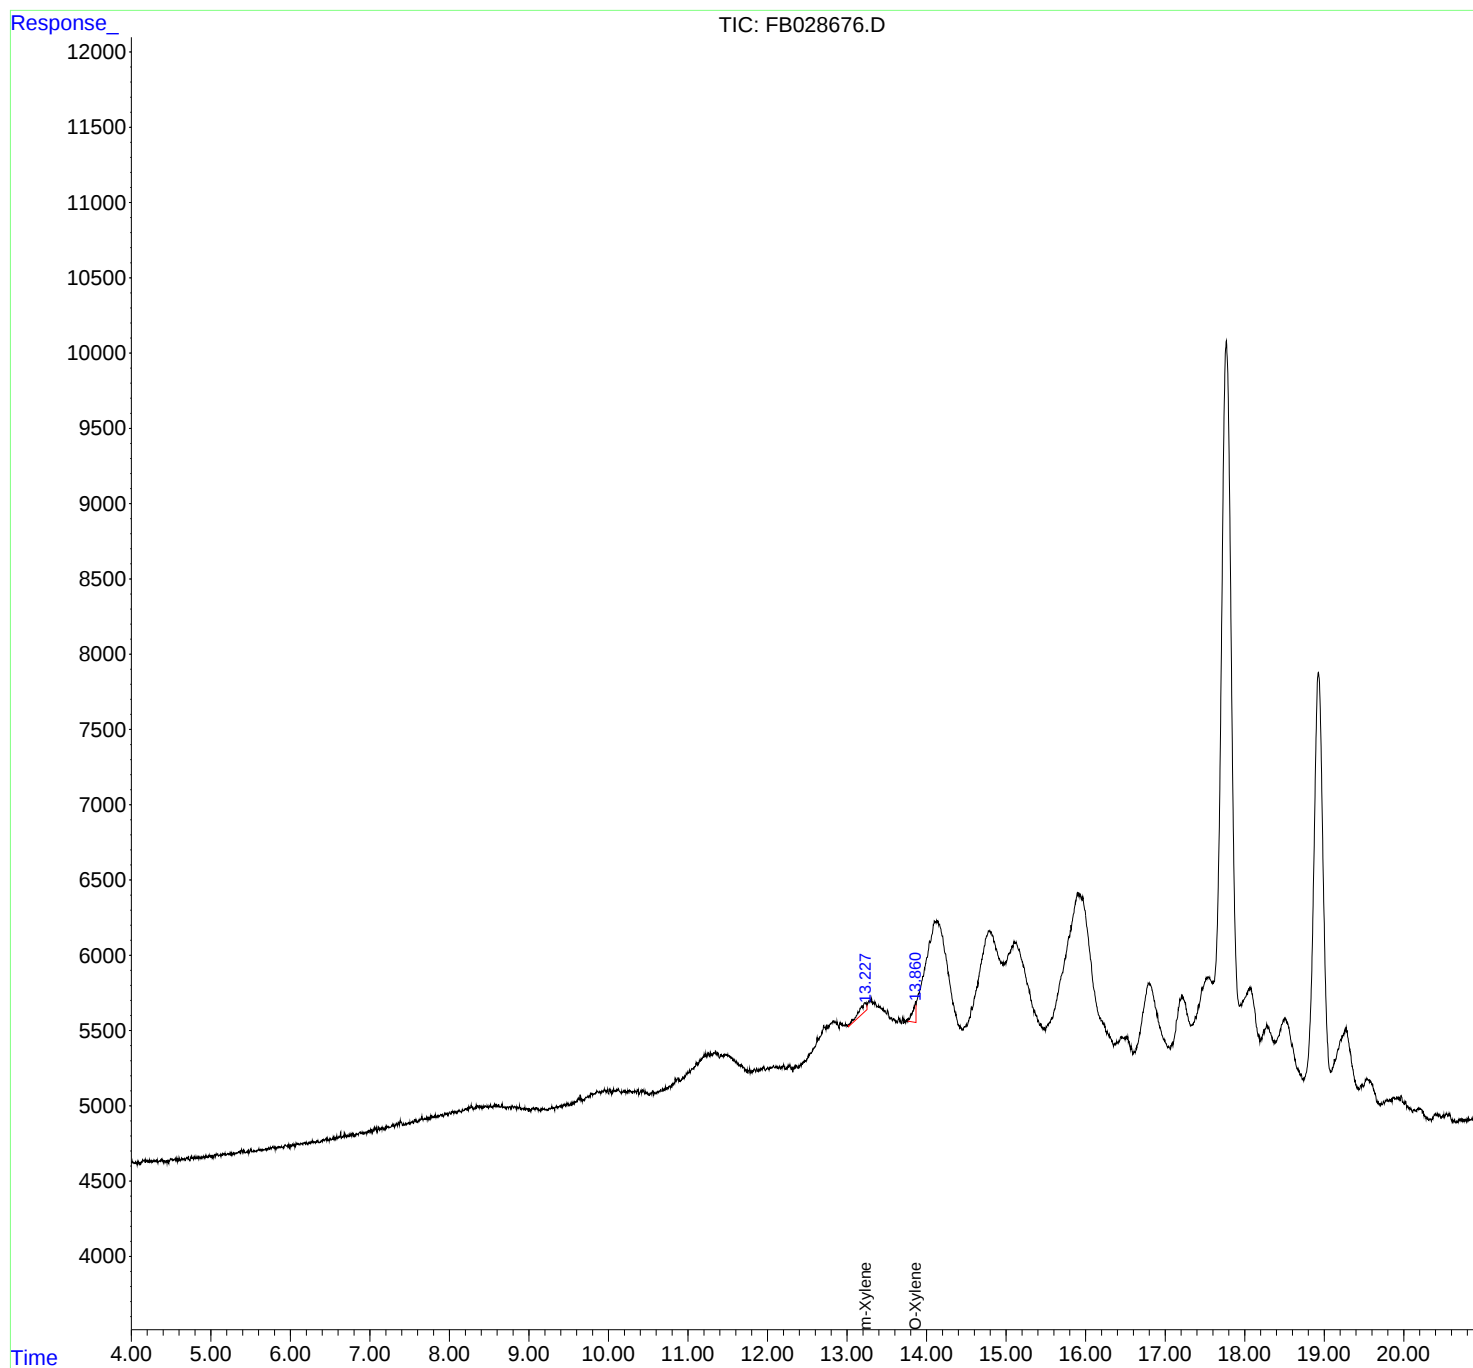


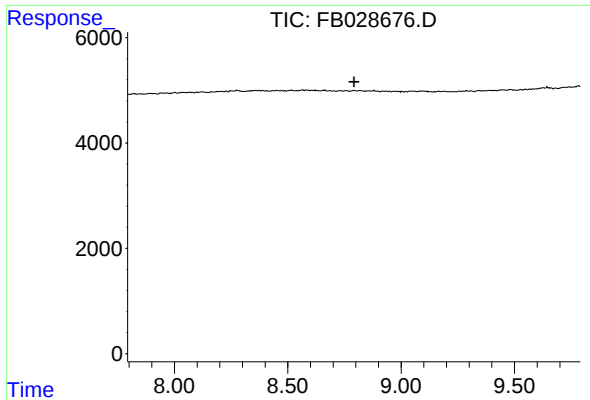

#5 AAA-TFT


R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
LSP-SS-07-20-40

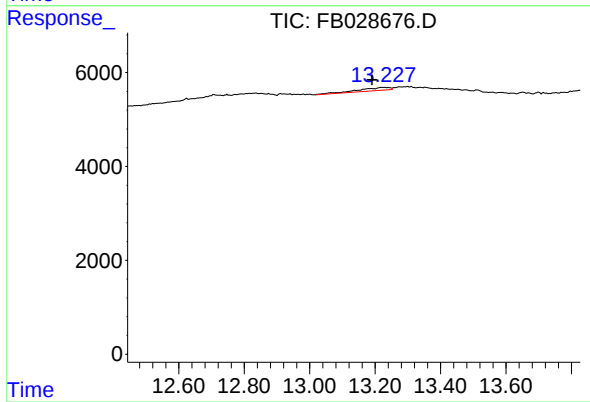

#8 m-Xylene

R.T.: 13.228 min  
Delta R.T.: 0.038 min  
Response: 4365  
Conc: 0.22 ng/ml

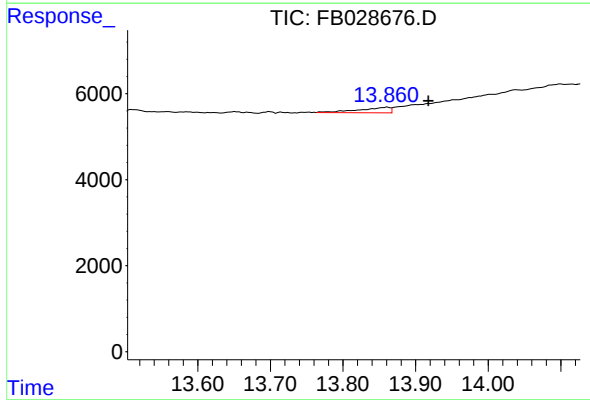

#9 O-Xylene

R.T.: 13.861 min  
Delta R.T.: -0.056 min  
Response: 3691  
Conc: 0.19 ng/ml