

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
 Data File : FB028684.D
 Signal(s) : FID2B.CH
 Acq On : 21 Oct 2022 22:57
 Operator : AJ/MA
 Sample : BSF1021S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1021S3

Integration File: Calibration.e
 Quant Time: Oct 22 16:41:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	248327	19.195 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	474843	29.026 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	535231	29.616 ng/ml
3) t n-Heptane	7.750	160360	9.467 ng/ml
4) t Benzene	7.887	204622	9.316 ng/ml
6) t Toluene	10.620	578934	27.621 ng/ml
7) t Ethylbenzene	13.056	182976	9.220 ng/ml
8) t m-Xylene	13.189	365755	18.565 ng/ml
9) t O-Xylene	13.917	368415	18.937 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	370851	19.156 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102122\
Data File : FB028684.D
Signal(s) : FID2B.CH
Acq On : 21 Oct 2022 22:57
Operator : AJ/MA
Sample : BSF1021S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1021S3

Integration File: Calibration.e
Quant Time: Oct 22 16:41:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

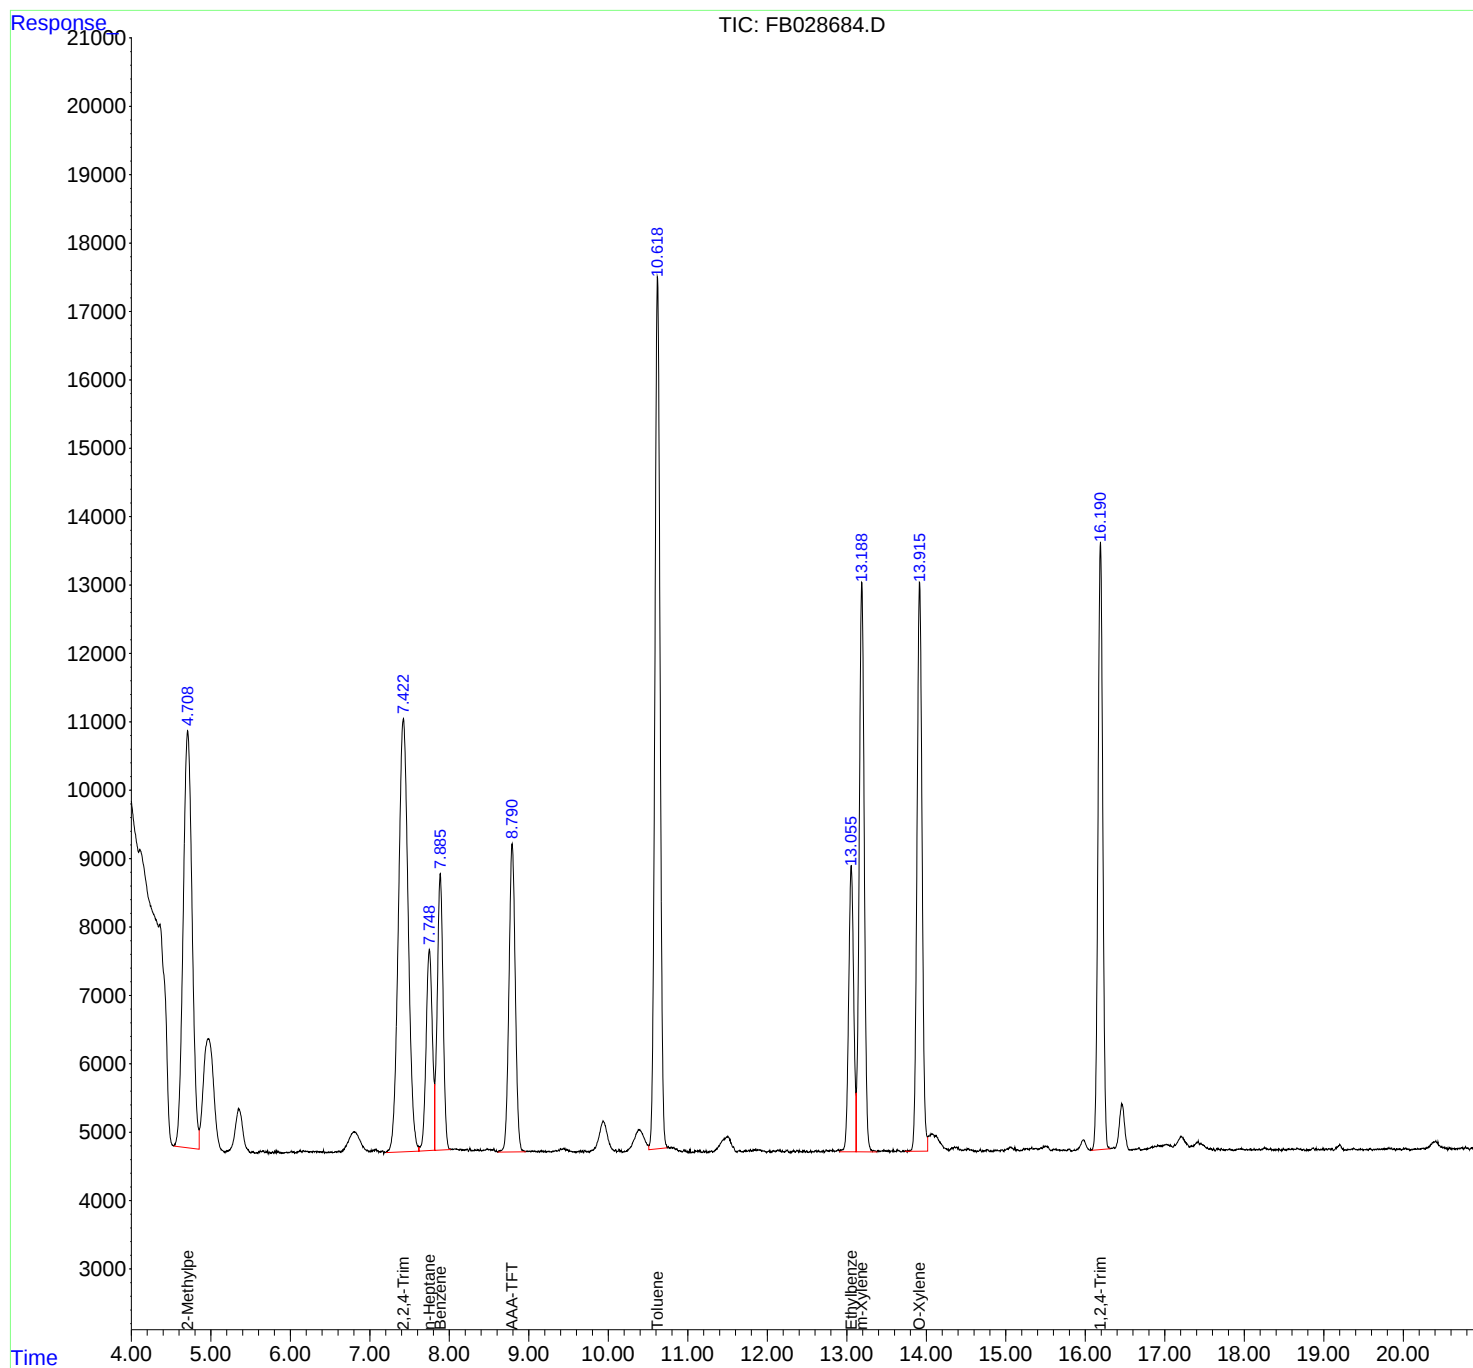


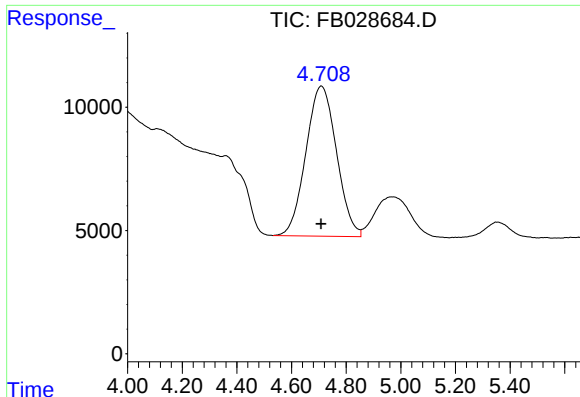

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.002 min
Response: 474843
Conc: 29.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S3

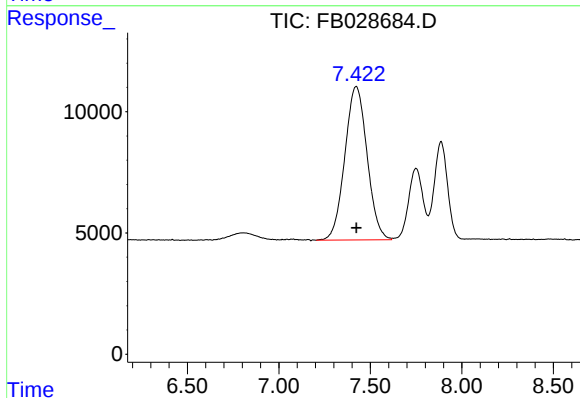


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 535231
Conc: 29.62 ng/ml

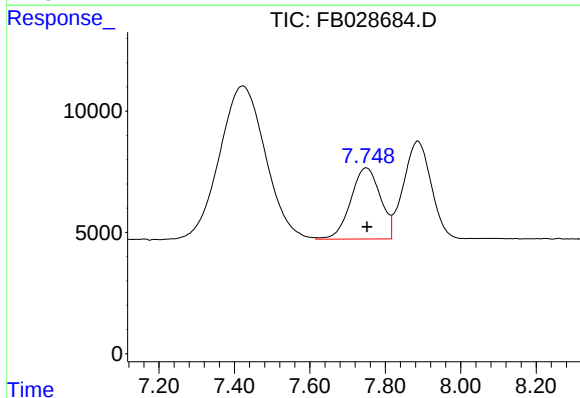


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 160360
Conc: 9.47 ng/ml

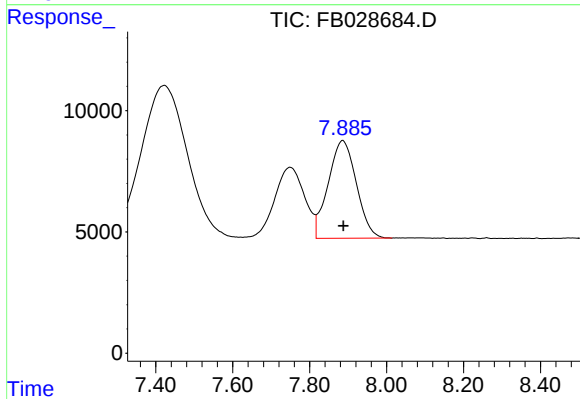

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.001 min
Response: 204622
Conc: 9.32 ng/ml

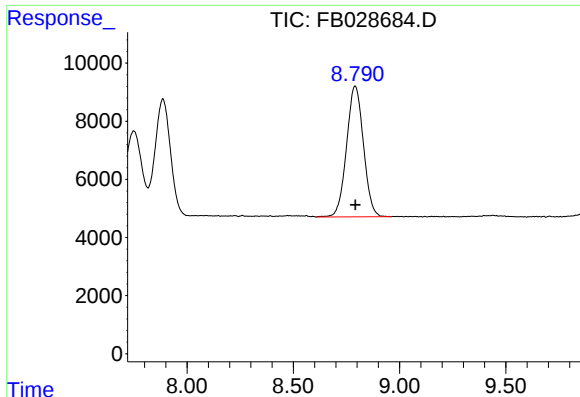

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 248327
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S3

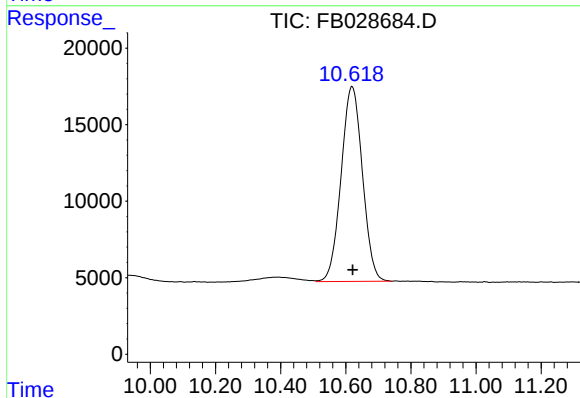


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 578934
Conc: 27.62 ng/ml

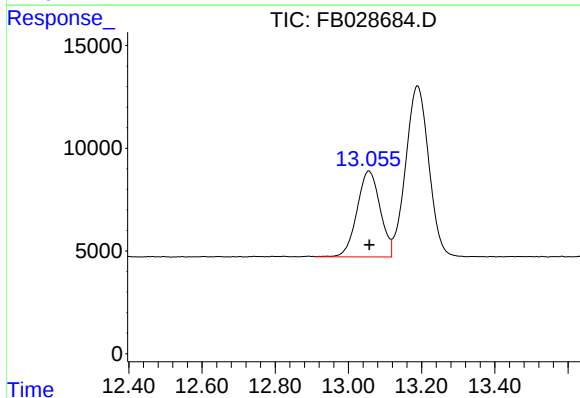


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.001 min
Response: 182976
Conc: 9.22 ng/ml

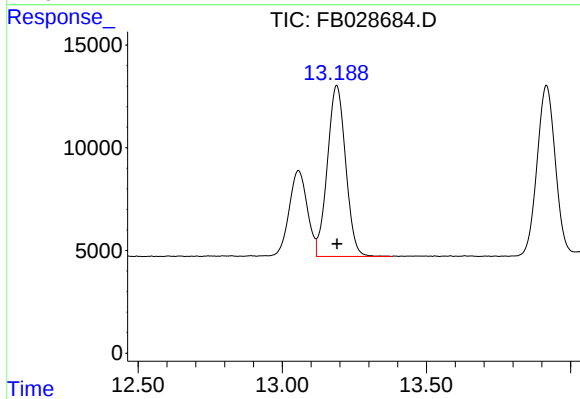

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.001 min
Response: 365755
Conc: 18.57 ng/ml

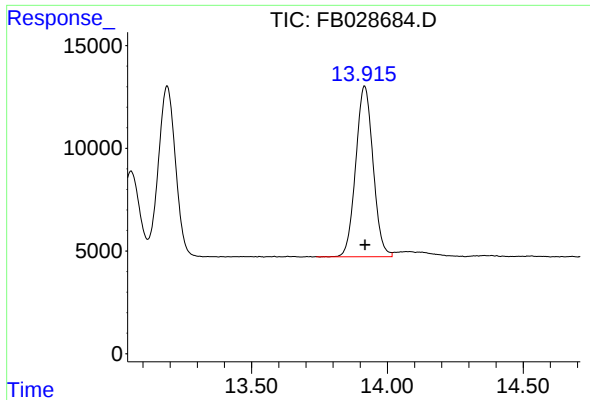

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 368415
Conc: 18.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1021S3

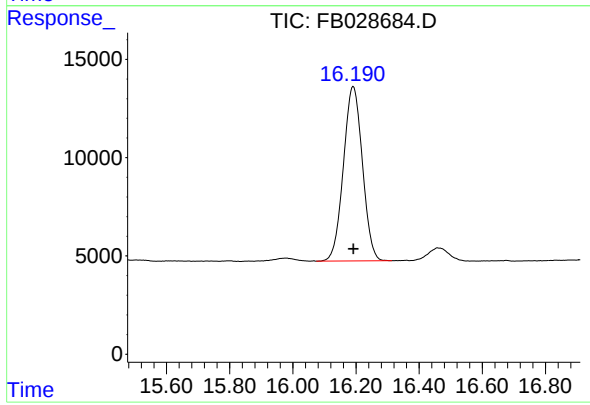

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 370851
Conc: 19.16 ng/ml