

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
 Data File : FB018304.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2018 22:45
 Operator : MJ/SJ
 Sample : J5605-08MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 23 08:16:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.108	195337	22.680 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.959	459980	30.075 ng/ml
2) t	2,2,4-Trimethylpentane	7.725	425029	28.764 ng/ml
3) t	n-Heptane	8.064	133910	9.449 ng/ml
4) t	Benzene	8.203	198056	10.632 ng/ml
6) t	Toluene	10.957	484530	31.792 ng/ml
7) t	Ethylbenzene	13.406	154007	9.707 ng/ml
8) t	m-Xylene	13.539	328184	19.724 ng/ml
9) t	O-Xylene	14.271	345980	19.405 ng/ml
10) t	1,2,4-Trimethylbenzene	16.554	383180	18.836 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
Data File : FB018304.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2018 22:45
Operator : MJ/SJ
Sample : J5605-08MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 23 08:16:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

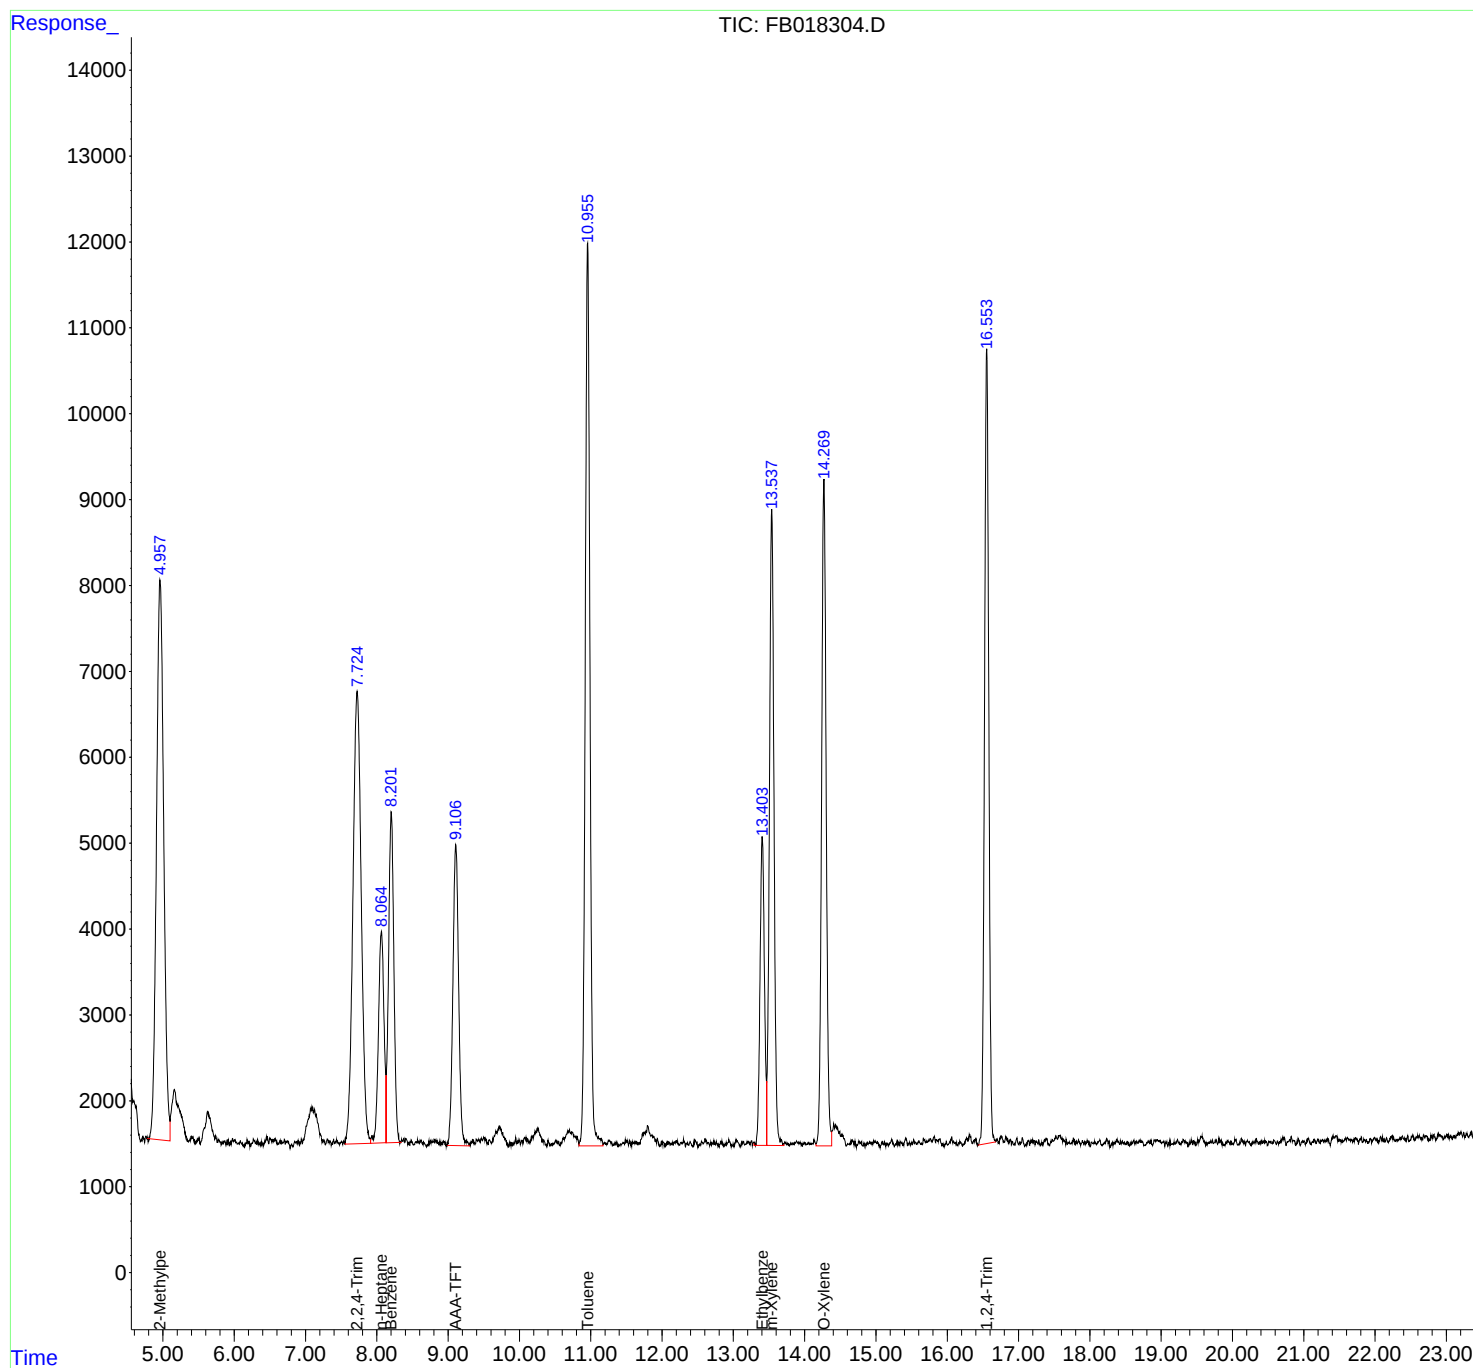

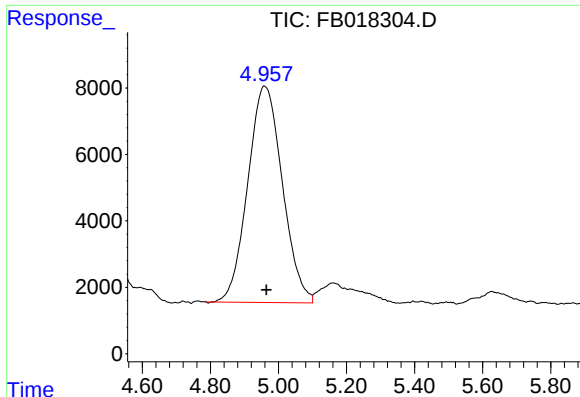


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 459980
Conc: 30.08 ng/ml

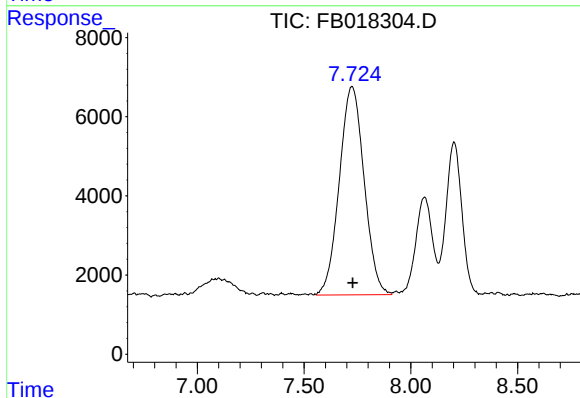


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.004 min
Response: 425029
Conc: 28.76 ng/ml

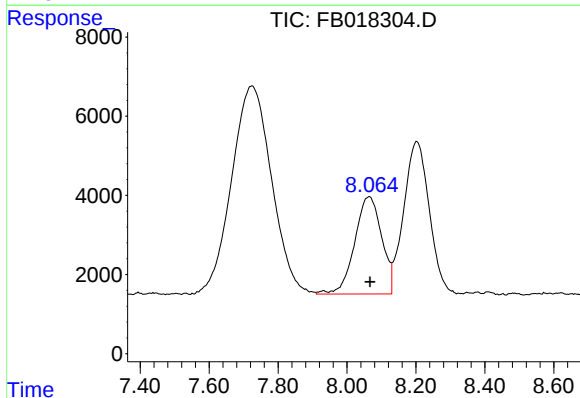


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.003 min
Response: 133910
Conc: 9.45 ng/ml

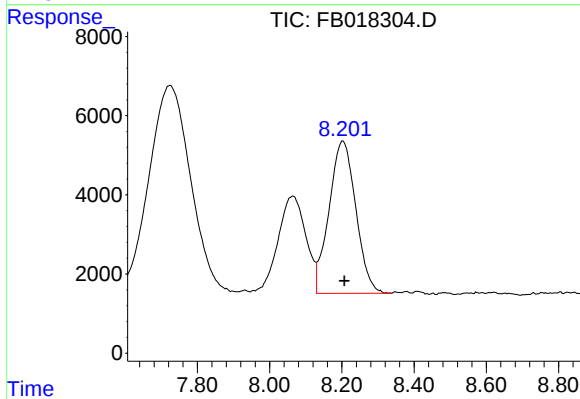


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 198056
Conc: 10.63 ng/ml

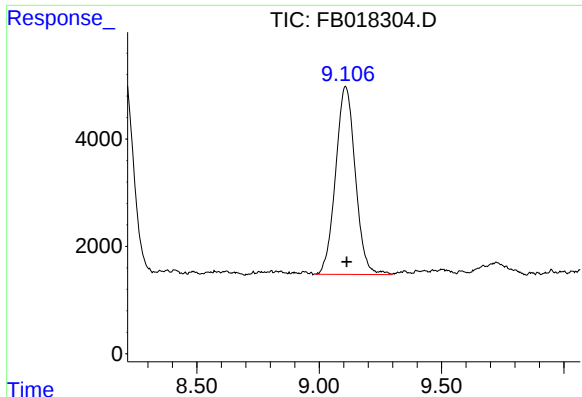


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.005 min
Response: 195337
Conc: 22.68 ng/ml

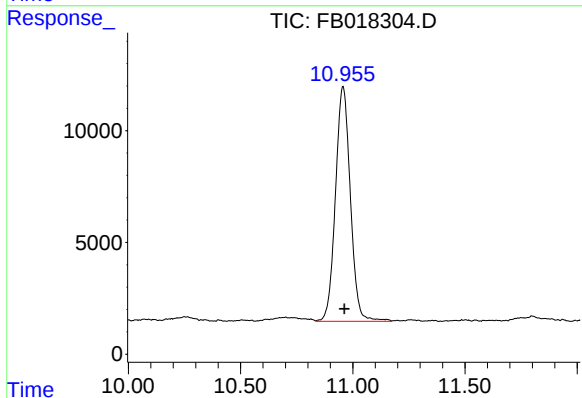


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.005 min
Response: 484530
Conc: 31.79 ng/ml

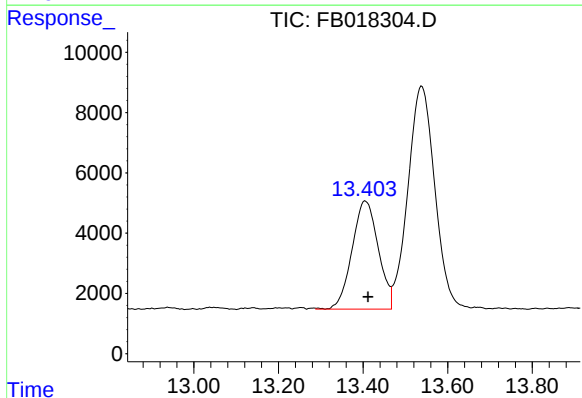


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.006 min
Response: 154007
Conc: 9.71 ng/ml

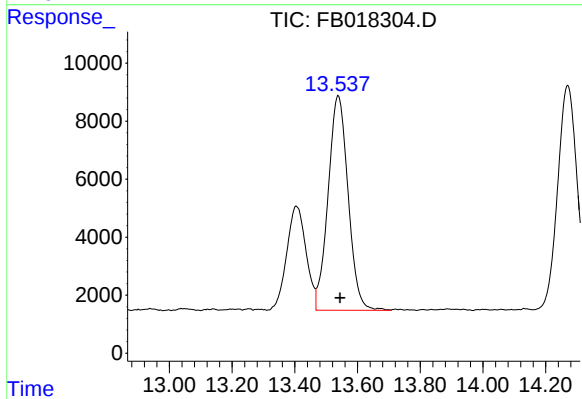


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.006 min
Response: 328184
Conc: 19.72 ng/ml

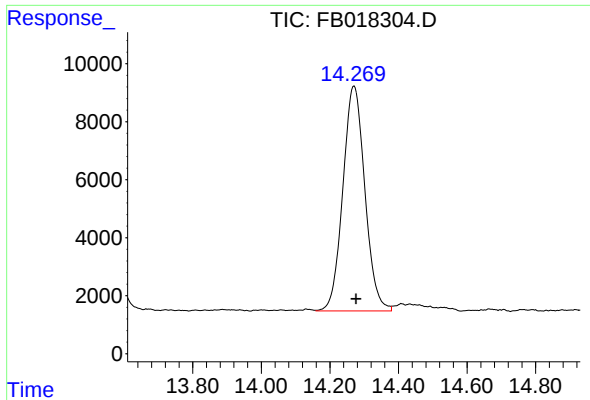

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.006 min
Response: 345980
Conc: 19.40 ng/ml

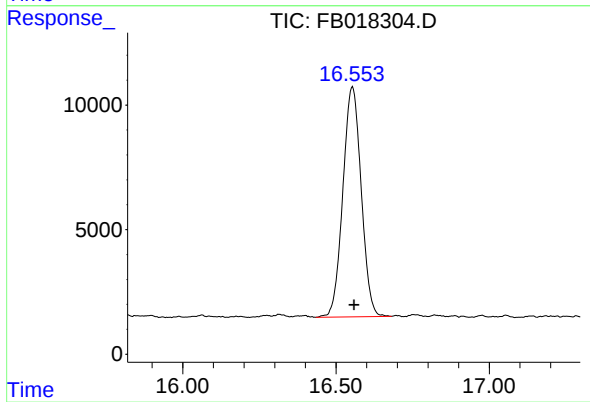

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.006 min
Response: 383180
Conc: 18.84 ng/ml