

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
 Data File : FB018307.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2018 00:46
 Operator : MJ/SJ
 Sample : J5604-03
 Misc : 5.05g/5.00mL DI Water
 ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 23 08:16:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.117	106835	12.404 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.017	45974	3.006 ng/ml
2) t 2,2,4-Trimethylpentane	7.711	6938	0.470 ng/ml
3) t n-Heptane	8.082	22858	1.613 ng/ml
4) t Benzene	8.202	24347	1.307 ng/ml
6) t Toluene	10.958	28006	1.838 ng/ml
7) t Ethylbenzene	13.391	49680	3.131 ng/ml
8) t m-Xylene	13.536	53190	3.197 ng/ml
9) t O-Xylene	14.275	67891	3.808 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	30822	1.515 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
Data File : FB018307.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2018 00:46
Operator : MJ/SJ
Sample : J5604-03
Misc : 5.05g/5.00mL DI Water
ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 23 08:16:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

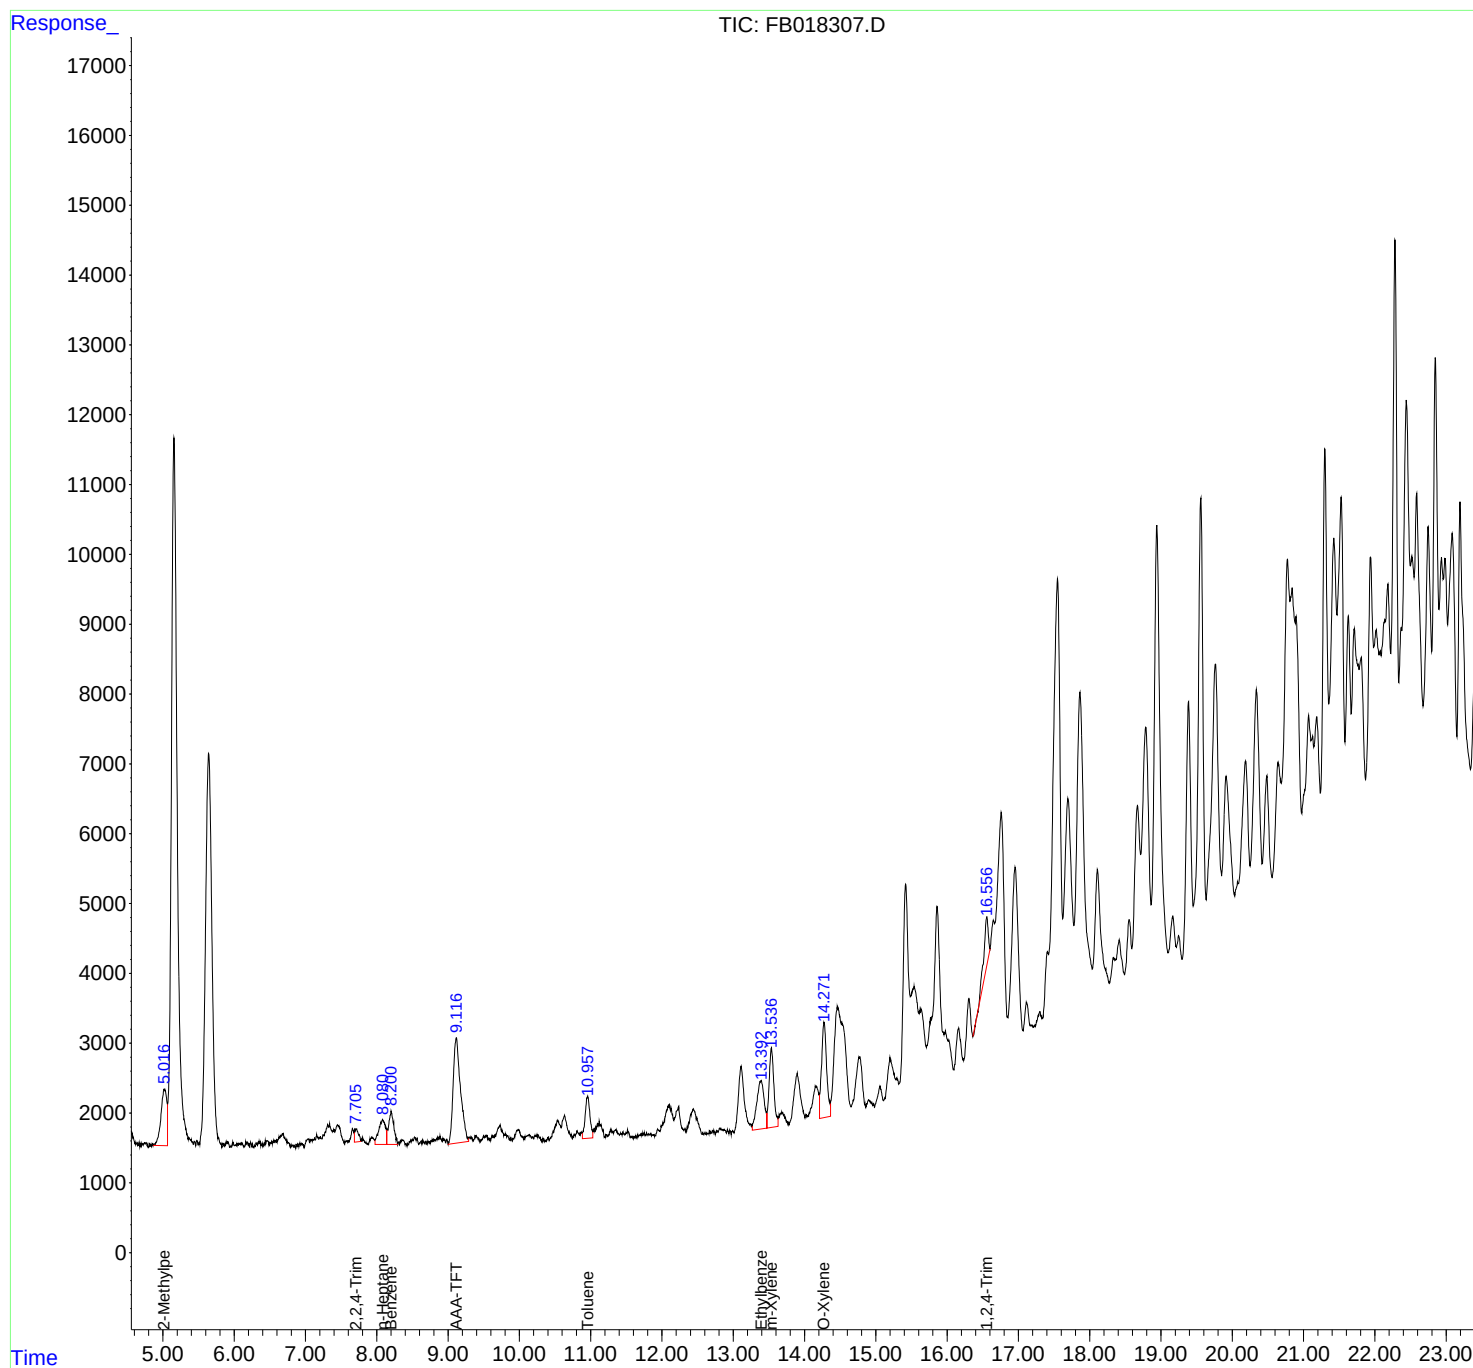

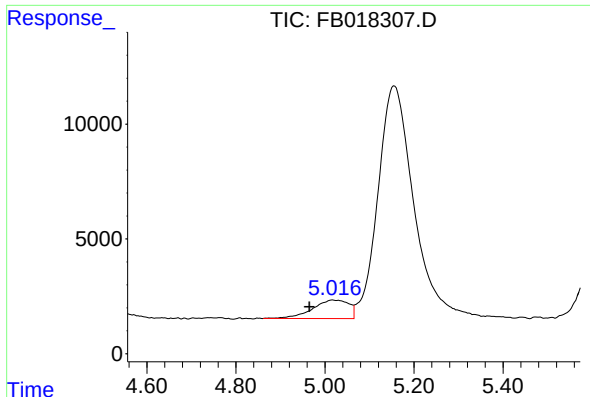


#1 2-Methylpentane

R.T.: 5.017 min
Delta R.T.: 0.052 min
Response: 45974
Conc: 3.01 ng/ml

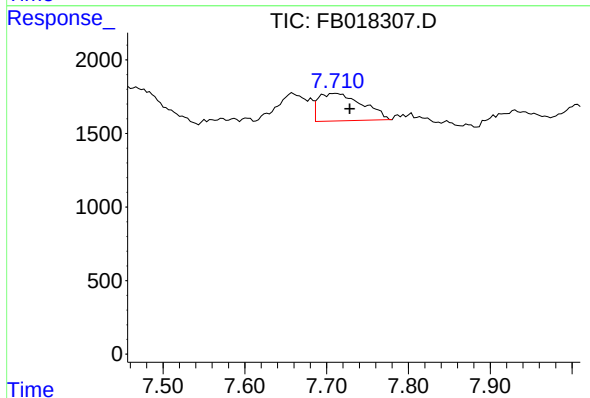


#2 2,2,4-Trimethylpentane

R.T.: 7.711 min
Delta R.T.: -0.017 min
Response: 6938
Conc: 0.47 ng/ml

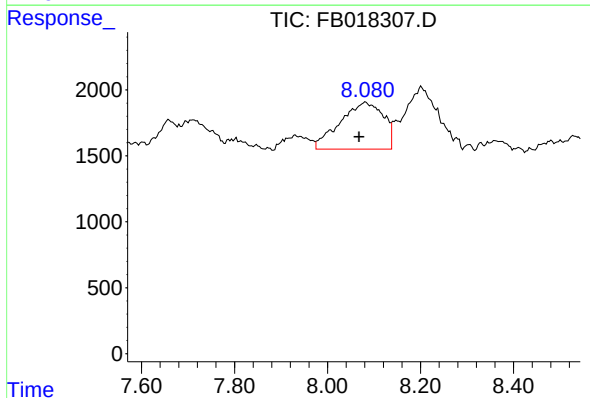


#3 n-Heptane

R.T.: 8.082 min
Delta R.T.: 0.014 min
Response: 22858
Conc: 1.61 ng/ml

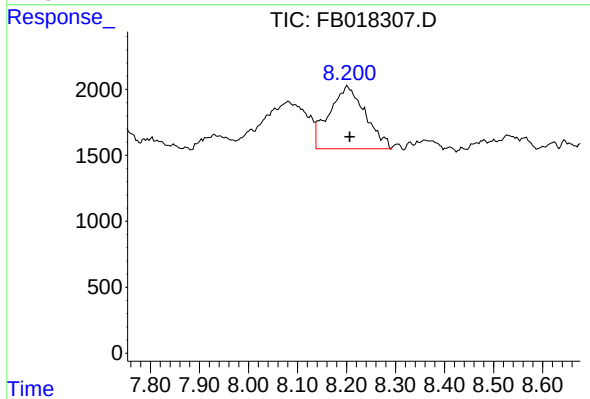


#4 Benzene

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 24347
Conc: 1.31 ng/ml

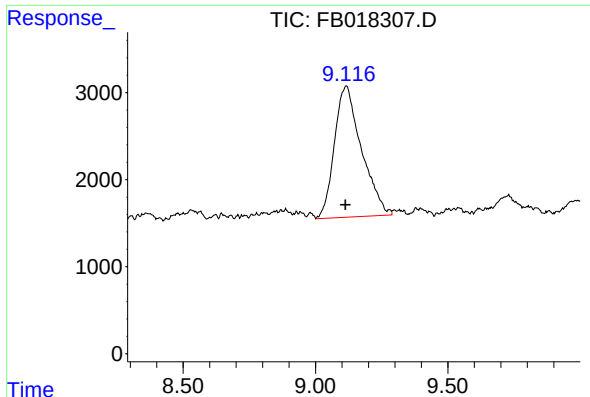


#5 AAA-TFT

R.T.: 9.117 min
Delta R.T.: 0.005 min
Response: 106835
Conc: 12.40 ng/ml

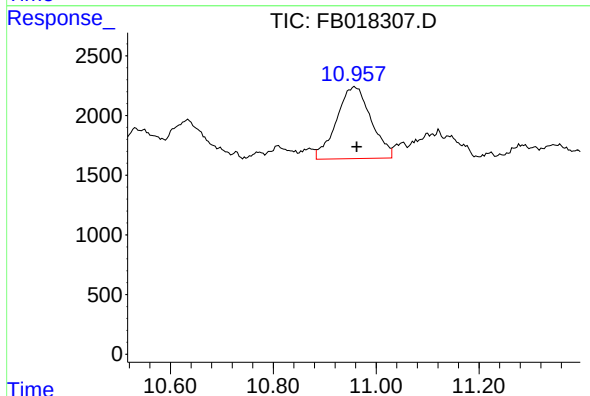


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.004 min
Response: 28006
Conc: 1.84 ng/ml

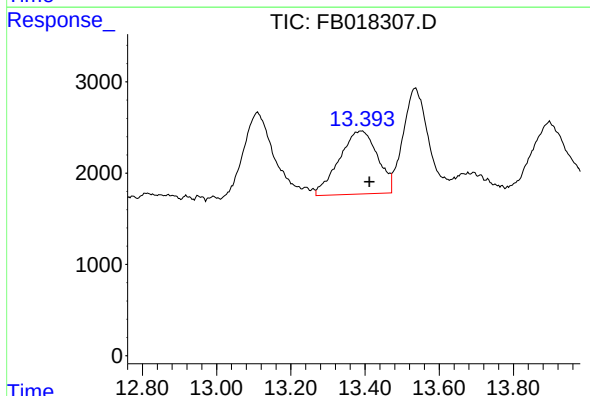


#7 Ethylbenzene

R.T.: 13.391 min
Delta R.T.: -0.021 min
Response: 49680
Conc: 3.13 ng/ml

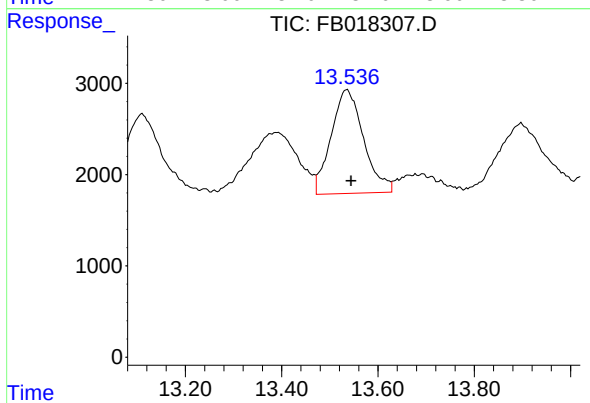


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.009 min
Response: 53190
Conc: 3.20 ng/ml

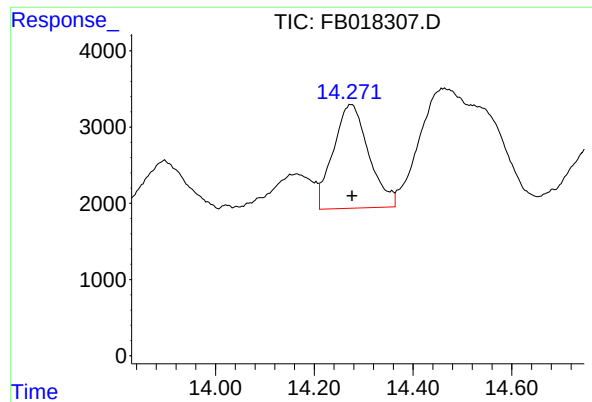

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.002 min
Response: 67891
Conc: 3.81 ng/ml

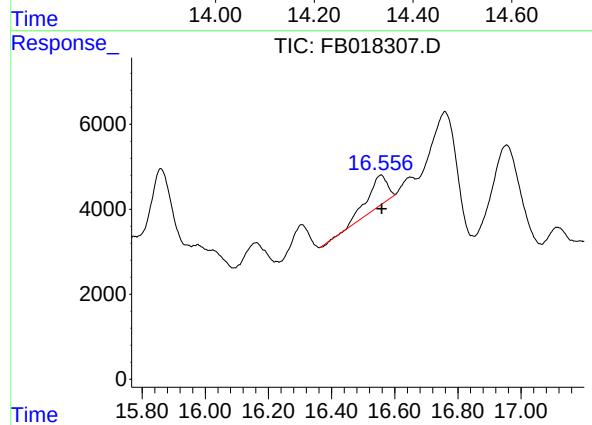

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: -0.003 min
Response: 30822
Conc: 1.52 ng/ml