

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
 Data File : FB018290.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2018 8:57
 Operator : MJ/SJ
 Sample : BSF1022S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 23 08:15:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.100	183915	21.354 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.953	468015	30.601 ng/ml
2) t	2,2,4-Trimethylpentane	7.716	479784	32.469 ng/ml
3) t	n-Heptane	8.056	153069	10.801 ng/ml
4) t	Benzene	8.194	190931	10.249 ng/ml
6) t	Toluene	10.949	495487	32.511 ng/ml
7) t	Ethylbenzene	13.399	178710	11.264 ng/ml
8) t	m-Xylene	13.532	386192	23.210 ng/ml
9) t	O-Xylene	14.264	397666	22.304 ng/ml
10) t	1,2,4-Trimethylbenzene	16.547	437559	21.509 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
Data File : FB018290.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2018 8:57
Operator : MJ/SJ
Sample : BSF1022S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 23 08:15:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

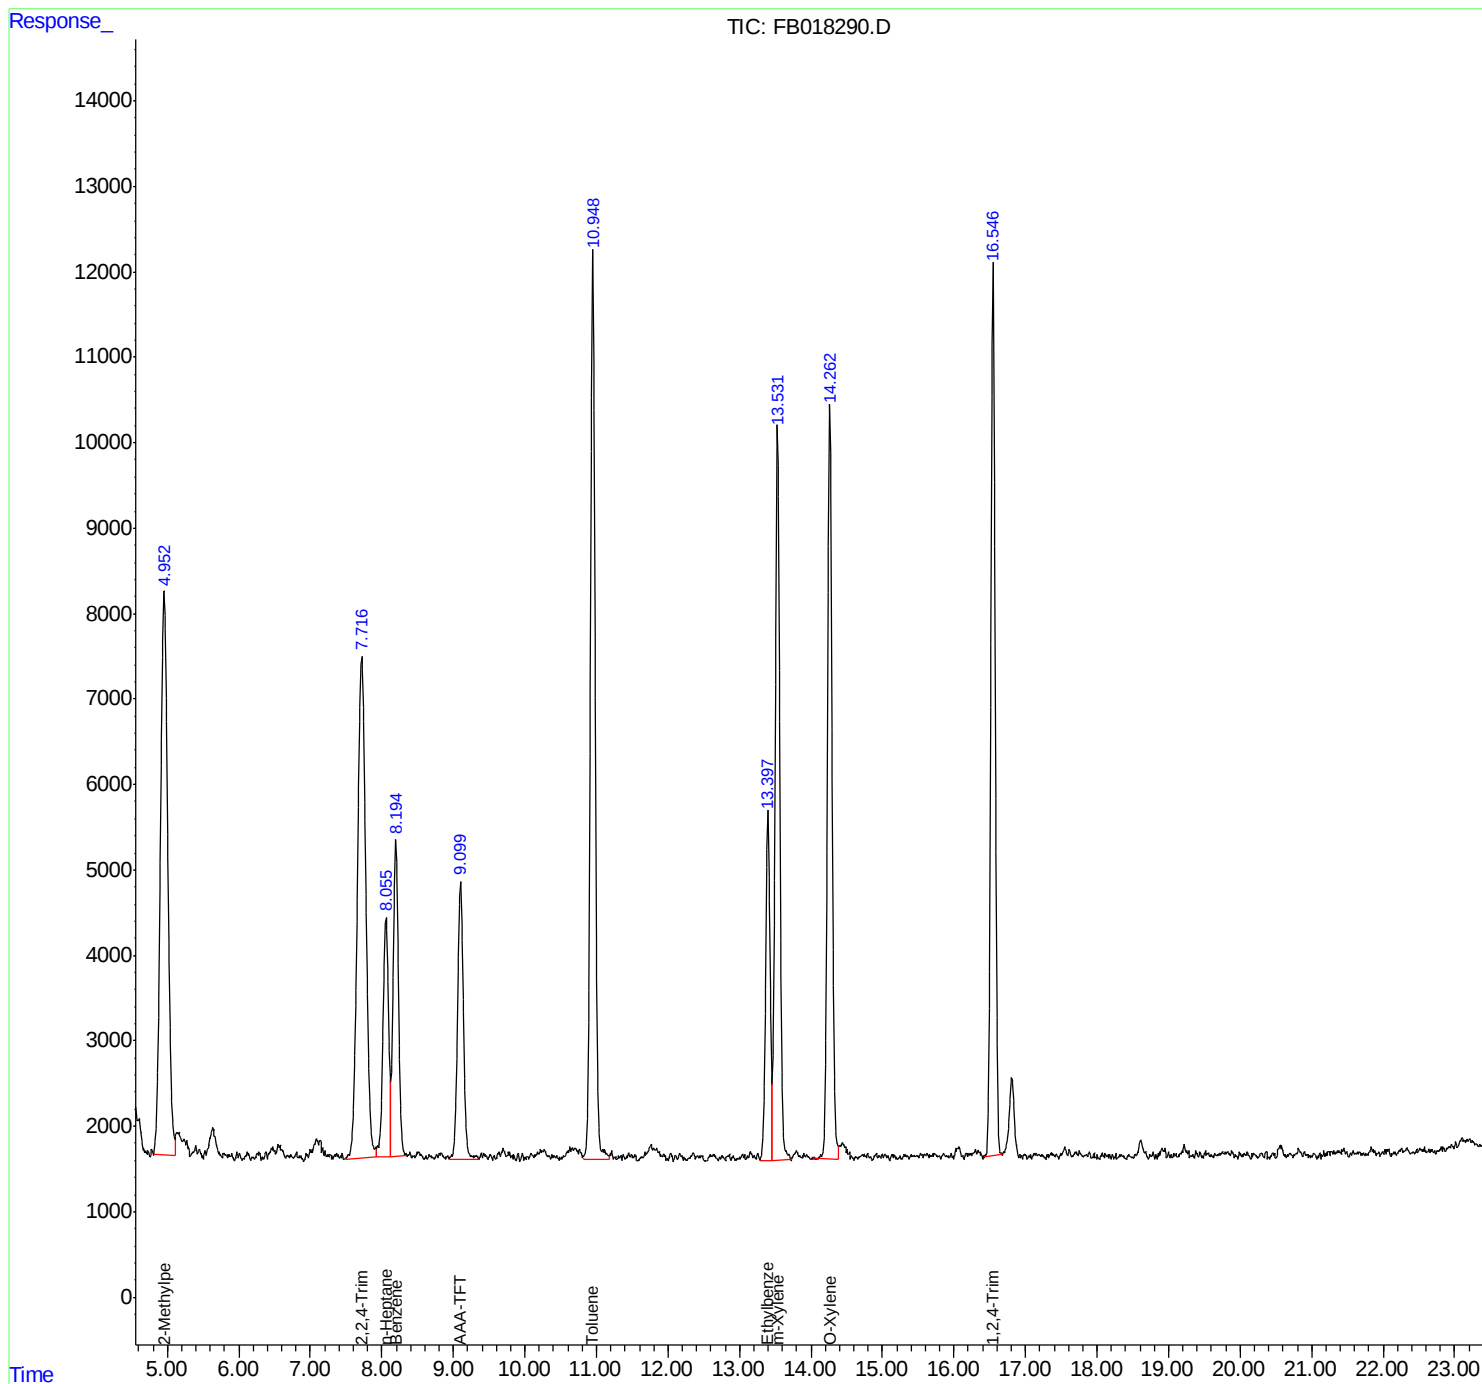

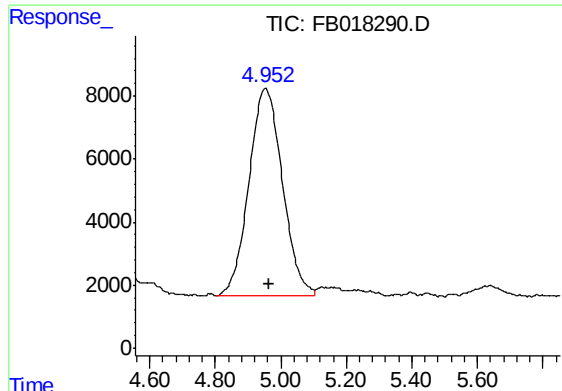


#1 2-Methylpentane

R.T.: 4.953 min
Delta R.T.: -0.012 min
Response: 468015
Conc: 30.60 ng/ml

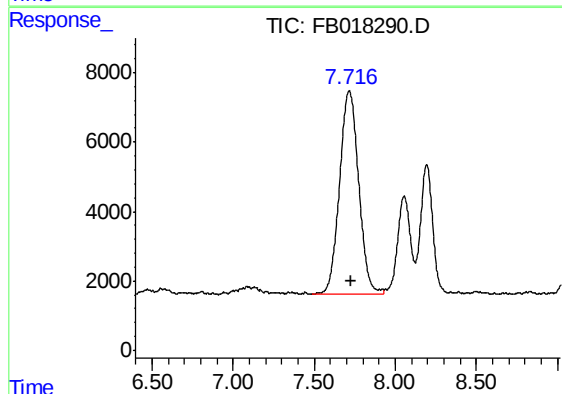


#2 2,2,4-Trimethylpentane

R.T.: 7.716 min
Delta R.T.: -0.012 min
Response: 479784
Conc: 32.47 ng/ml

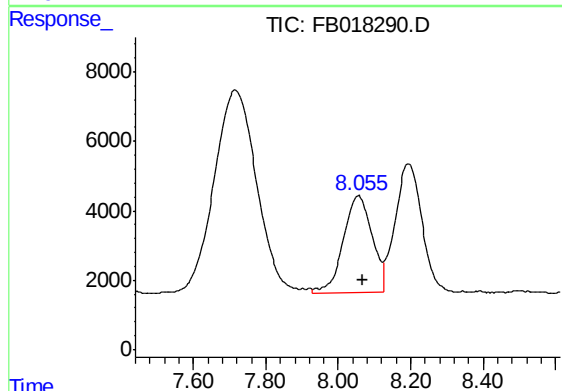


#3 n-Heptane

R.T.: 8.056 min
Delta R.T.: -0.012 min
Response: 153069
Conc: 10.80 ng/ml

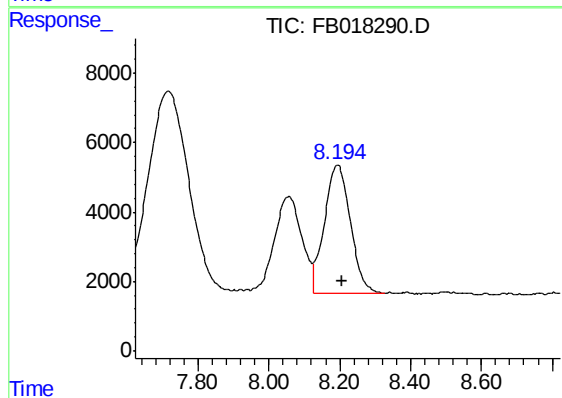


#4 Benzene

R.T.: 8.194 min
Delta R.T.: -0.012 min
Response: 190931
Conc: 10.25 ng/ml

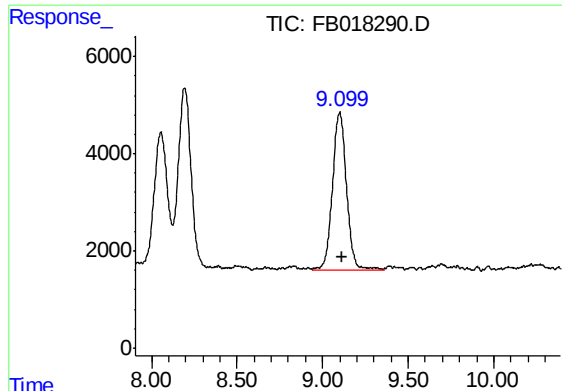


#5 AAA-TFT

R.T.: 9.100 min
Delta R.T.: -0.012 min
Response: 183915
Conc: 21.35 ng/ml

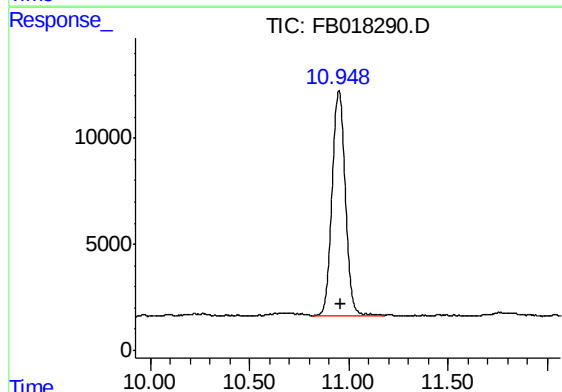


#6 Toluene

R.T.: 10.949 min
Delta R.T.: -0.013 min
Response: 495487
Conc: 32.51 ng/ml

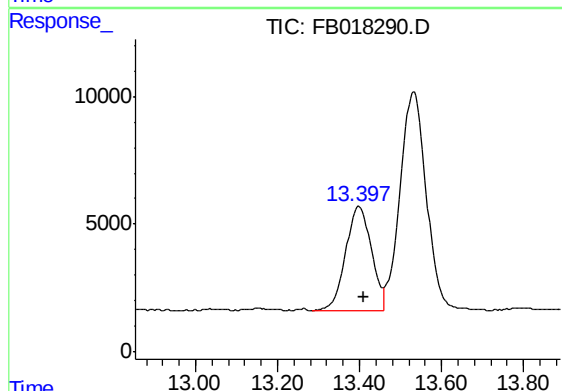


#7 Ethylbenzene

R.T.: 13.399 min
Delta R.T.: -0.013 min
Response: 178710
Conc: 11.26 ng/ml

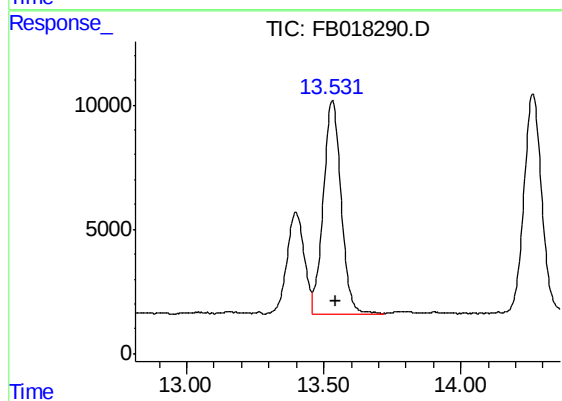


#8 m-Xylene

R.T.: 13.532 min
Delta R.T.: -0.013 min
Response: 386192
Conc: 23.21 ng/ml

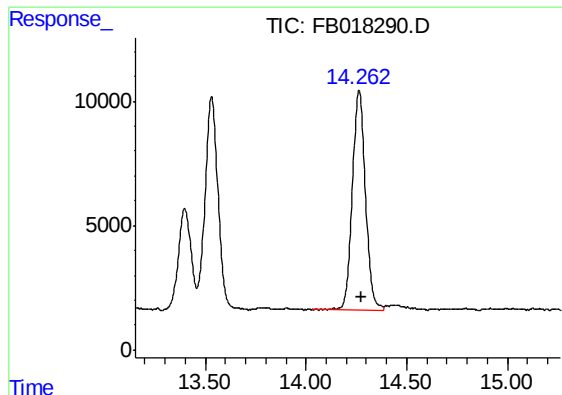

#9 O-Xylene

R.T.: 14.264 min
Delta R.T.: -0.013 min
Response: 397666
Conc: 22.30 ng/ml

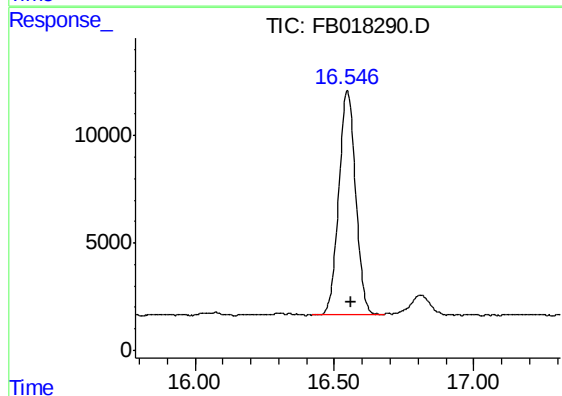

#10 1,2,4-Trimethylbenzene

R.T.: 16.547 min
Delta R.T.: -0.012 min
Response: 437559
Conc: 21.51 ng/ml