

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
 Data File : FB018303.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2018 22:15
 Operator : MJ/SJ
 Sample : J5605-08MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 23 08:16:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	184788	21.455 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	457428	29.908 ng/ml
2) t 2,2,4-Trimethylpentane	7.724	428216	28.979 ng/ml
3) t n-Heptane	8.063	133342	9.409 ng/ml
4) t Benzene	8.202	200643	10.771 ng/ml
6) t Toluene	10.957	482156	31.636 ng/ml
7) t Ethylbenzene	13.407	155884	9.825 ng/ml
8) t m-Xylene	13.539	326776	19.639 ng/ml
9) t O-Xylene	14.271	343327	19.256 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	379166	18.638 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102218\
Data File : FB018303.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2018 22:15
Operator : MJ/SJ
Sample : J5605-08MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 23 08:16:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

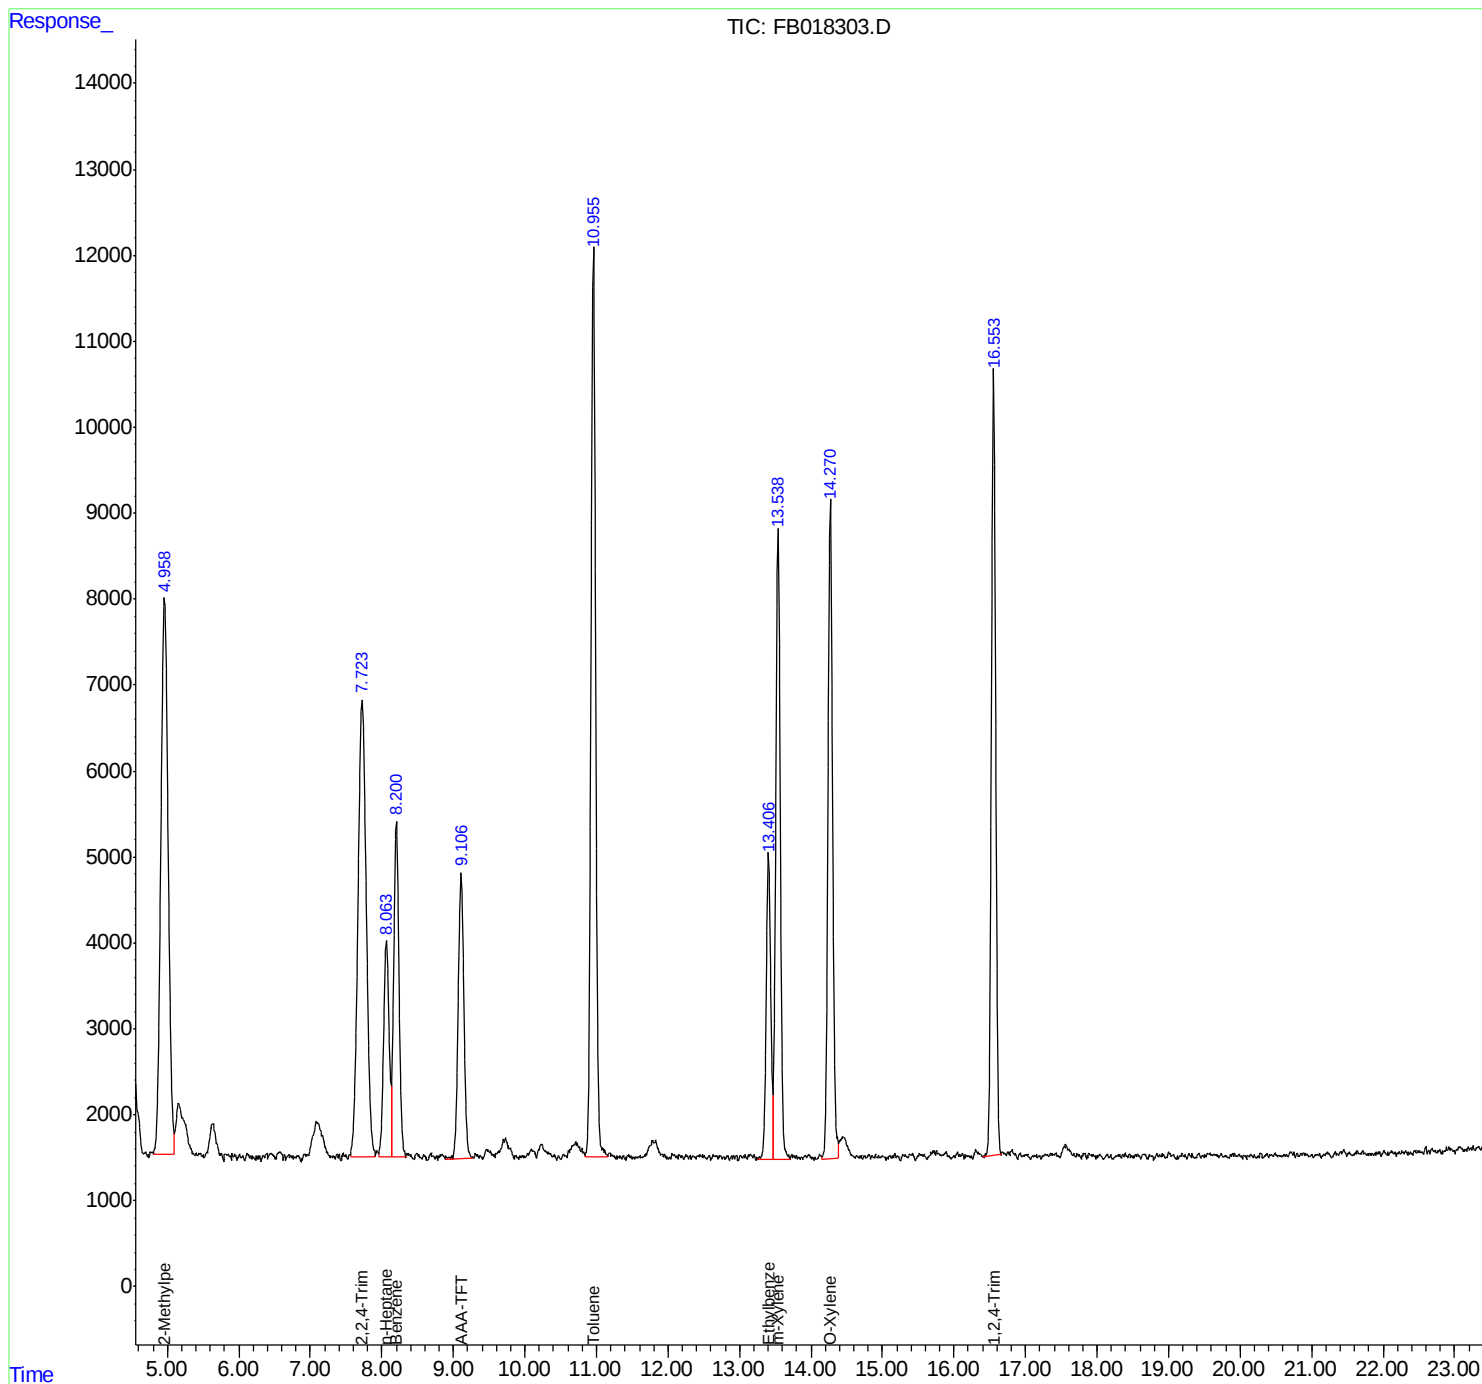

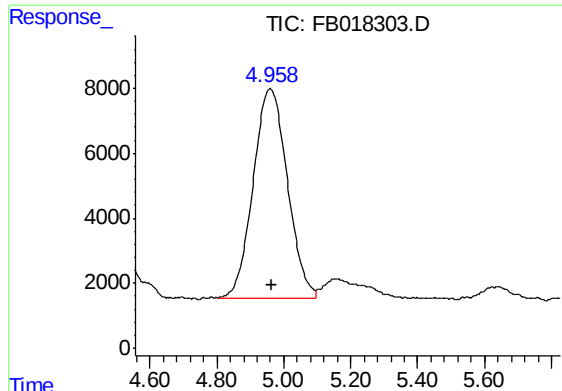


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 457428
Conc: 29.91 ng/ml

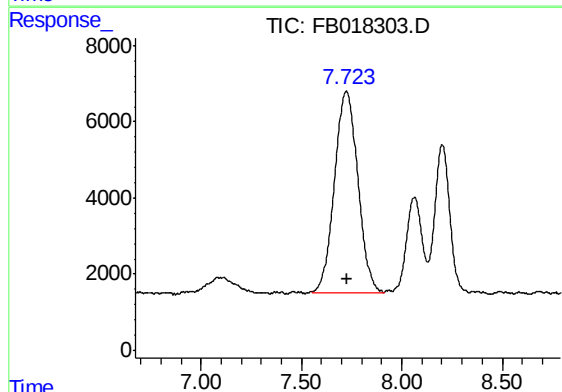


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: -0.004 min
Response: 428216
Conc: 28.98 ng/ml

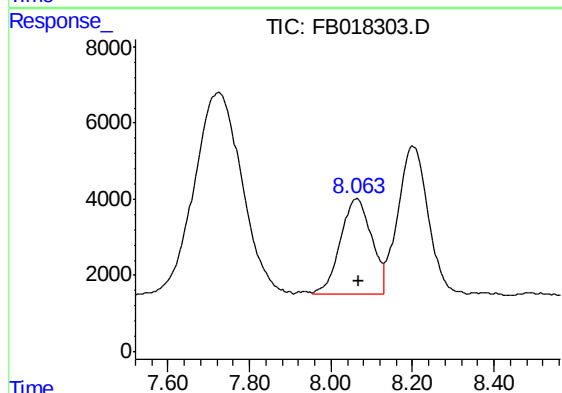


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.004 min
Response: 133342
Conc: 9.41 ng/ml

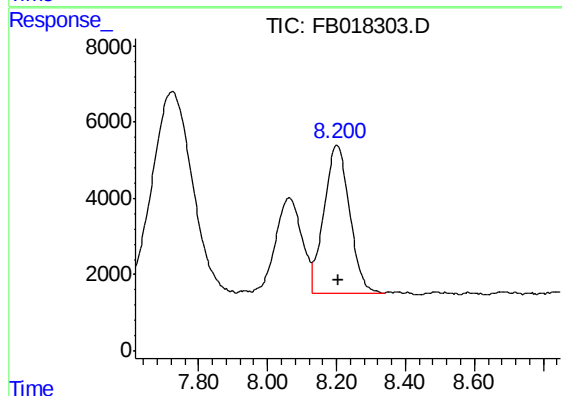


#4 Benzene

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 200643
Conc: 10.77 ng/ml

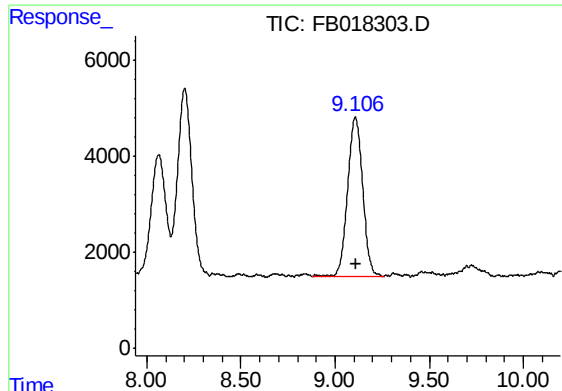


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.006 min
Response: 184788
Conc: 21.45 ng/ml

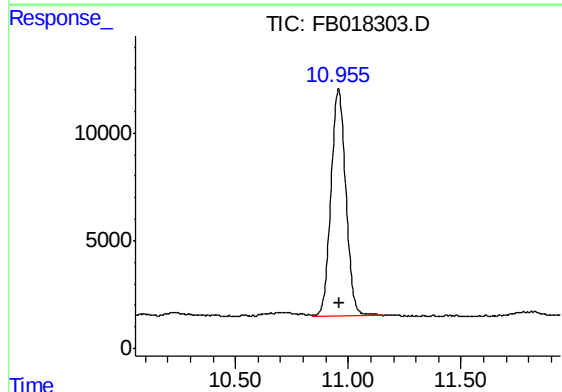


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.005 min
Response: 482156
Conc: 31.64 ng/ml

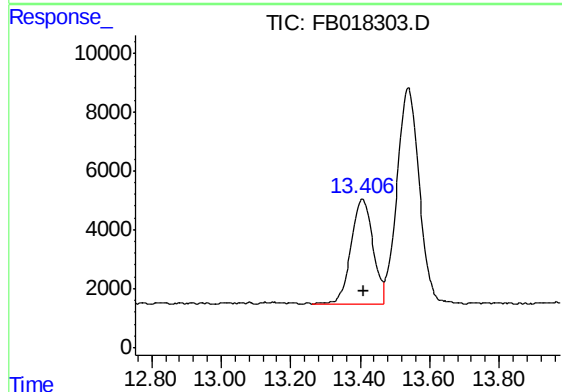


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.005 min
Response: 155884
Conc: 9.83 ng/ml

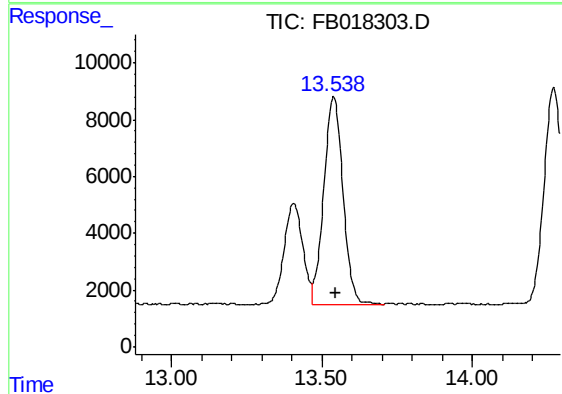


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.005 min
Response: 326776
Conc: 19.64 ng/ml

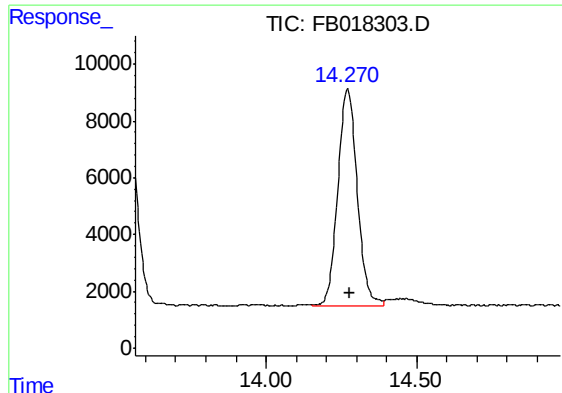

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.005 min
Response: 343327
Conc: 19.26 ng/ml

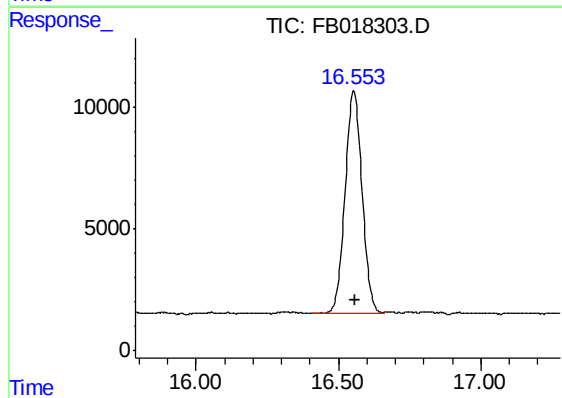

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.005 min
Response: 379166
Conc: 18.64 ng/ml