

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
 Data File : FB025131.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2020 12:14
 Operator : DD/AJ
 Sample : L4225-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-02-102120MSD

Integration File: Calibration.e
 Quant Time: Oct 23 00:38:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	371770	17.415 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	697075	22.919 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	659362	21.166 ng/ml
3) t n-Heptane	7.757	215754	7.017 ng/ml
4) t Benzene	7.891	323469	8.607 ng/ml
6) t Toluene	10.629	888153	24.921 ng/ml
7) t Ethylbenzene	13.069	267327	8.212 ng/ml
8) t m-Xylene	13.202	534153	16.655 ng/ml
9) t O-Xylene	13.930	518658	16.825 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	420268	16.097 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
Data File : FB025131.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2020 12:14
Operator : DD/AJ
Sample : L4225-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-02-102120MSD

Integration File: Calibration.e
Quant Time: Oct 23 00:38:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

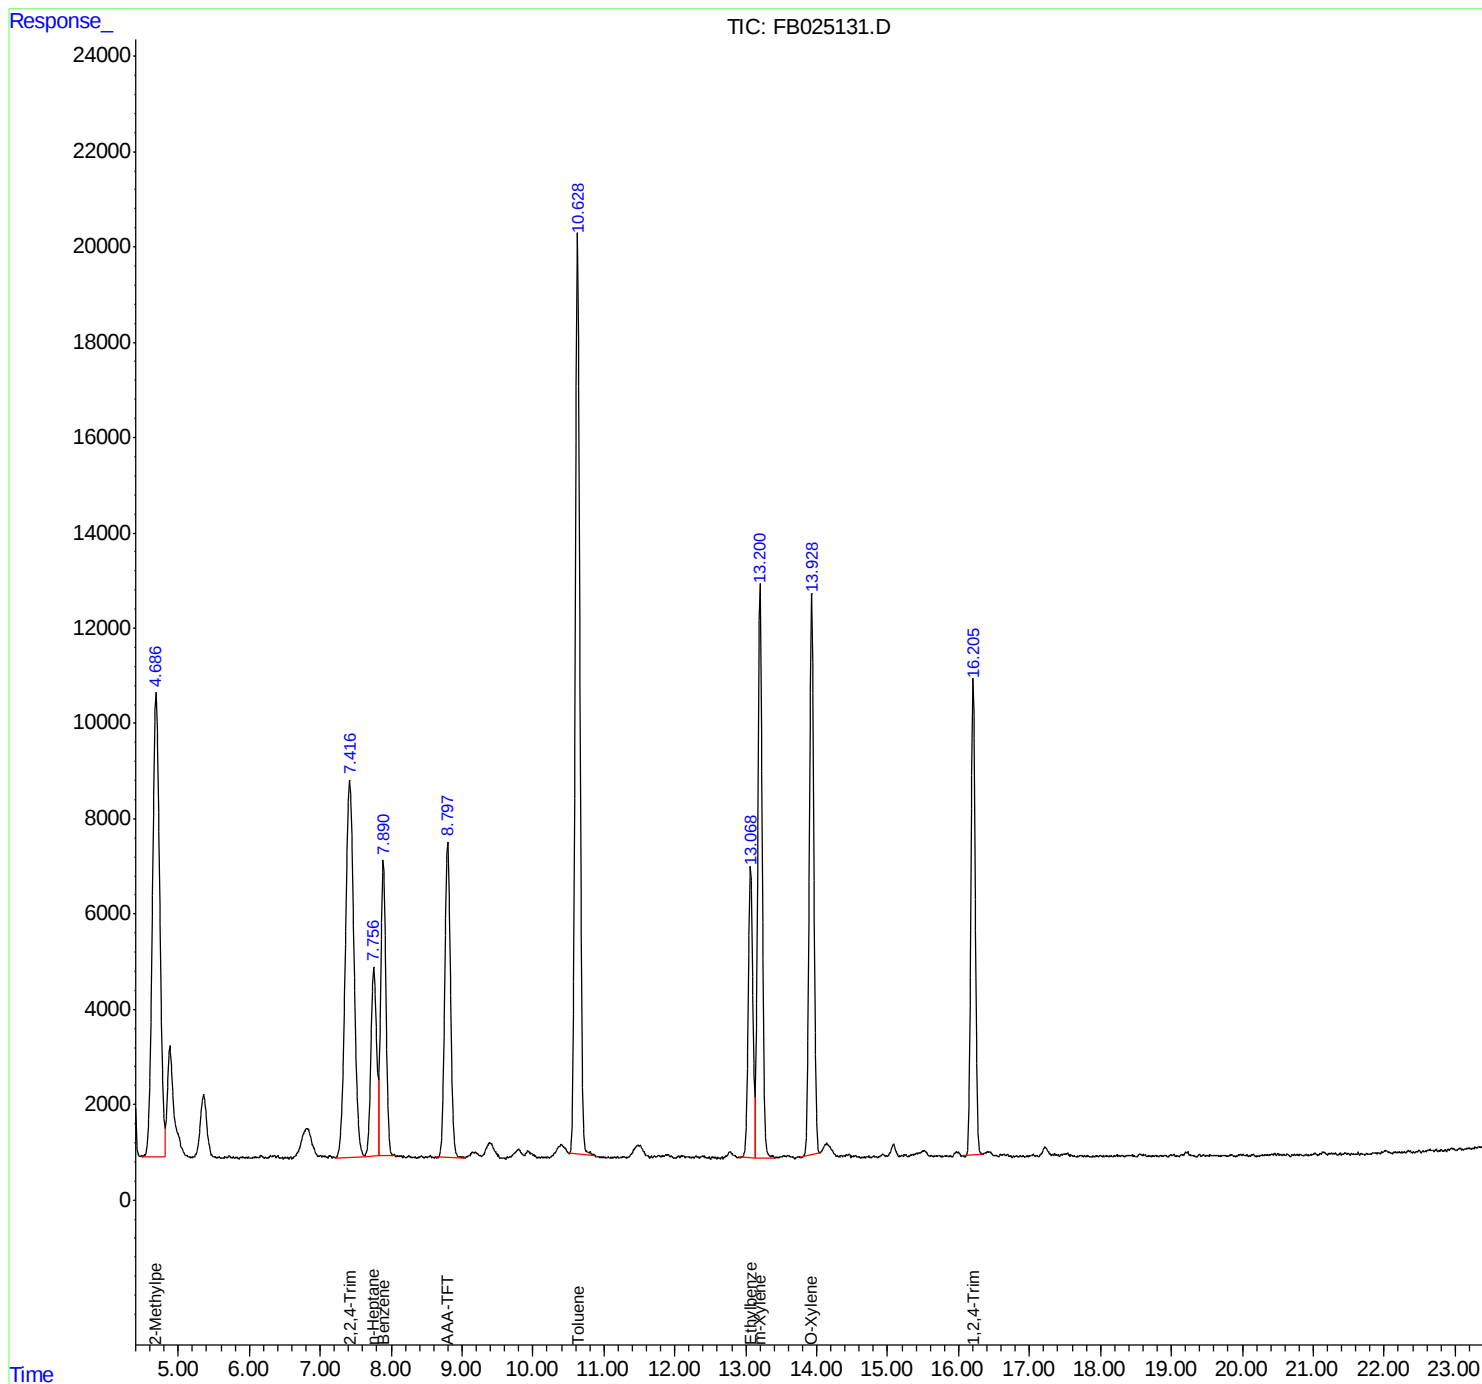


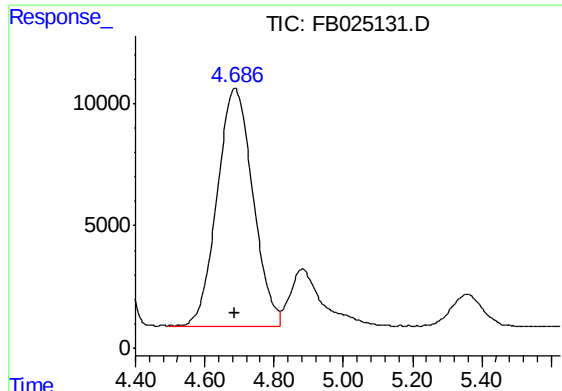

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 697075
Conc: 22.92 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MSD

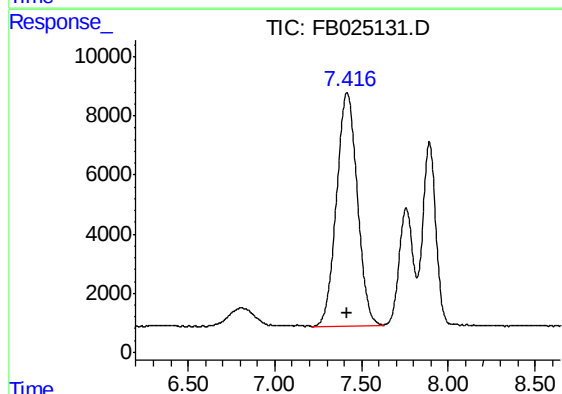


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 659362
Conc: 21.17 ng/ml

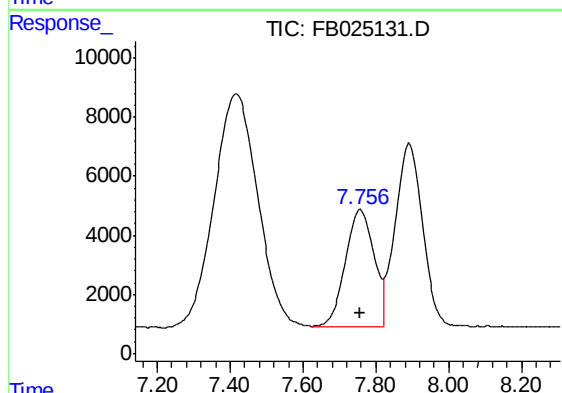


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 215754
Conc: 7.02 ng/ml

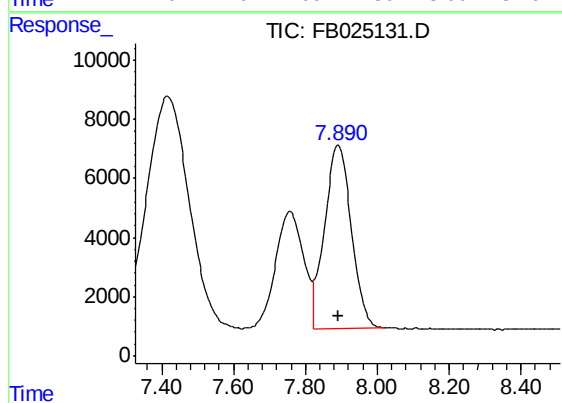

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 323469
Conc: 8.61 ng/ml

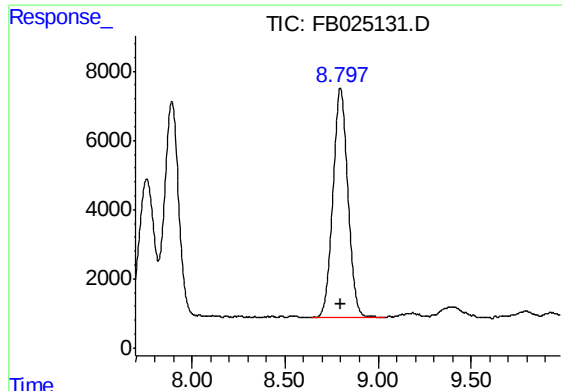

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 371770
Conc: 17.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MSD

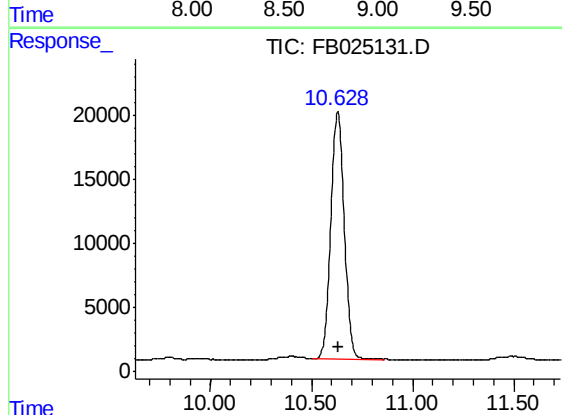


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 888153
Conc: 24.92 ng/ml

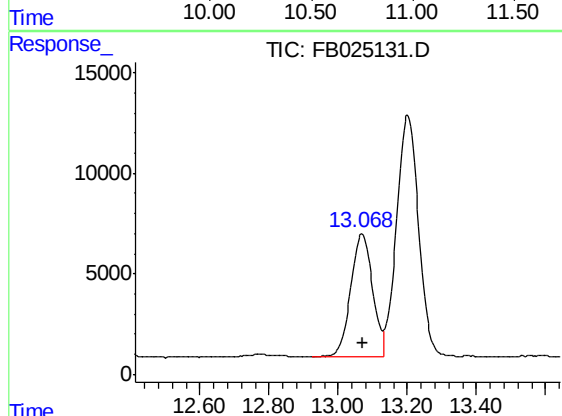


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 267327
Conc: 8.21 ng/ml

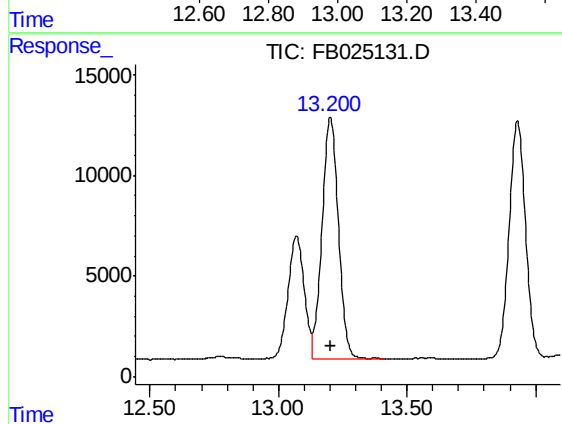

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 534153
Conc: 16.66 ng/ml

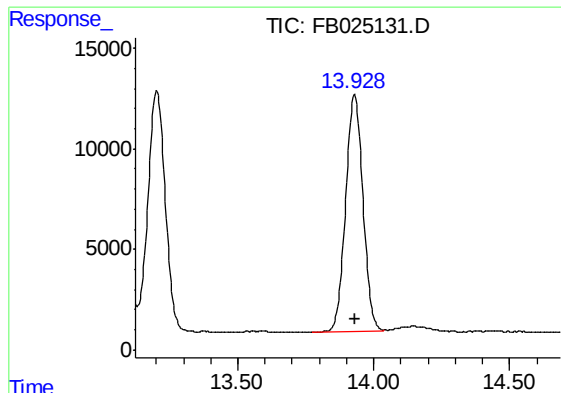

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 518658
Conc: 16.82 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MSD

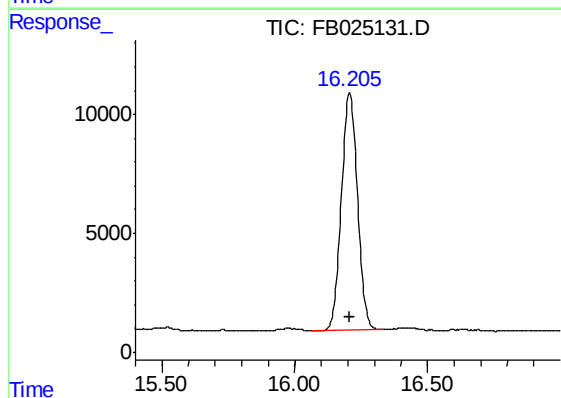

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.001 min
Response: 420268
Conc: 16.10 ng/ml