

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
 Data File : FB025128.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2020 10:42
 Operator : DD/AJ
 Sample : BSF1022S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1022S1

Integration File: Calibration.e
 Quant Time: Oct 23 00:37:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	408122	19.118 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	887928	29.194 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	939151	30.147 ng/ml
3) t n-Heptane	7.757	309366	10.062 ng/ml
4) t Benzene	7.892	364559	9.700 ng/ml
6) t Toluene	10.630	1041602	29.227 ng/ml
7) t Ethylbenzene	13.069	320840	9.856 ng/ml
8) t m-Xylene	13.203	632441	19.720 ng/ml
9) t O-Xylene	13.930	602846	19.556 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	514946	19.723 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
Data File : FB025128.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2020 10:42
Operator : DD/AJ
Sample : BSF1022S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1022S1

Integration File: Calibration.e
Quant Time: Oct 23 00:37:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

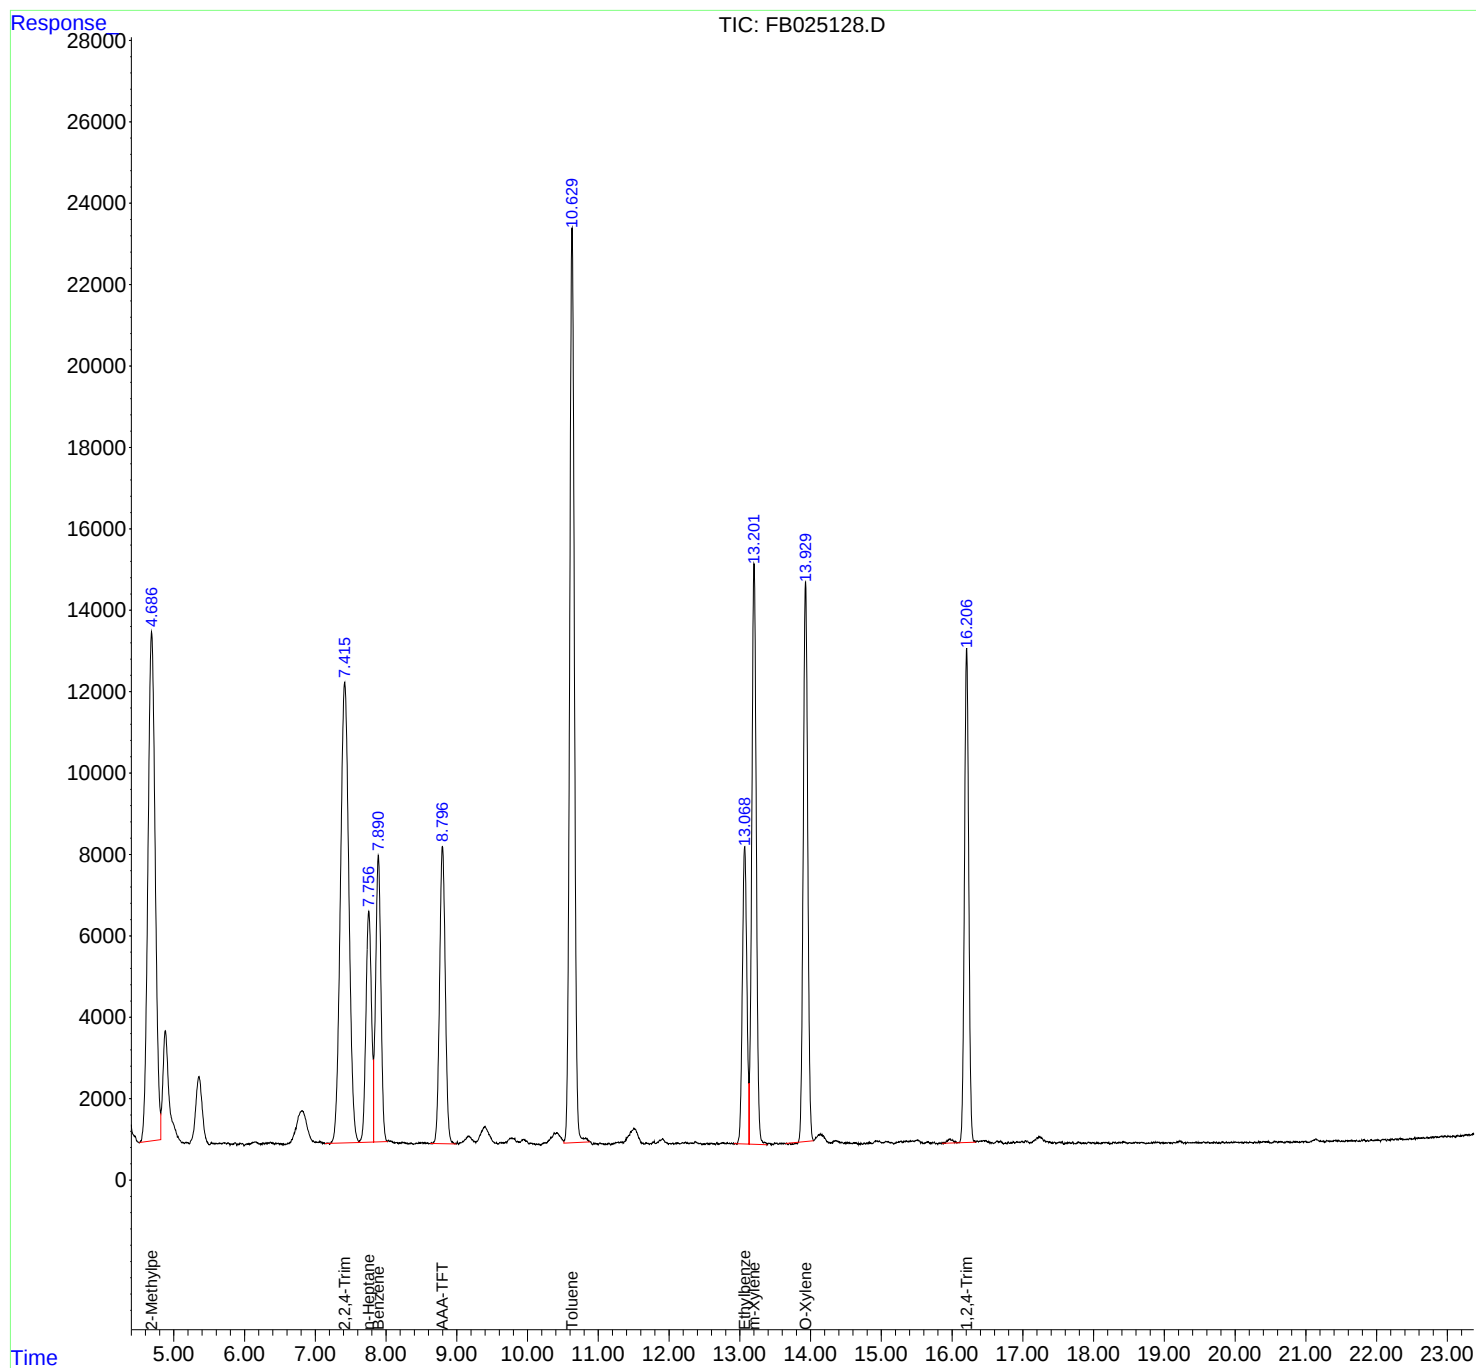


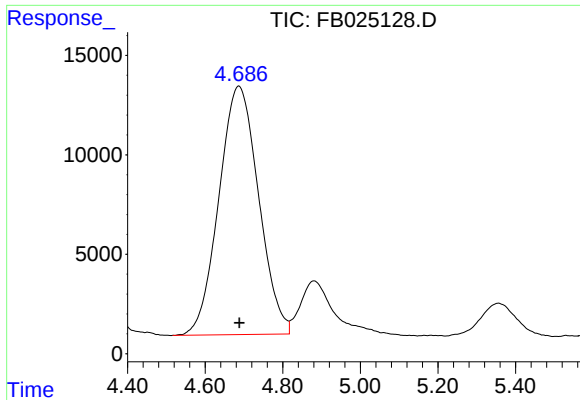

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 887928
Conc: 29.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1022S1

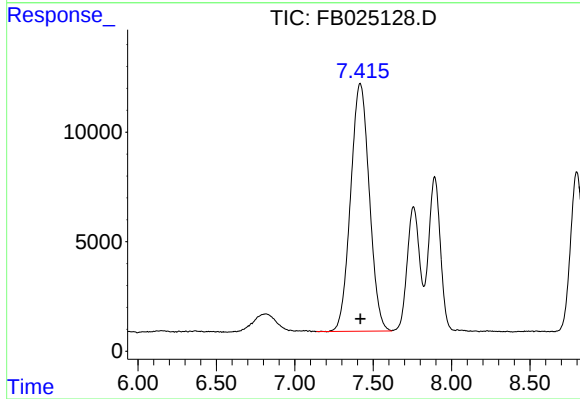


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 939151
Conc: 30.15 ng/ml

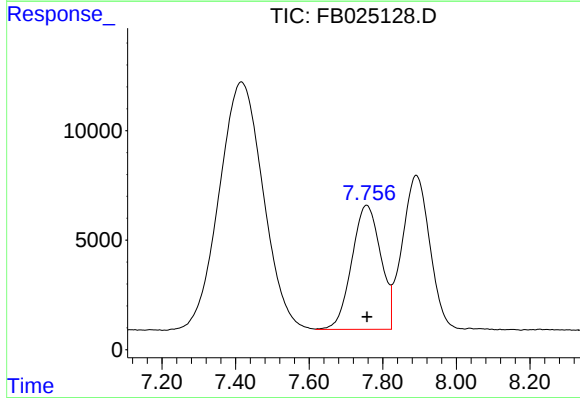


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 309366
Conc: 10.06 ng/ml

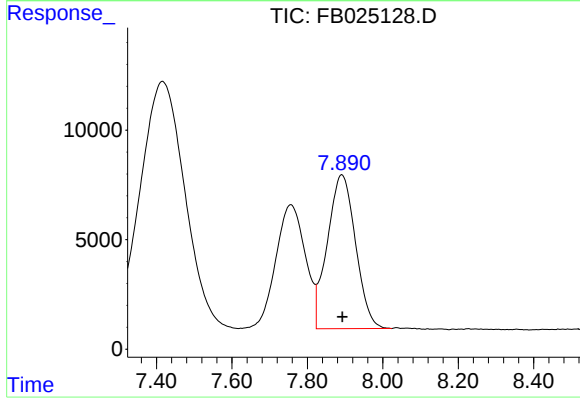

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 364559
Conc: 9.70 ng/ml

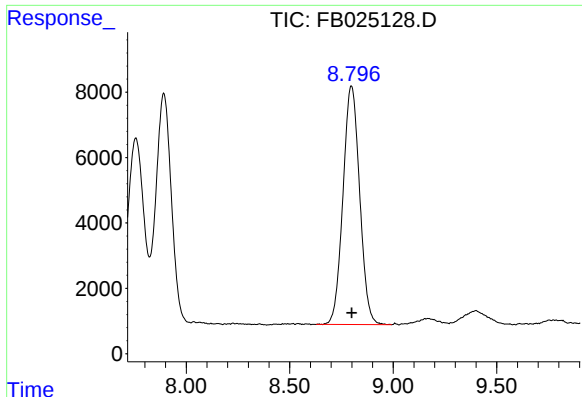

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 408122
Conc: 19.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1022S1

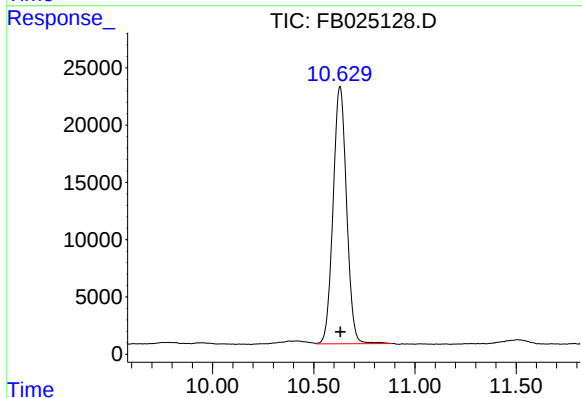


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1041602
Conc: 29.23 ng/ml

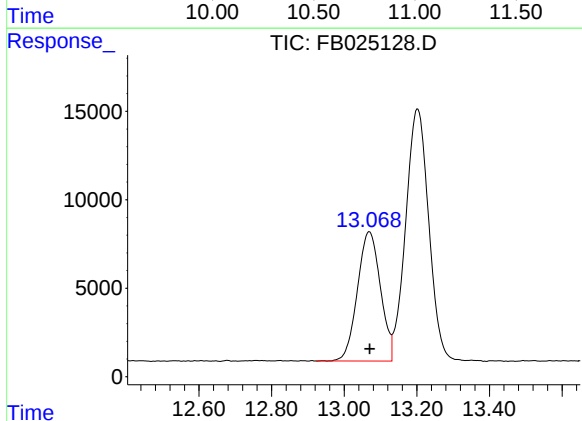


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 320840
Conc: 9.86 ng/ml

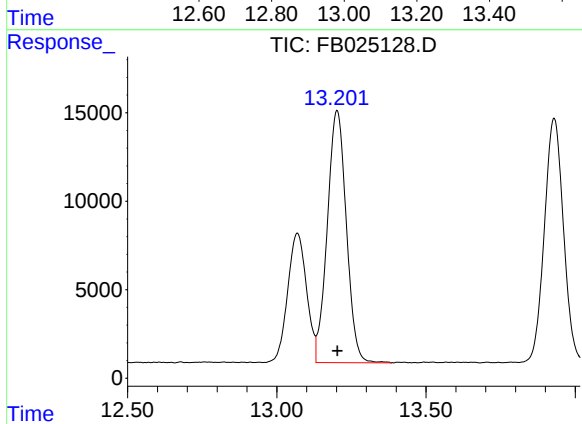

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 632441
Conc: 19.72 ng/ml

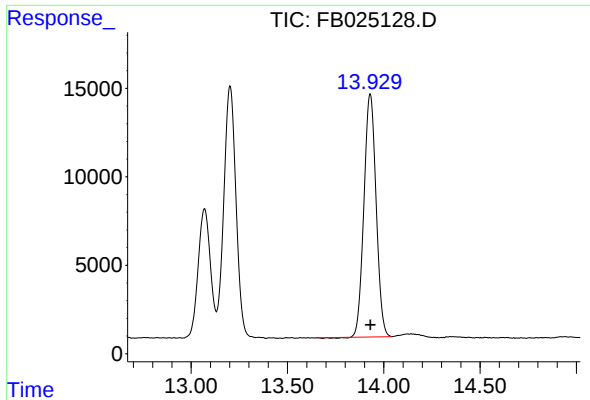

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 602846
Conc: 19.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1022S1

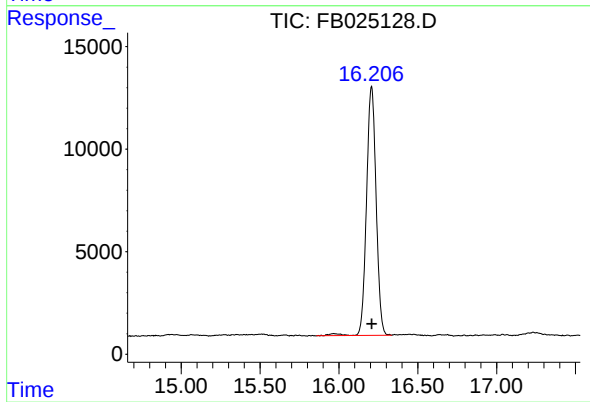

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.001 min
Response: 514946
Conc: 19.72 ng/ml