

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
 Data File : FB025130.D
 Signal(s) : FID2B.CH
 Acq On : 22 Oct 2020 11:43
 Operator : DD/AJ
 Sample : L4225-11MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-02-102120MS

Integration File: Calibration.e
 Quant Time: Oct 23 00:38:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	405295	18.985 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	831817	27.349 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	796599	25.571 ng/ml
3) t n-Heptane	7.758	263251	8.562 ng/ml
4) t Benzene	7.892	362349	9.641 ng/ml
6) t Toluene	10.629	989730	27.771 ng/ml
7) t Ethylbenzene	13.069	292456	8.984 ng/ml
8) t m-Xylene	13.202	585589	18.259 ng/ml
9) t O-Xylene	13.930	566742	18.385 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	462106	17.699 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102220\
Data File : FB025130.D
Signal(s) : FID2B.CH
Acq On : 22 Oct 2020 11:43
Operator : DD/AJ
Sample : L4225-11MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-02-102120MS

Integration File: Calibration.e
Quant Time: Oct 23 00:38:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

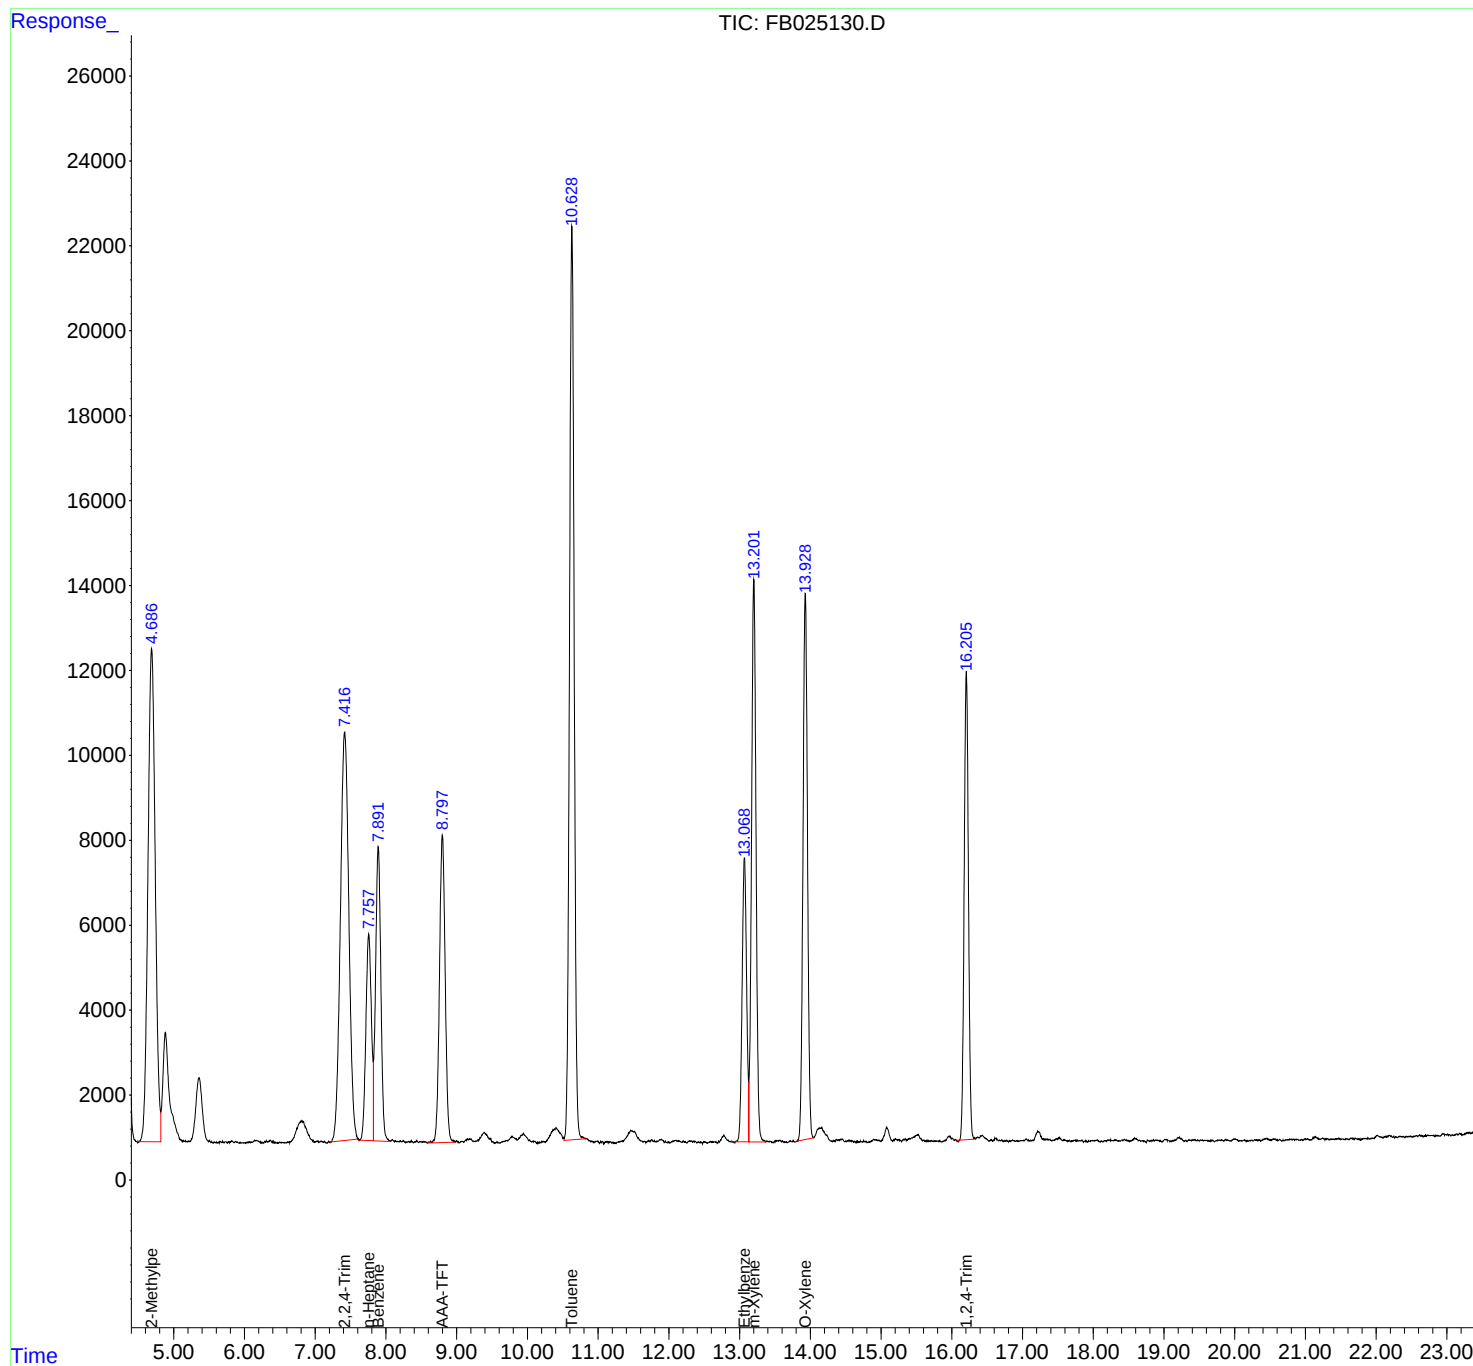


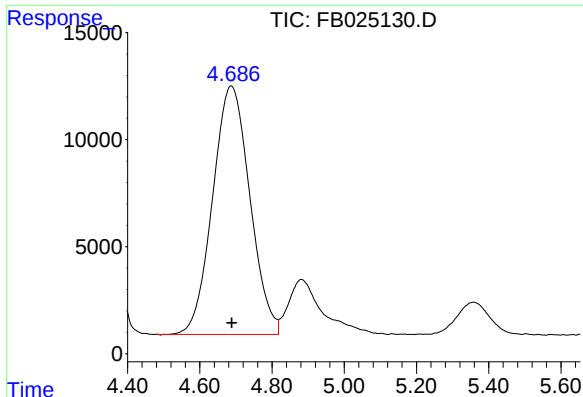

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 831817
Conc: 27.35 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MS

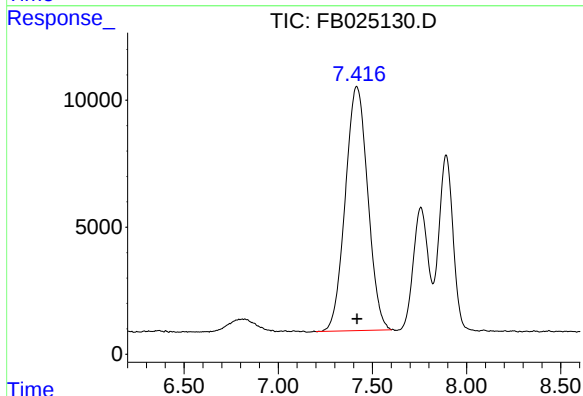


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 796599
Conc: 25.57 ng/ml

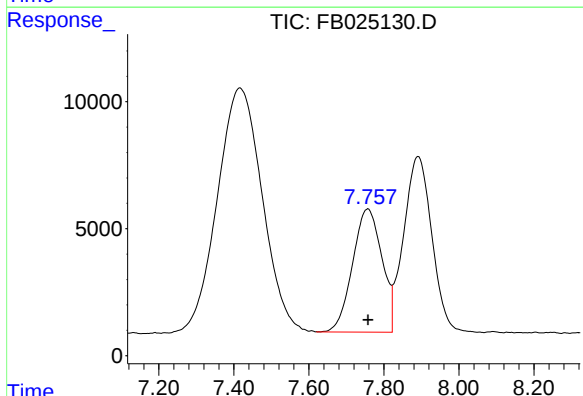


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 263251
Conc: 8.56 ng/ml

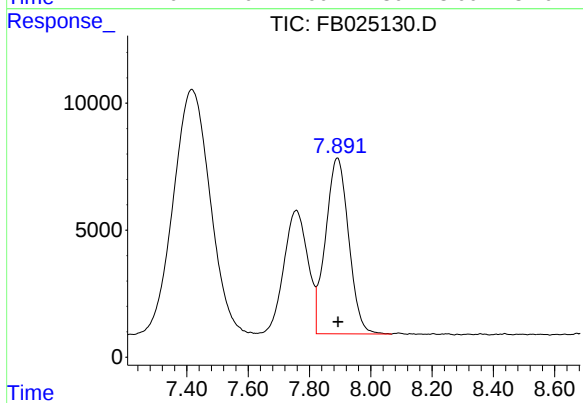

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 362349
Conc: 9.64 ng/ml

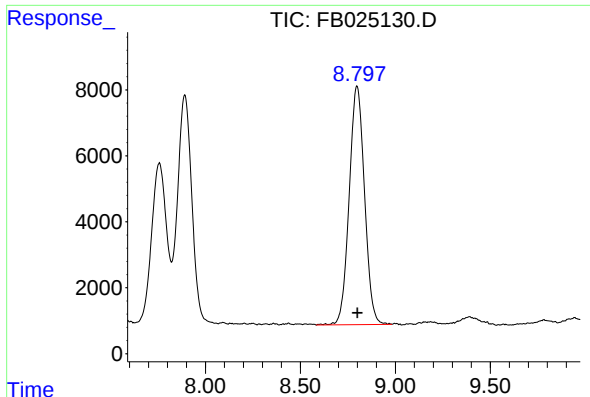

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 405295
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MS

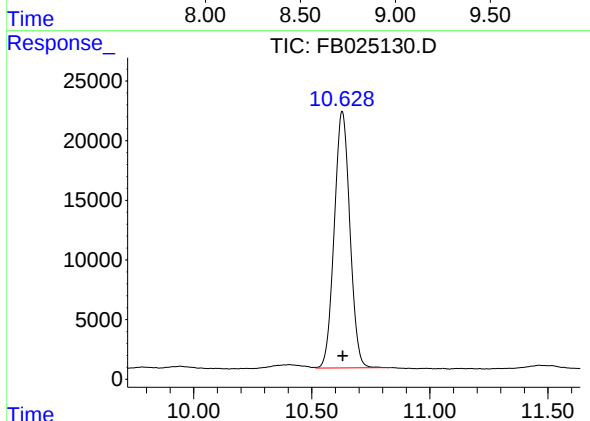


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 989730
Conc: 27.77 ng/ml

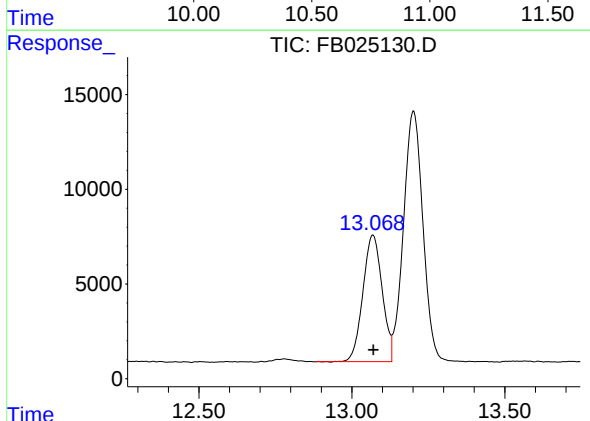


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 292456
Conc: 8.98 ng/ml

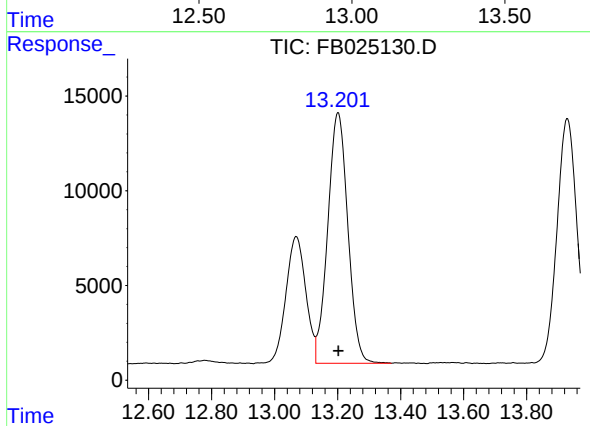

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 585589
Conc: 18.26 ng/ml

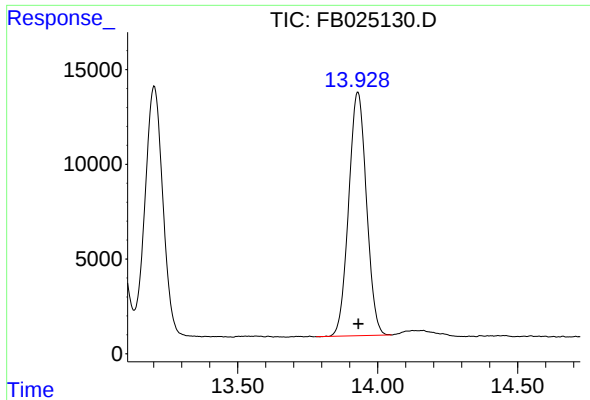

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 566742
Conc: 18.38 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-102120MS

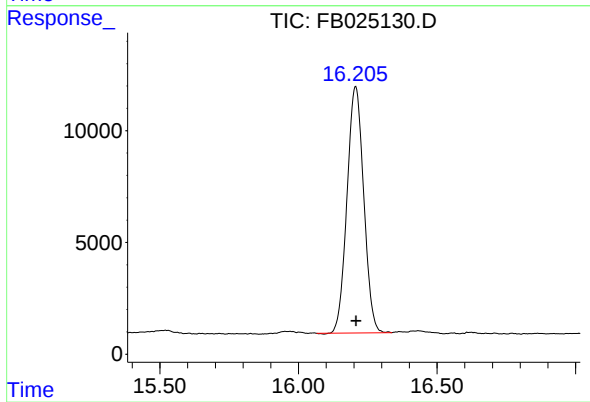

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.002 min
Response: 462106
Conc: 17.70 ng/ml