

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102318\
 Data File : FB018316.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2018 9:54
 Operator : MJ/SJ
 Sample : BSF1023S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 08:36:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	181980	21.129 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	476114	31.130 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	495644	33.543 ng/ml
3) t n-Heptane	8.064	163792	11.558 ng/ml
4) t Benzene	8.204	204341	10.969 ng/ml
6) t Toluene	10.958	486039	31.891 ng/ml
7) t Ethylbenzene	13.408	169393	10.677 ng/ml
8) t m-Xylene	13.541	362220	21.769 ng/ml
9) t O-Xylene	14.273	381682	21.407 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	447359	21.990 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102318\
Data File : FB018316.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2018 9:54
Operator : MJ/SJ
Sample : BSF1023S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 08:36:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

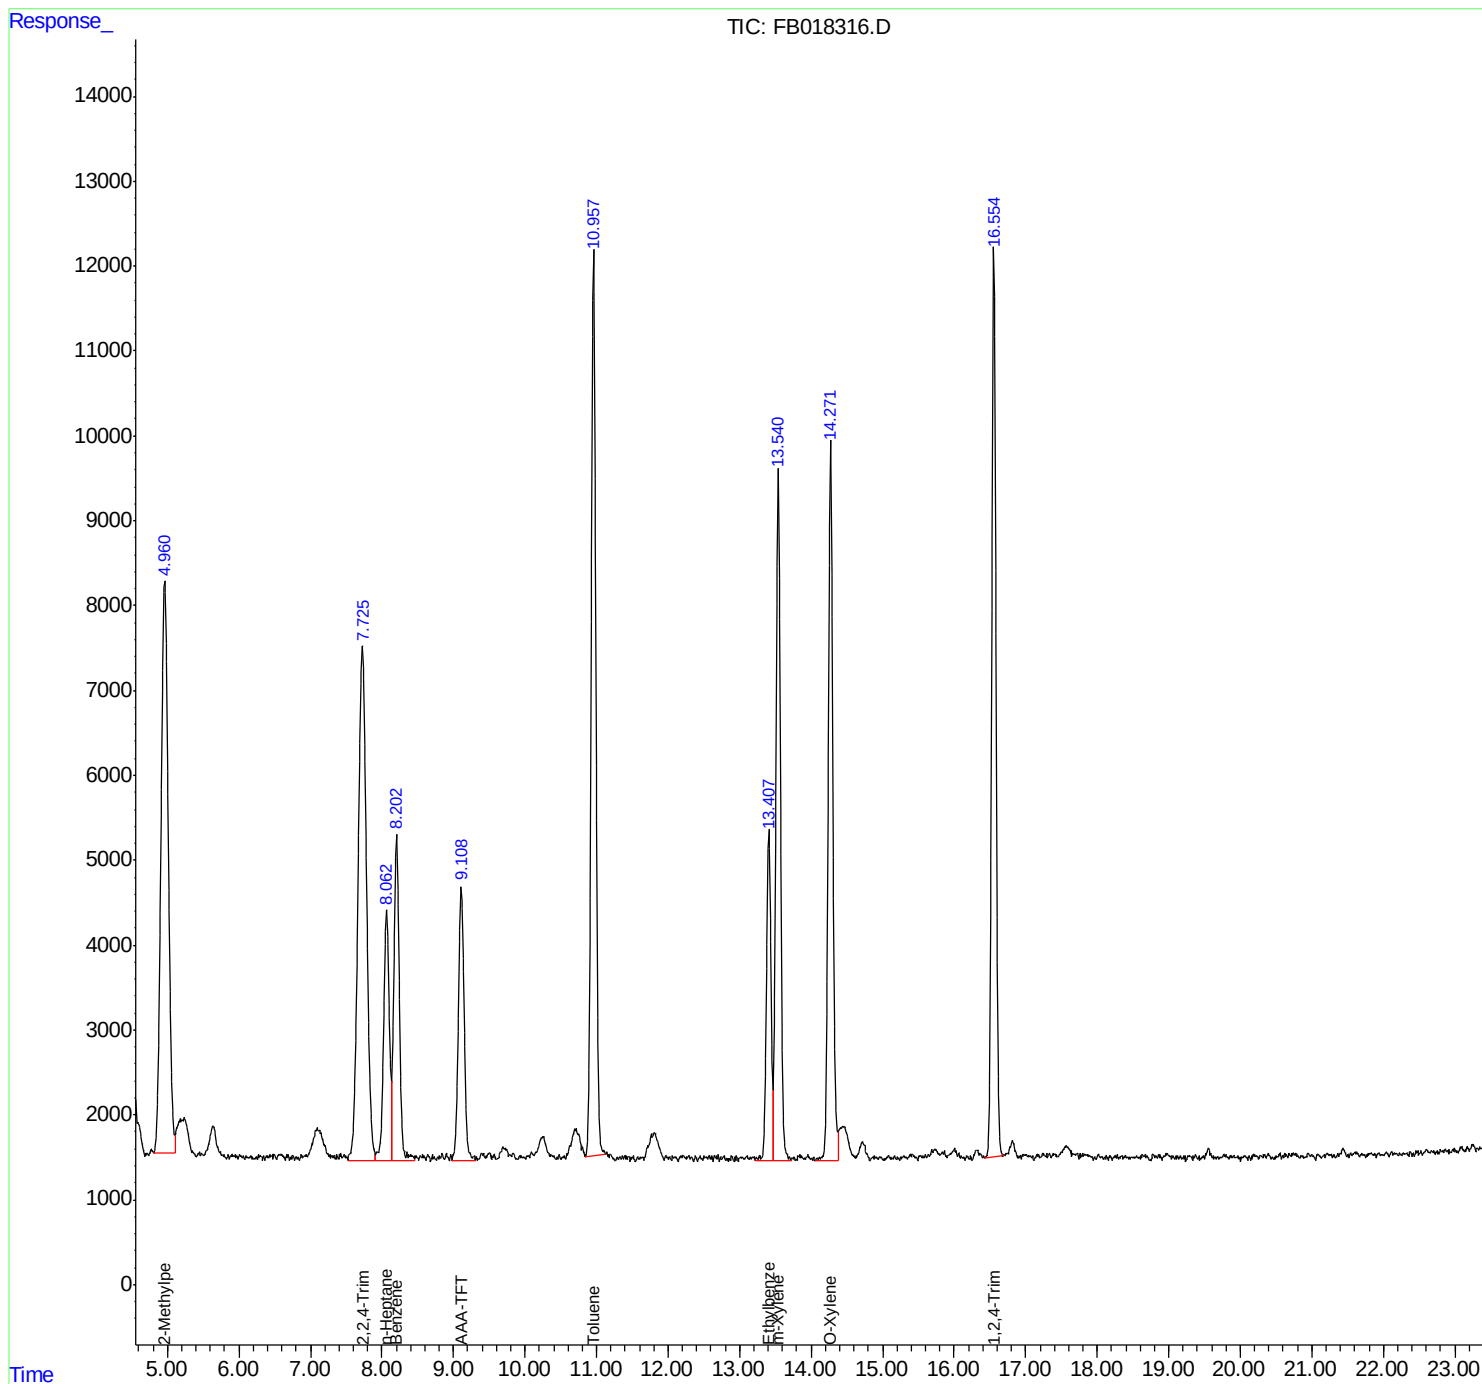

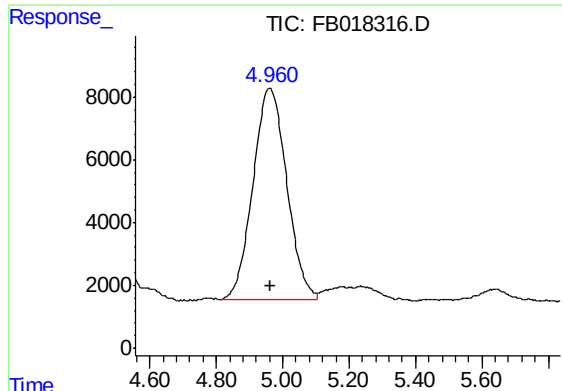


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 476114
Conc: 31.13 ng/ml

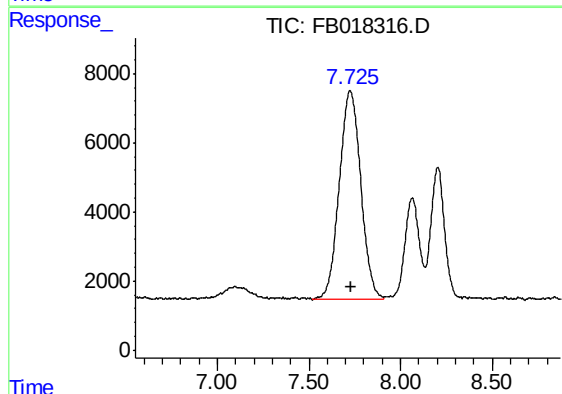


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.003 min
Response: 495644
Conc: 33.54 ng/ml

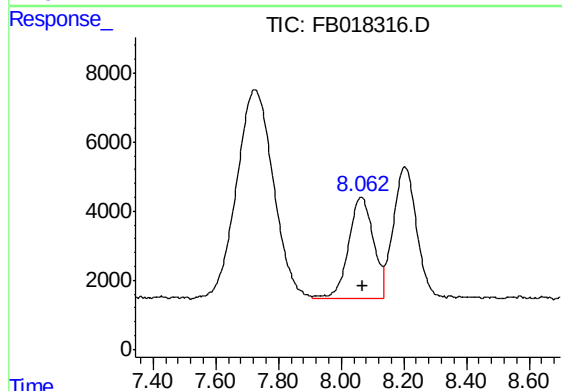


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.003 min
Response: 163792
Conc: 11.56 ng/ml

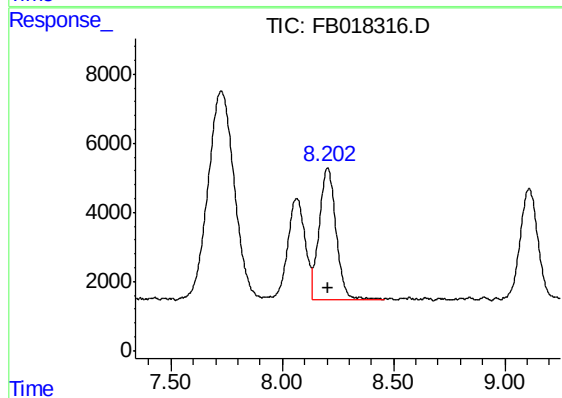


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 204341
Conc: 10.97 ng/ml

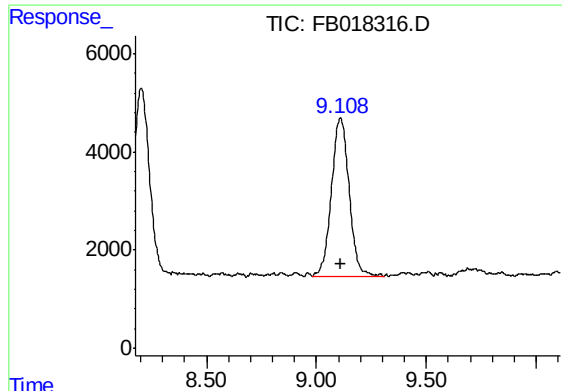


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.003 min
Response: 181980
Conc: 21.13 ng/ml

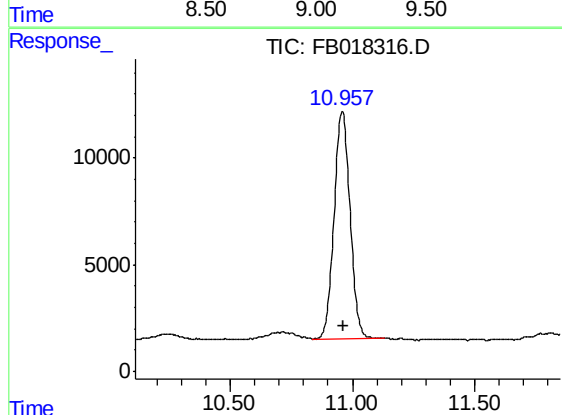


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.004 min
Response: 486039
Conc: 31.89 ng/ml

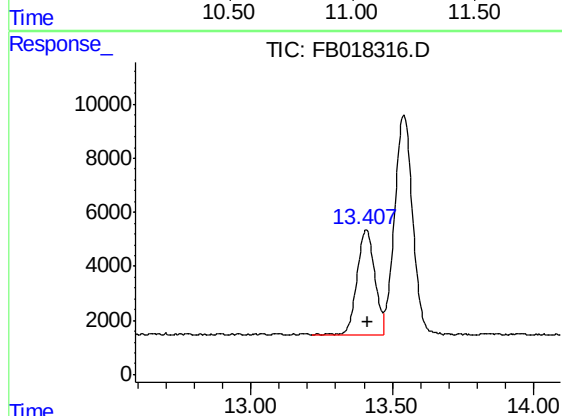


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.004 min
Response: 169393
Conc: 10.68 ng/ml

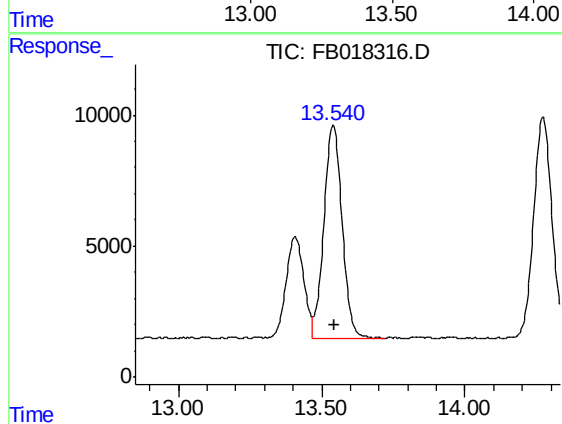


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.004 min
Response: 362220
Conc: 21.77 ng/ml

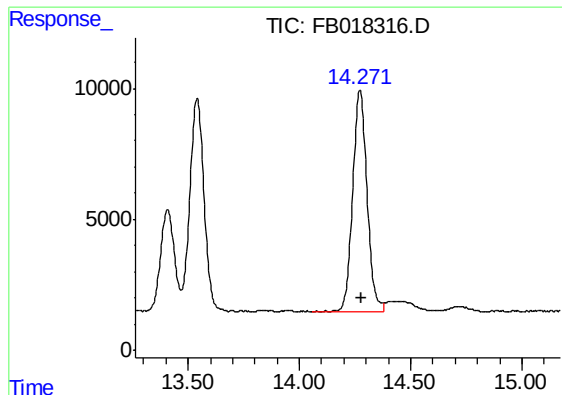

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.004 min
Response: 381682
Conc: 21.41 ng/ml

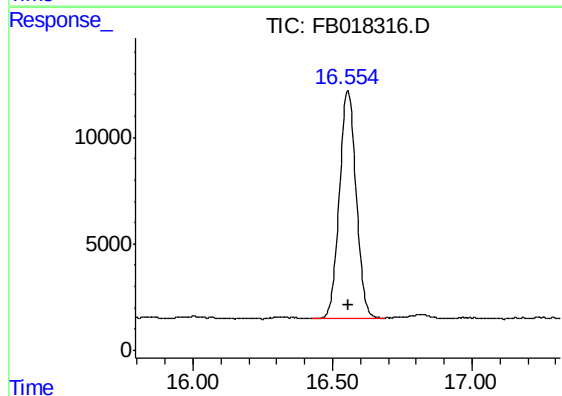

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.004 min
Response: 447359
Conc: 21.99 ng/ml