

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
 Data File : FB022810.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2019 16:39
 Operator : DD/AJ
 Sample : K5152-11MSD
 Misc : 4.97g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 00:39:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	453703	17.930 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	819101	24.102 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	877071	24.104 ng/ml
3) t n-Heptane	7.758	284035	7.785 ng/ml
4) t Benzene	7.891	374487	8.482 ng/ml
6) t Toluene	10.630	1108379	25.716 ng/ml
7) t Ethylbenzene	13.070	340180	8.376 ng/ml
8) t m-Xylene	13.203	638681	16.600 ng/ml
9) t O-Xylene	13.931	619619	17.012 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	500179	17.553 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022810.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 16:39
Operator : DD/AJ
Sample : K5152-11MSD
Misc : 4.97g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:39:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

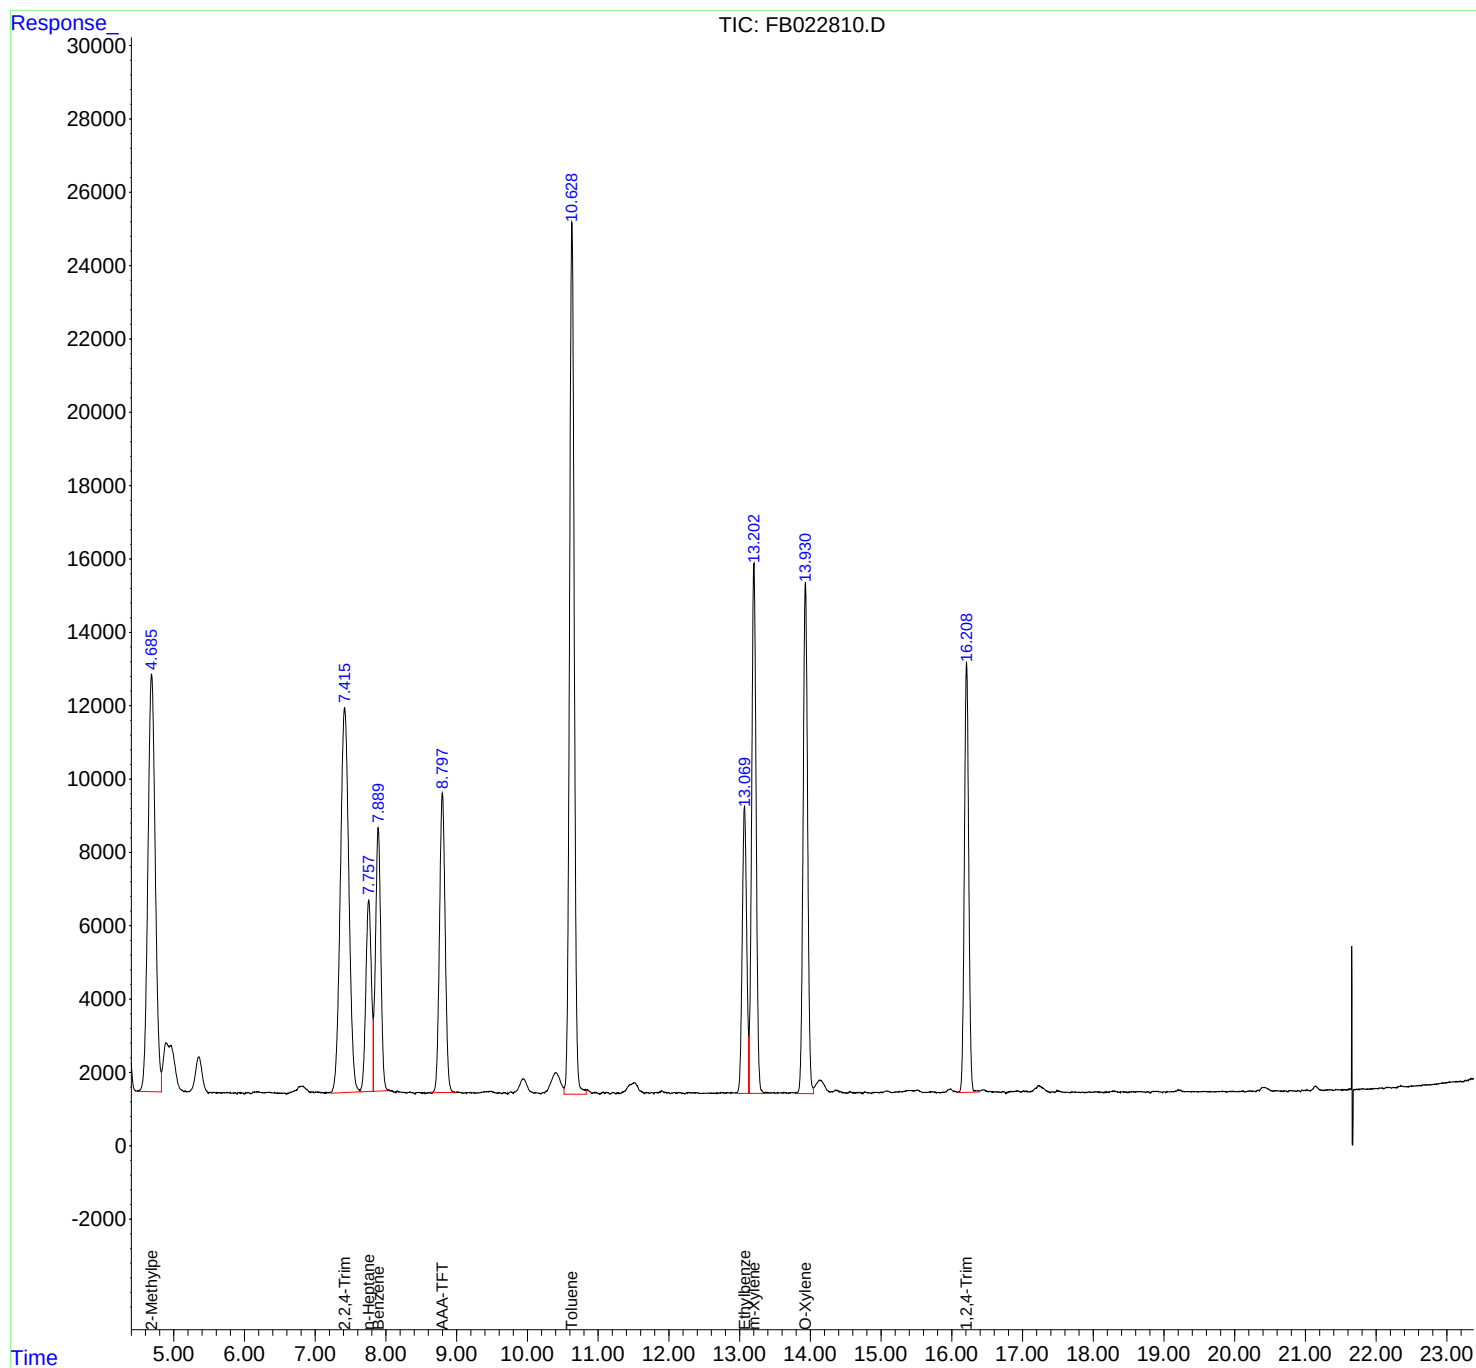

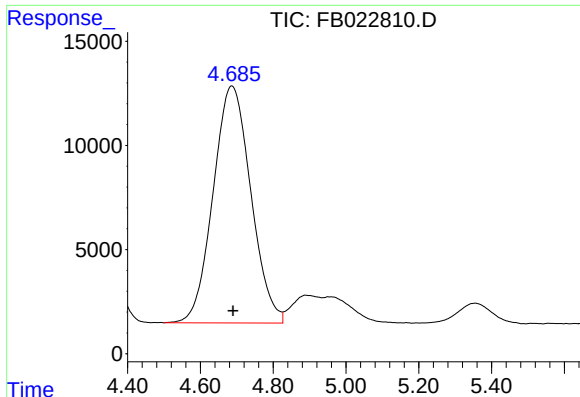


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.003 min
Response: 819101
Conc: 24.10 ng/ml

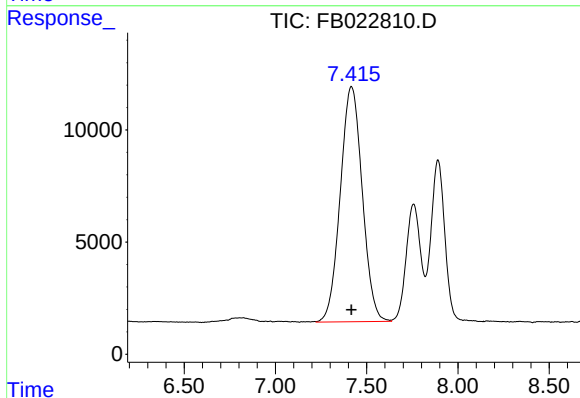


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 877071
Conc: 24.10 ng/ml

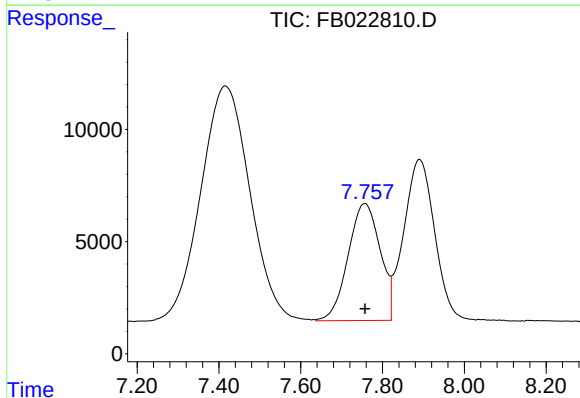


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 284035
Conc: 7.78 ng/ml

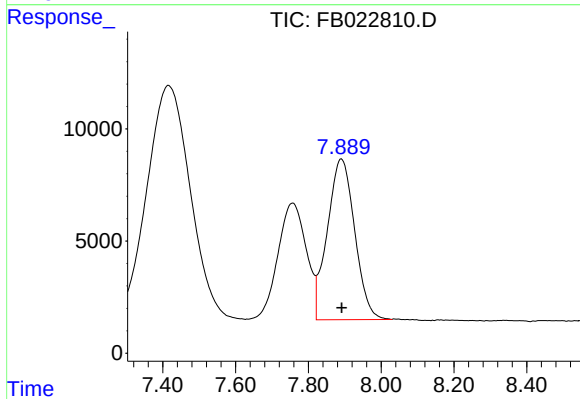


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 374487
Conc: 8.48 ng/ml

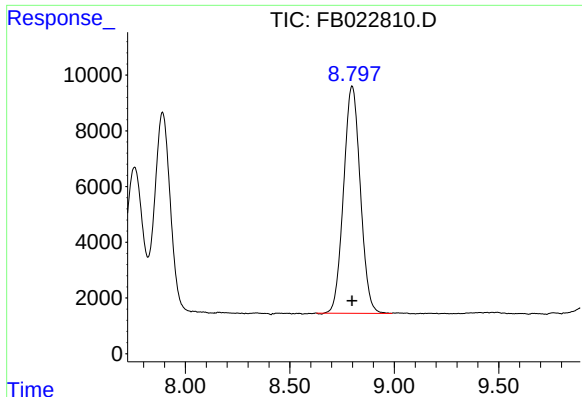


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 453703
Conc: 17.93 ng/ml

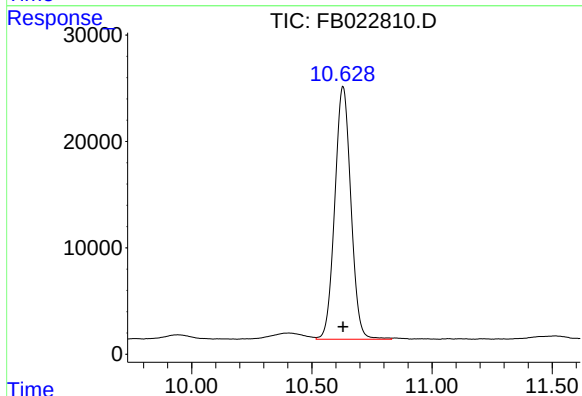


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1108379
Conc: 25.72 ng/ml

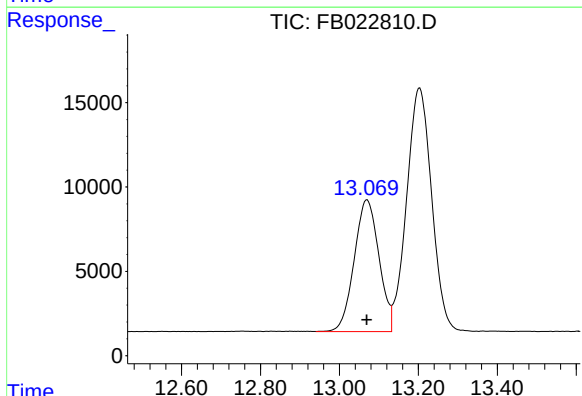


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 340180
Conc: 8.38 ng/ml

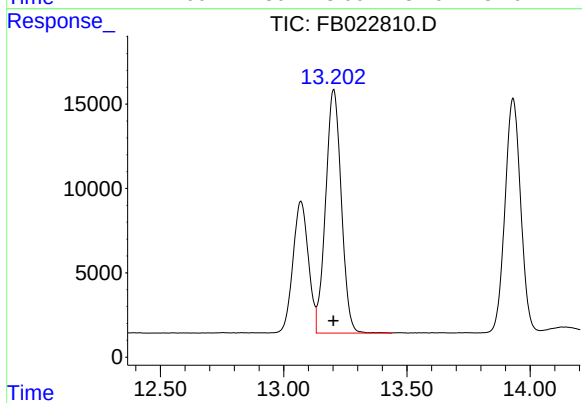


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 638681
Conc: 16.60 ng/ml

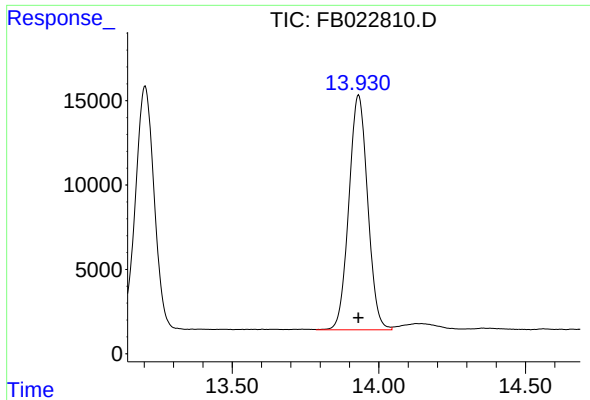

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 619619
Conc: 17.01 ng/ml

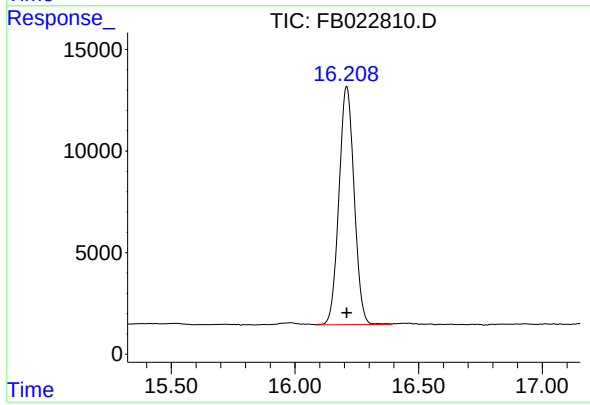

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 500179
Conc: 17.55 ng/ml