

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022811.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 17:09
Operator : DD/AJ
Sample : K5111-03
Misc : 4.97g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:39:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	21373	0.845 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.693	15116	0.445 ng/ml
2) t	2,2,4-Trimethylpentane	7.414	11091	0.305 ng/ml
3) t	n-Heptane	7.765	1411	0.039 ng/ml
4) t	Benzene	7.885	3906	0.088 ng/ml
6) t	Toluene	10.632	22717	0.527 ng/ml
7) t	Ethylbenzene	13.075	6663	0.164 ng/ml
8) t	m-Xylene	13.206	13767	0.358 ng/ml
9) t	O-Xylene	13.934	12192	0.335 ng/ml
10) t	1,2,4-Trimethylbenzene	16.212	14523	0.510 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022811.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 17:09
Operator : DD/AJ
Sample : K5111-03
Misc : 4.97g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:39:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

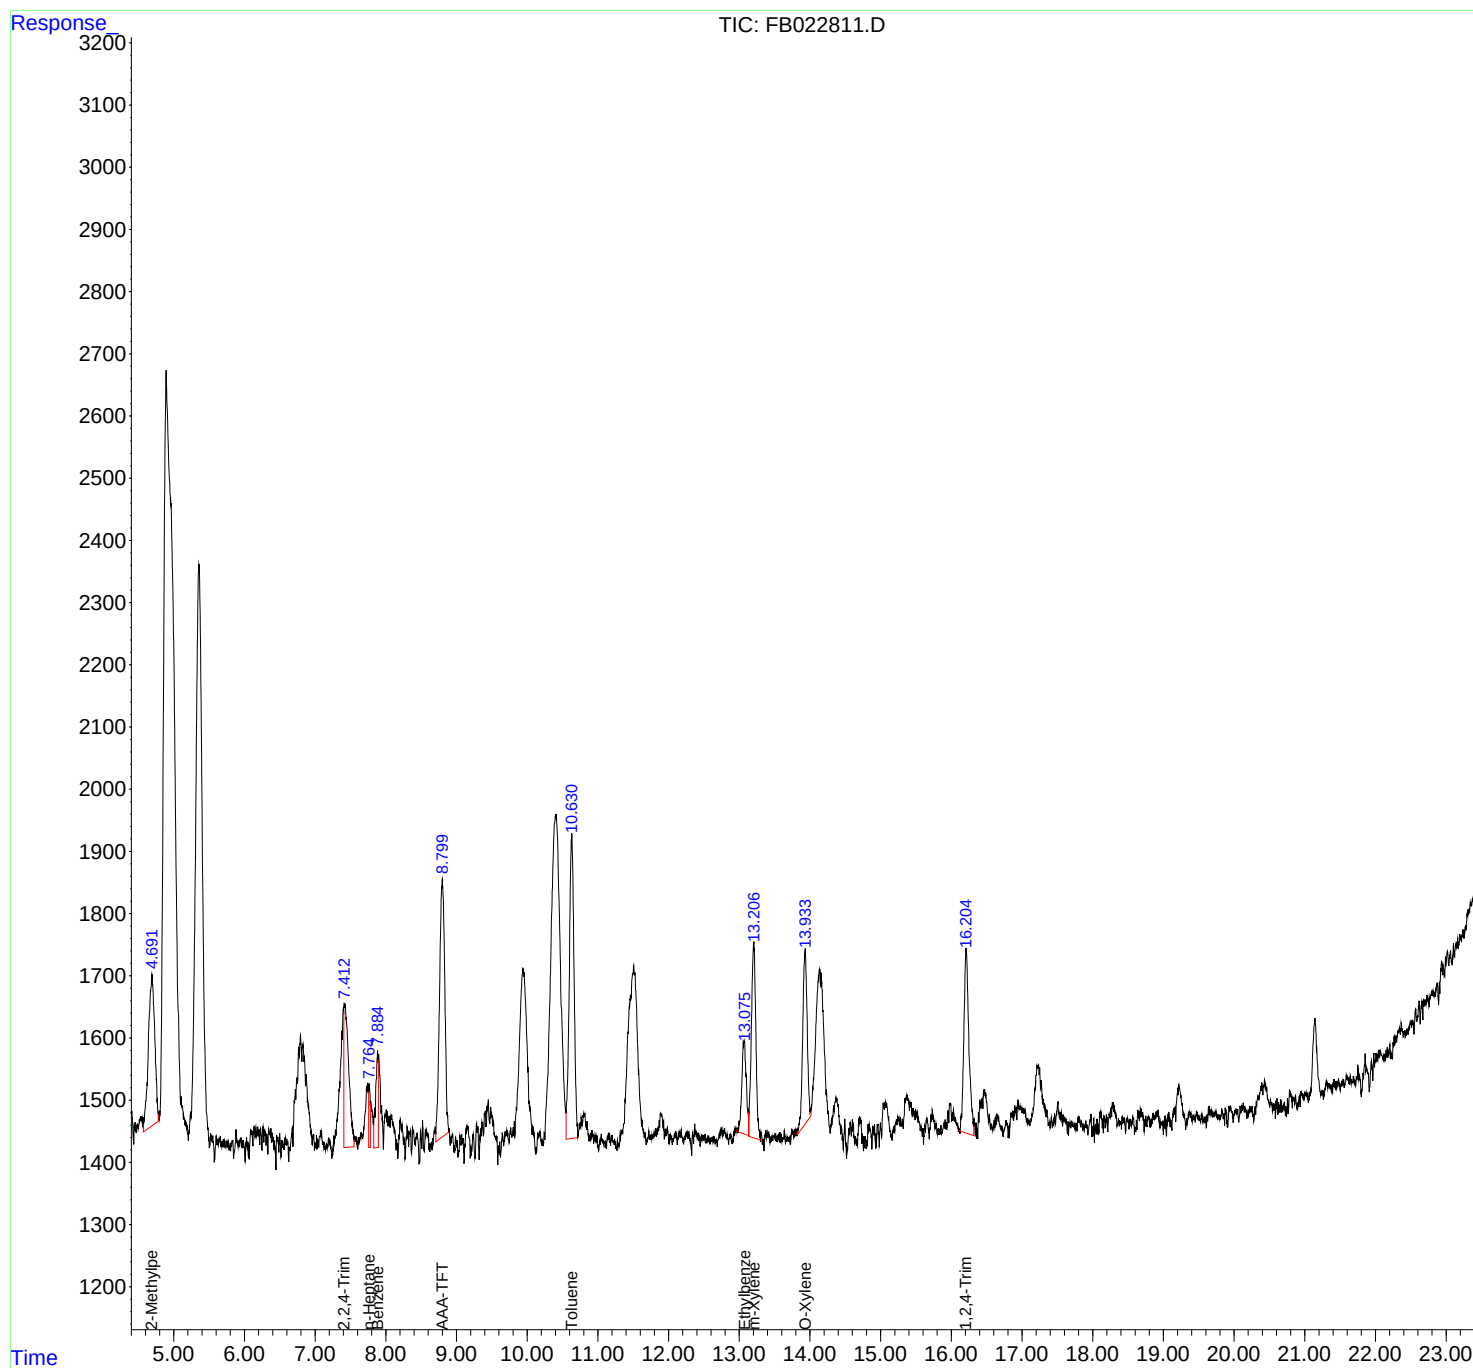

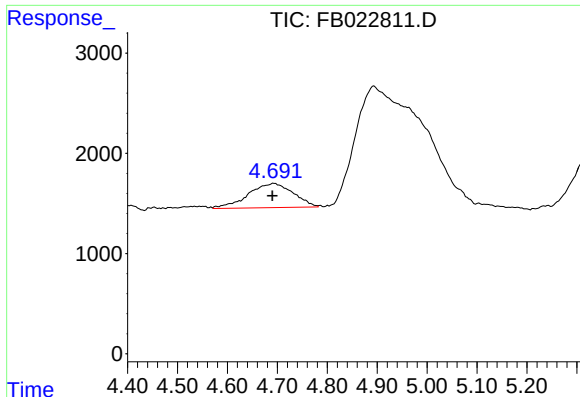


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.003 min
Response: 15116
Conc: 0.44 ng/ml

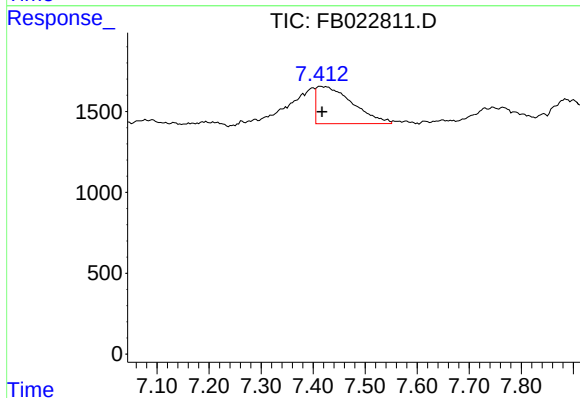


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.003 min
Response: 11091
Conc: 0.30 ng/ml

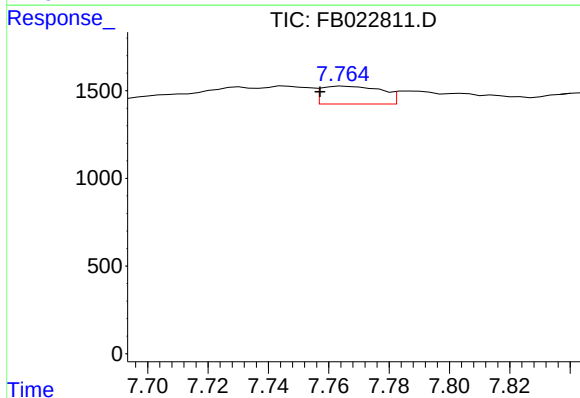


#3 n-Heptane

R.T.: 7.765 min
Delta R.T.: 0.008 min
Response: 1411
Conc: 0.04 ng/ml

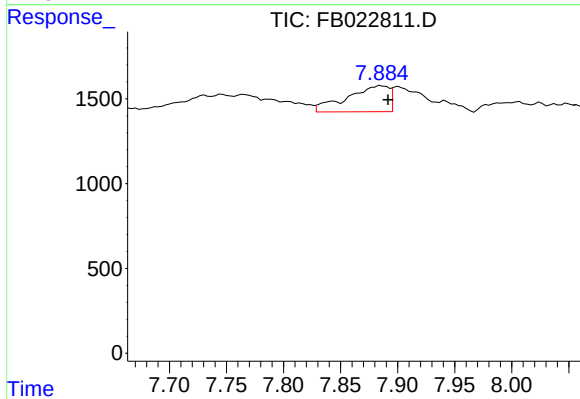


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.006 min
Response: 3906
Conc: 0.09 ng/ml

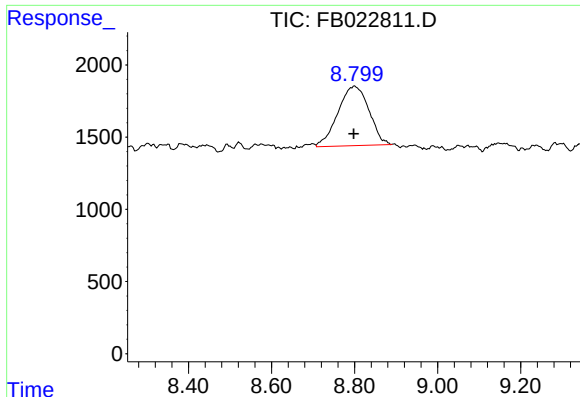


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 21373
Conc: 0.84 ng/ml

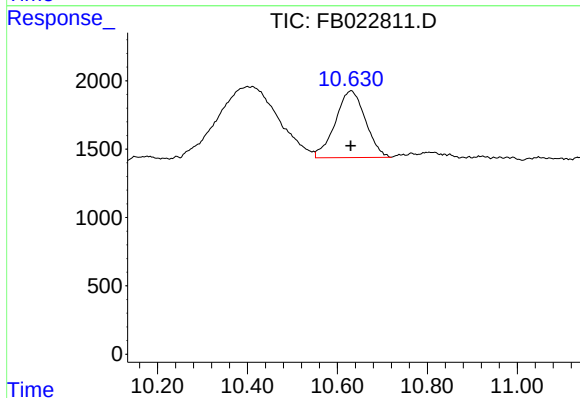


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 22717
Conc: 0.53 ng/ml

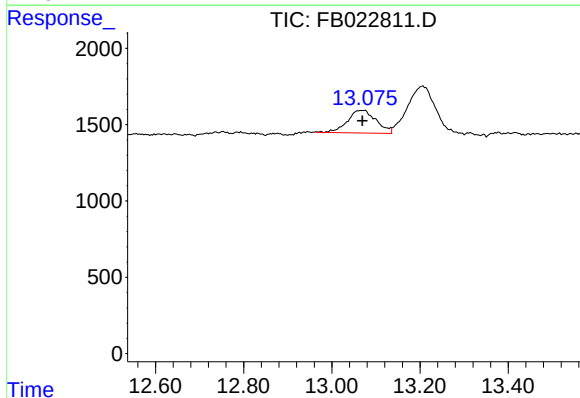


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.006 min
Response: 6663
Conc: 0.16 ng/ml

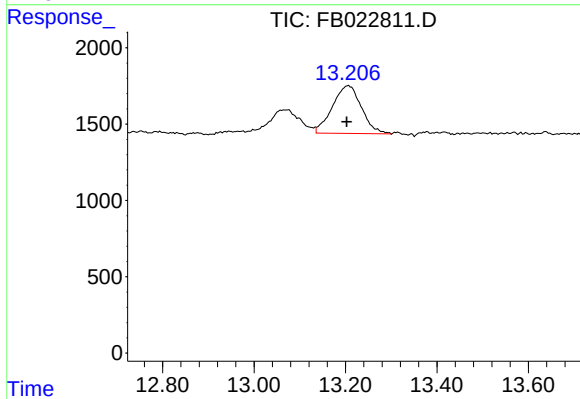


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.004 min
Response: 13767
Conc: 0.36 ng/ml

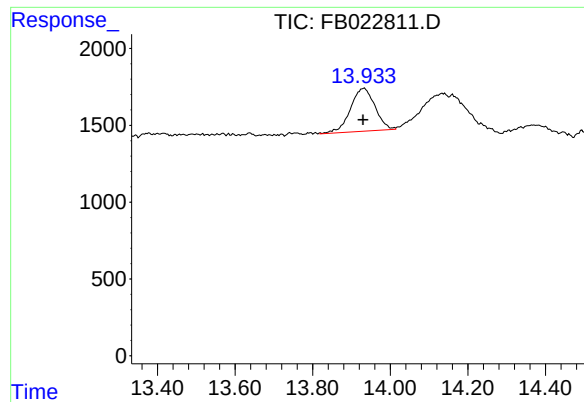

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.003 min
Response: 12192
Conc: 0.33 ng/ml

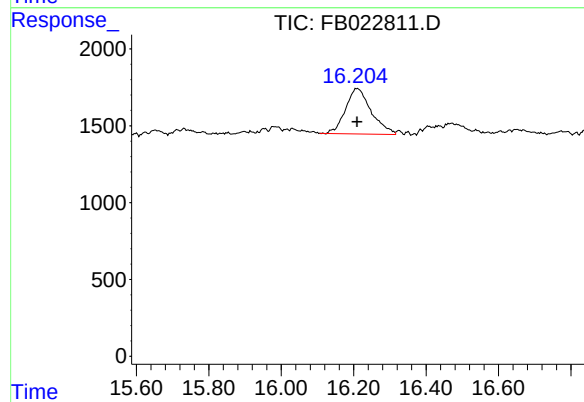

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.002 min
Response: 14523
Conc: 0.51 ng/ml