

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
 Data File : FB022806.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2019 14:17
 Operator : DD/AJ
 Sample : BSF1023S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 00:38:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	535462	21.161 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	1057477	31.116 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	1163308	31.970 ng/ml
3) t	n-Heptane	7.757	382360	10.479 ng/ml
4) t	Benzene	7.892	459144	10.399 ng/ml
6) t	Toluene	10.630	1326199	30.770 ng/ml
7) t	Ethylbenzene	13.069	409022	10.071 ng/ml
8) t	m-Xylene	13.203	763558	19.845 ng/ml
9) t	O-Xylene	13.930	726315	19.942 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	582630	20.446 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022806.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 14:17
Operator : DD/AJ
Sample : BSF1023S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

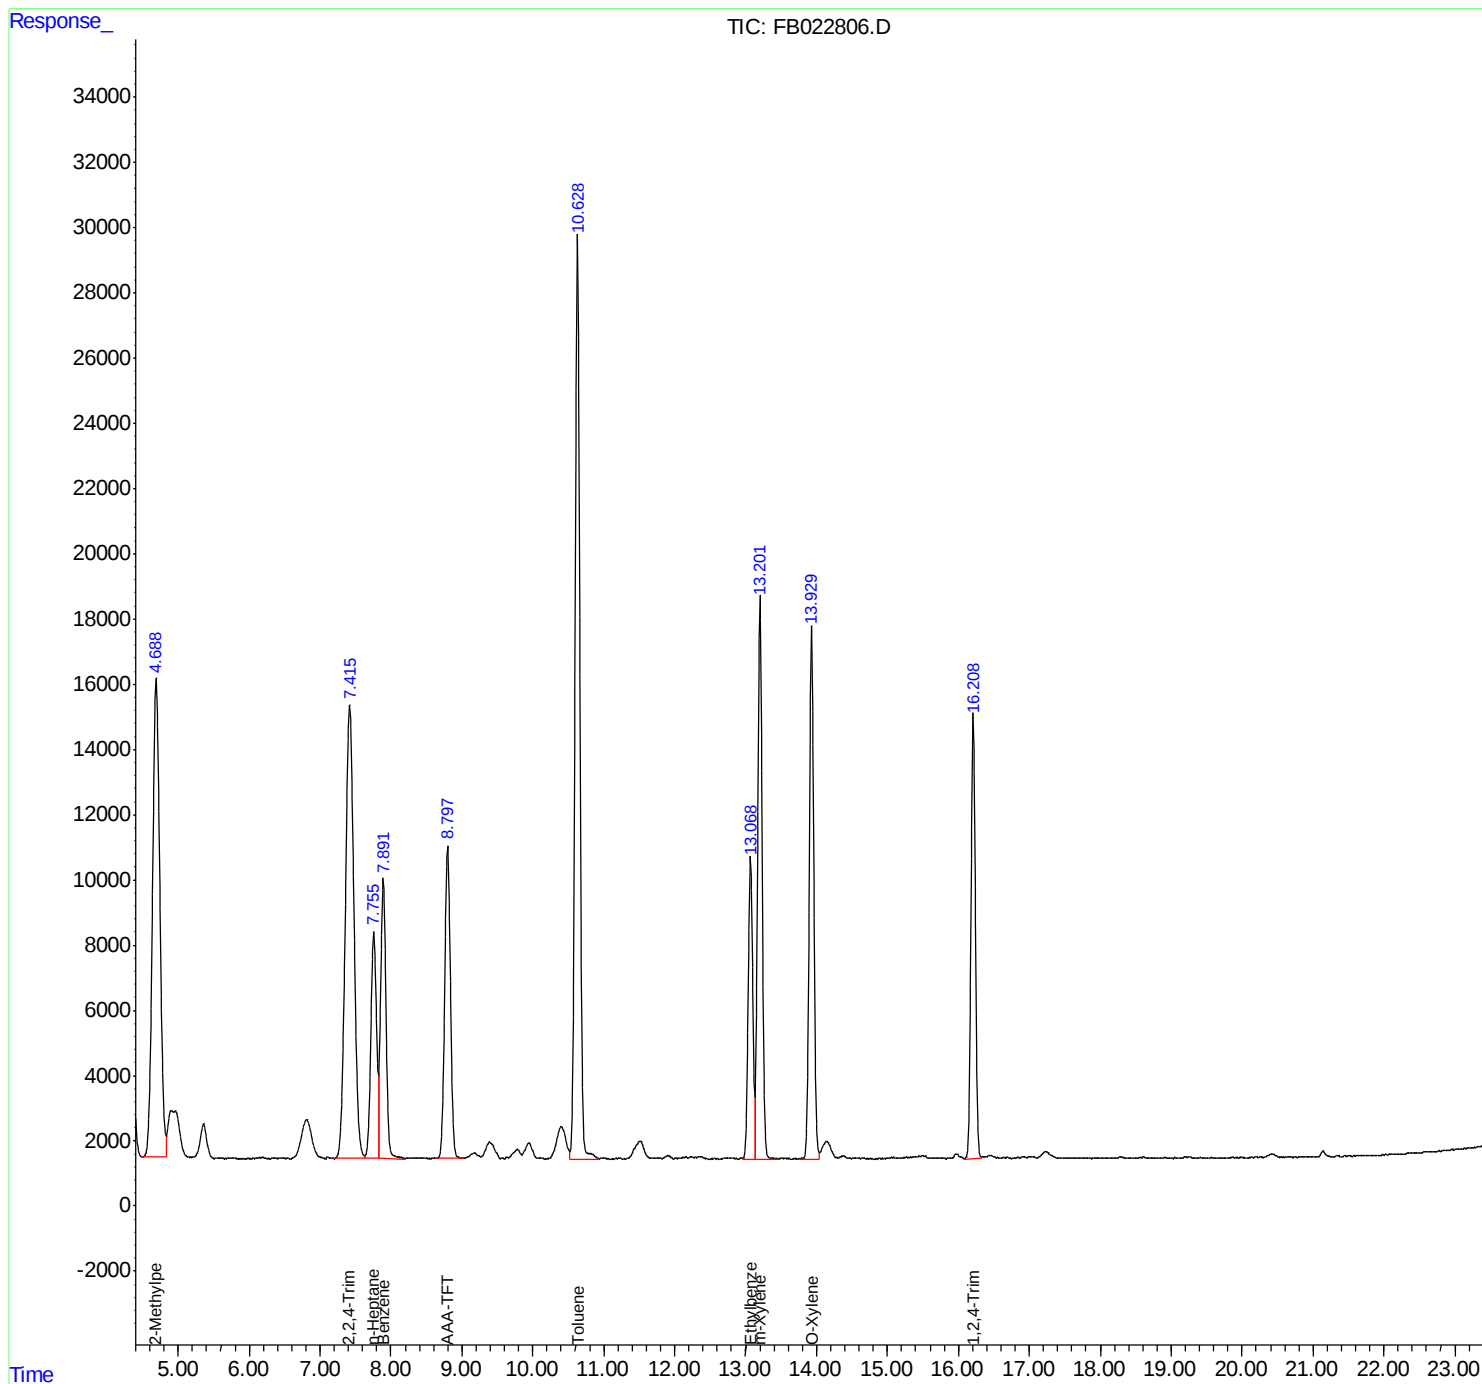

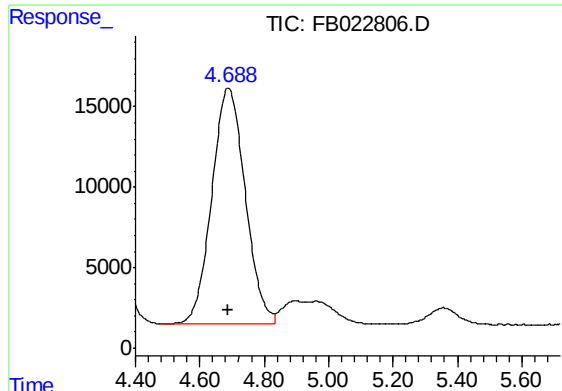


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 1057477
Conc: 31.12 ng/ml

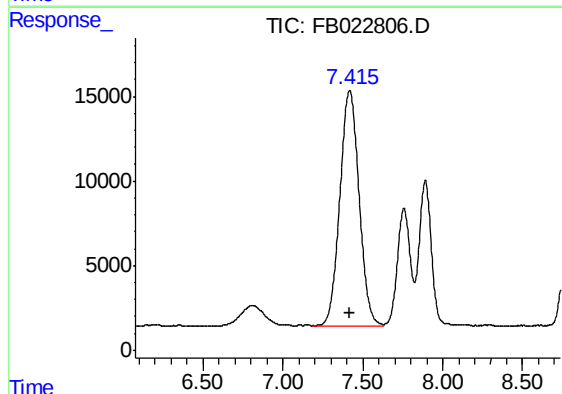


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 1163308
Conc: 31.97 ng/ml

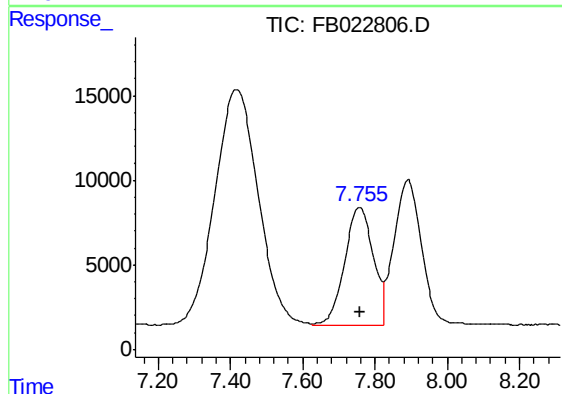


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 382360
Conc: 10.48 ng/ml

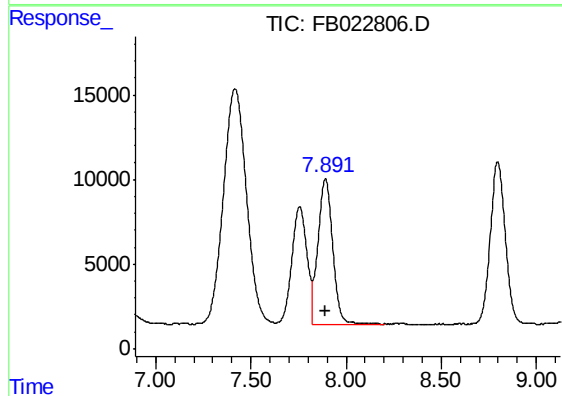


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 459144
Conc: 10.40 ng/ml

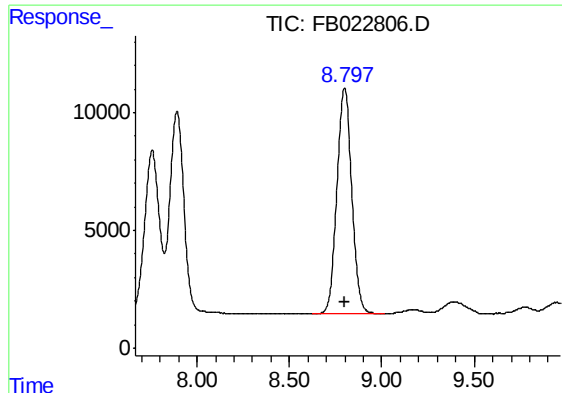


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 535462
Conc: 21.16 ng/ml

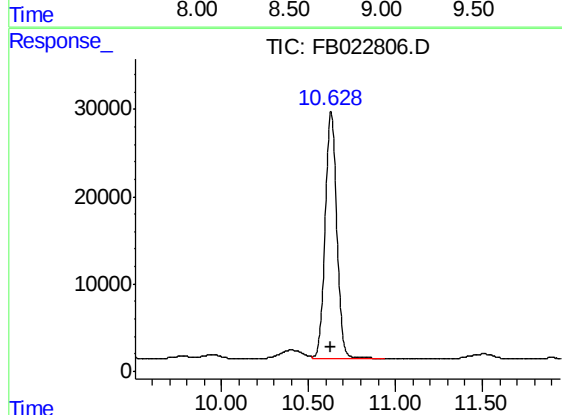


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1326199
Conc: 30.77 ng/ml

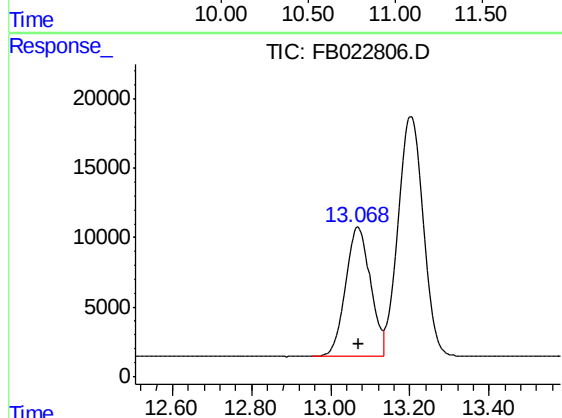


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 409022
Conc: 10.07 ng/ml

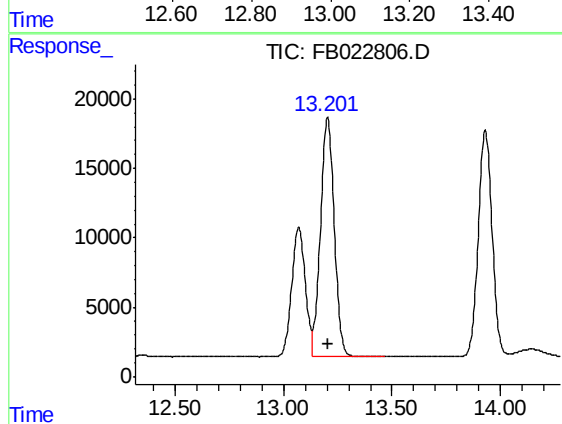


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 763558
Conc: 19.85 ng/ml

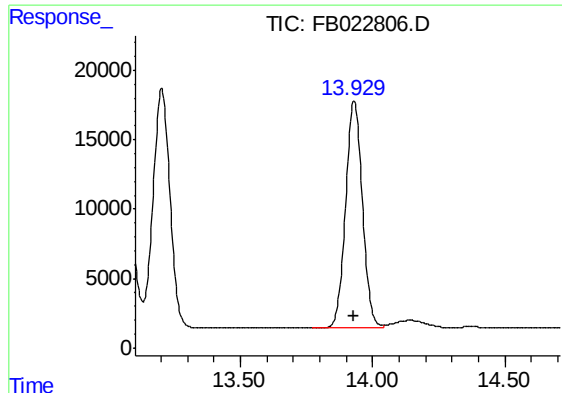

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 726315
Conc: 19.94 ng/ml

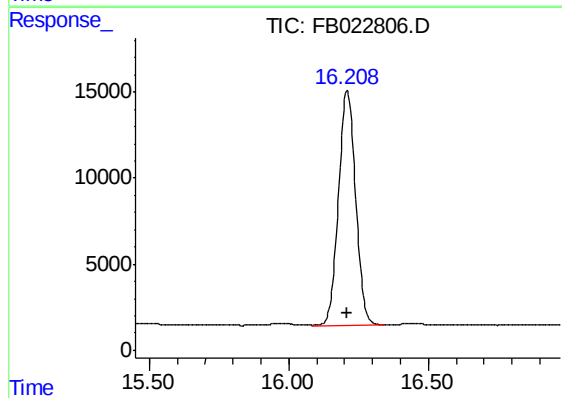

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 582630
Conc: 20.45 ng/ml