

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
 Data File : FB022812.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2019 17:39
 Operator : DD/AJ
 Sample : K5152-13
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 00:39:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	59572	2.354 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	87982	2.589 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	98992	2.720 ng/ml
3) t n-Heptane	7.757	32669	0.895 ng/ml
4) t Benzene	7.893	36549	0.828 ng/ml
6) t Toluene	10.630	110262	2.558 ng/ml
7) t Ethylbenzene	13.071	35854	0.883 ng/ml
8) t m-Xylene	13.202	68040	1.768 ng/ml
9) t O-Xylene	13.931	66152	1.816 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	53541	1.879 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022812.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 17:39
Operator : DD/AJ
Sample : K5152-13
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:39:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

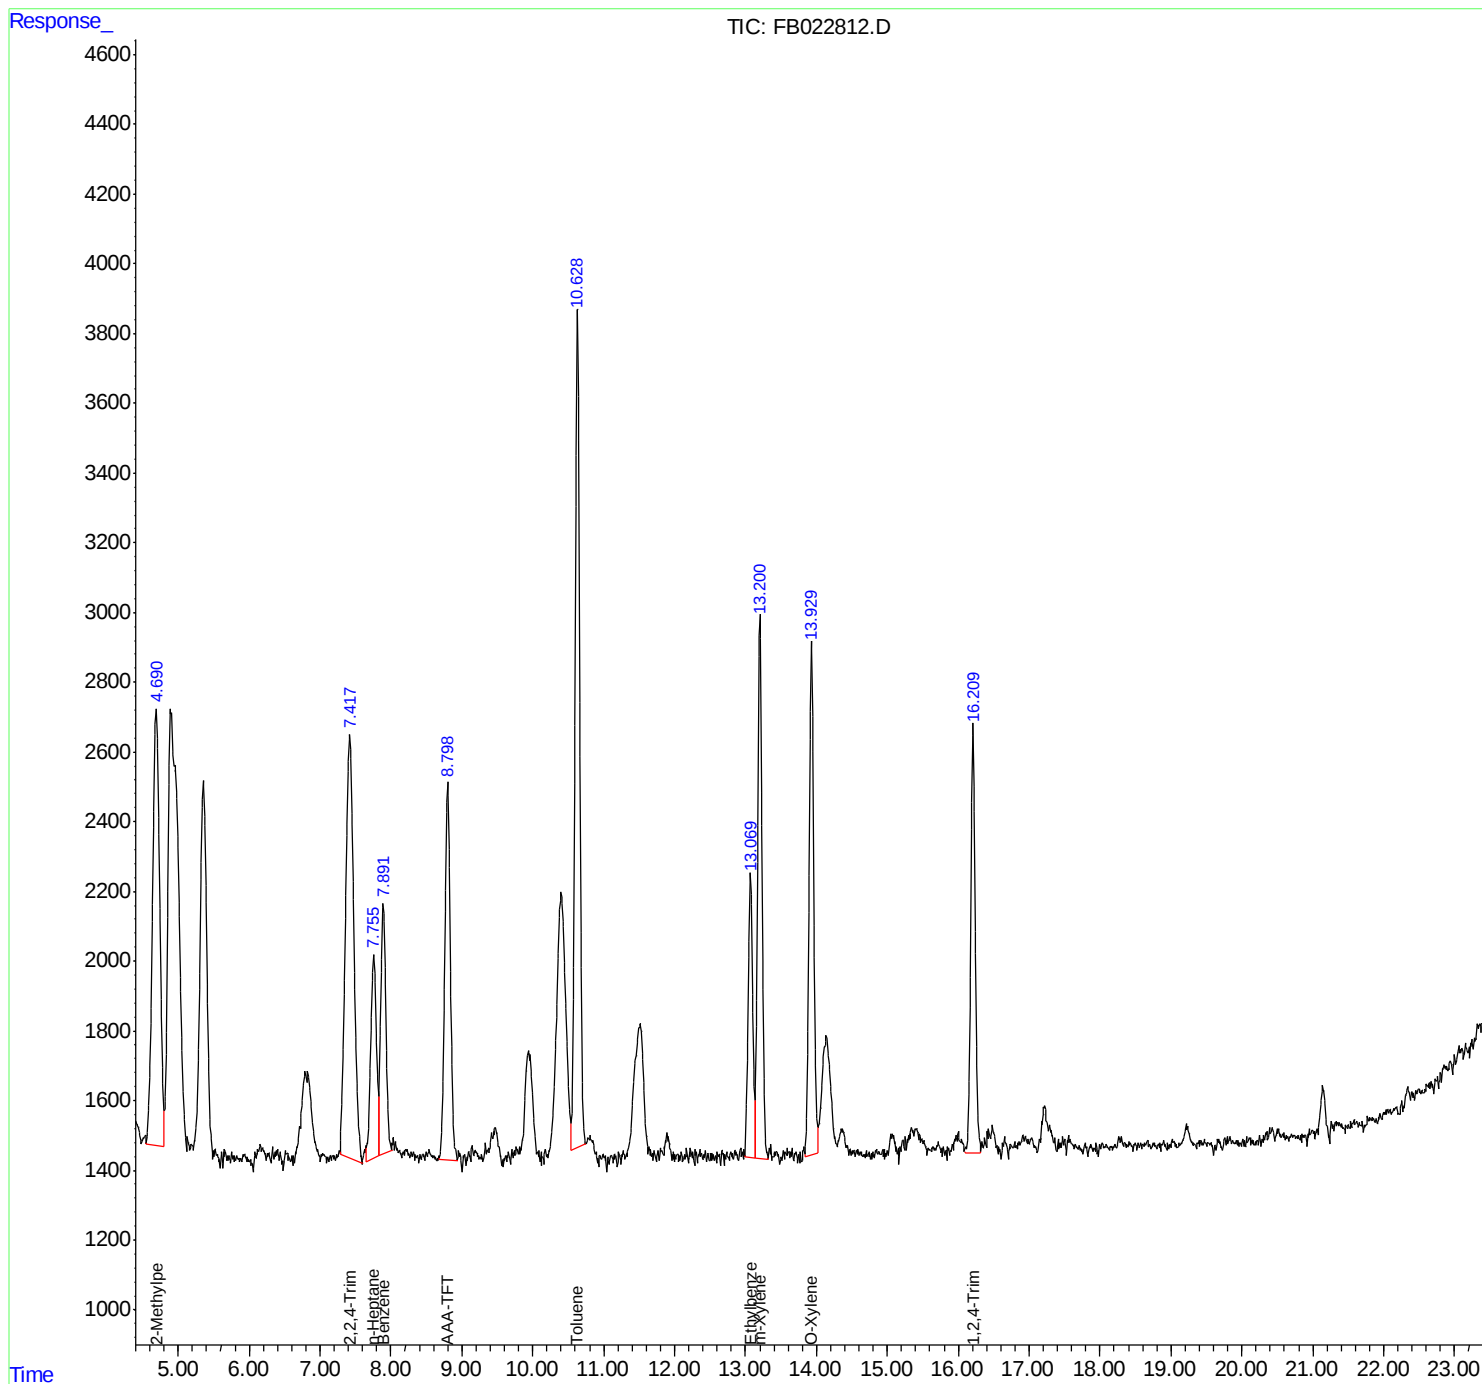

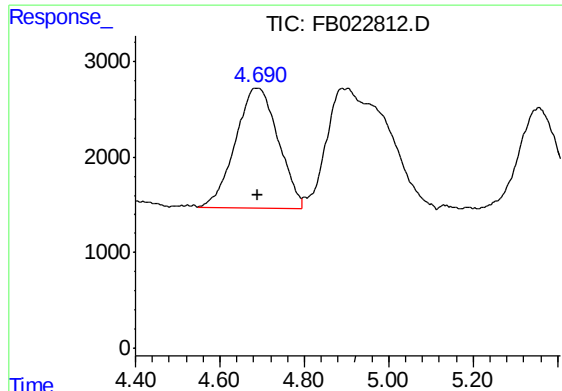


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.002 min
Response: 87982
Conc: 2.59 ng/ml

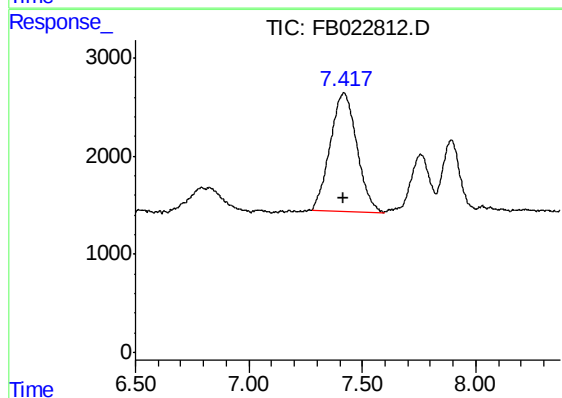


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 98992
Conc: 2.72 ng/ml

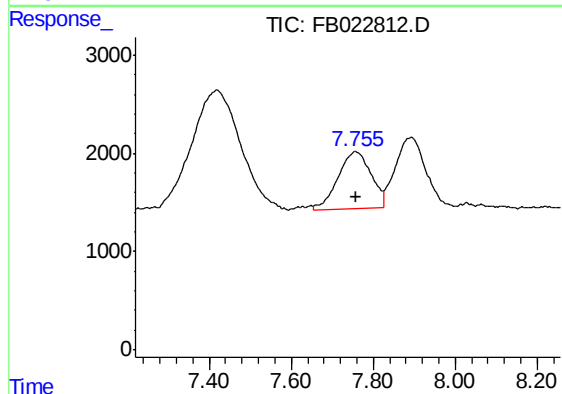


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 32669
Conc: 0.90 ng/ml

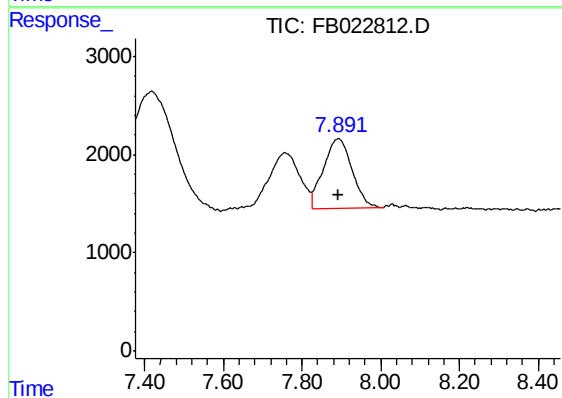


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 36549
Conc: 0.83 ng/ml

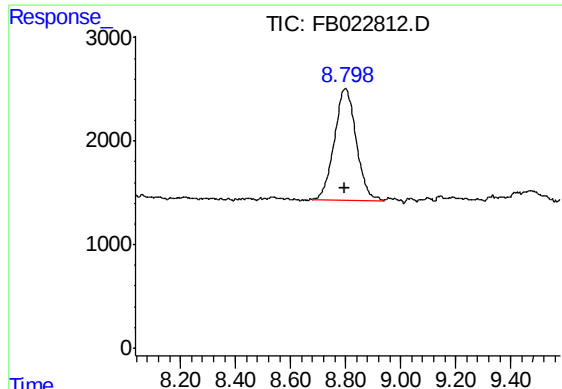


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.001 min
Response: 59572
Conc: 2.35 ng/ml

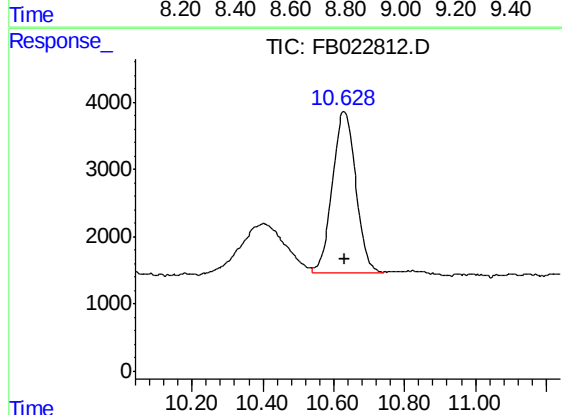


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 110262
Conc: 2.56 ng/ml

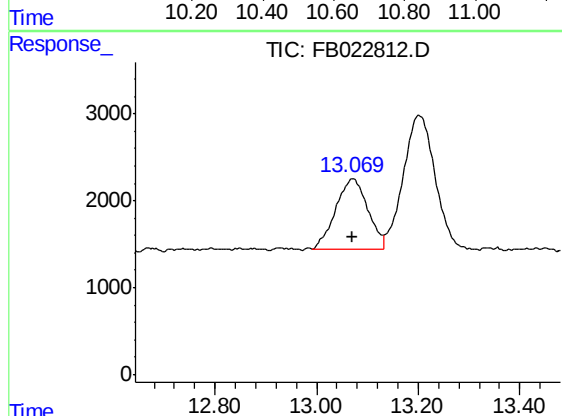


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.002 min
Response: 35854
Conc: 0.88 ng/ml

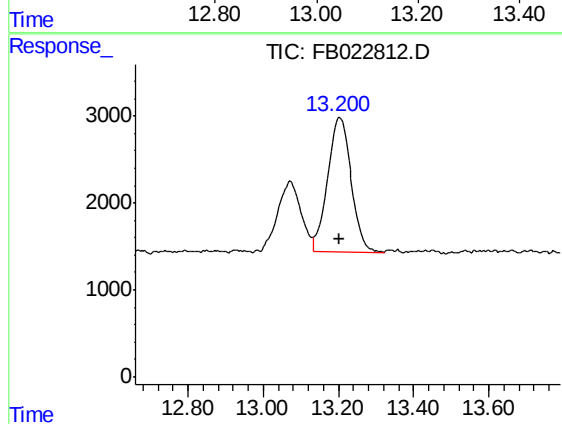


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 68040
Conc: 1.77 ng/ml

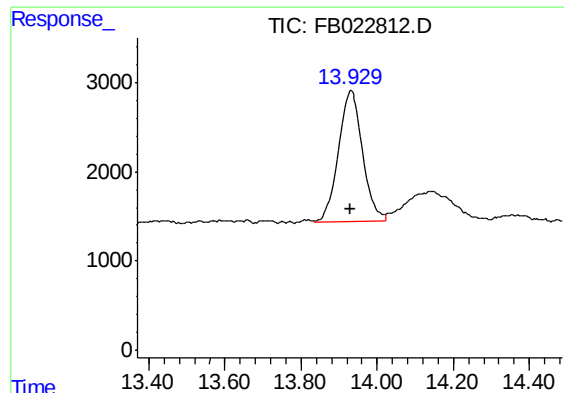

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 66152
Conc: 1.82 ng/ml

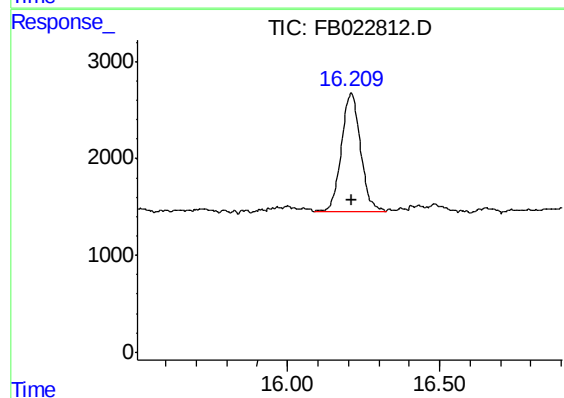

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 53541
Conc: 1.88 ng/ml