

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
 Data File : FB022816.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2019 19:39
 Operator : DD/AJ
 Sample : K5111-03
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 00:40:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	22839	0.903 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	47137	1.387 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	47222	1.298 ng/ml
3) t n-Heptane	7.762	14309	0.392 ng/ml
4) t Benzene	7.893	21926	0.497 ng/ml
6) t Toluene	10.631	70158	1.628 ng/ml
7) t Ethylbenzene	13.070	22633	0.557 ng/ml
8) t m-Xylene	13.202	41855	1.088 ng/ml
9) t O-Xylene	13.931	40802	1.120 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	30435	1.068 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102319\
Data File : FB022816.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2019 19:39
Operator : DD/AJ
Sample : K5111-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:40:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

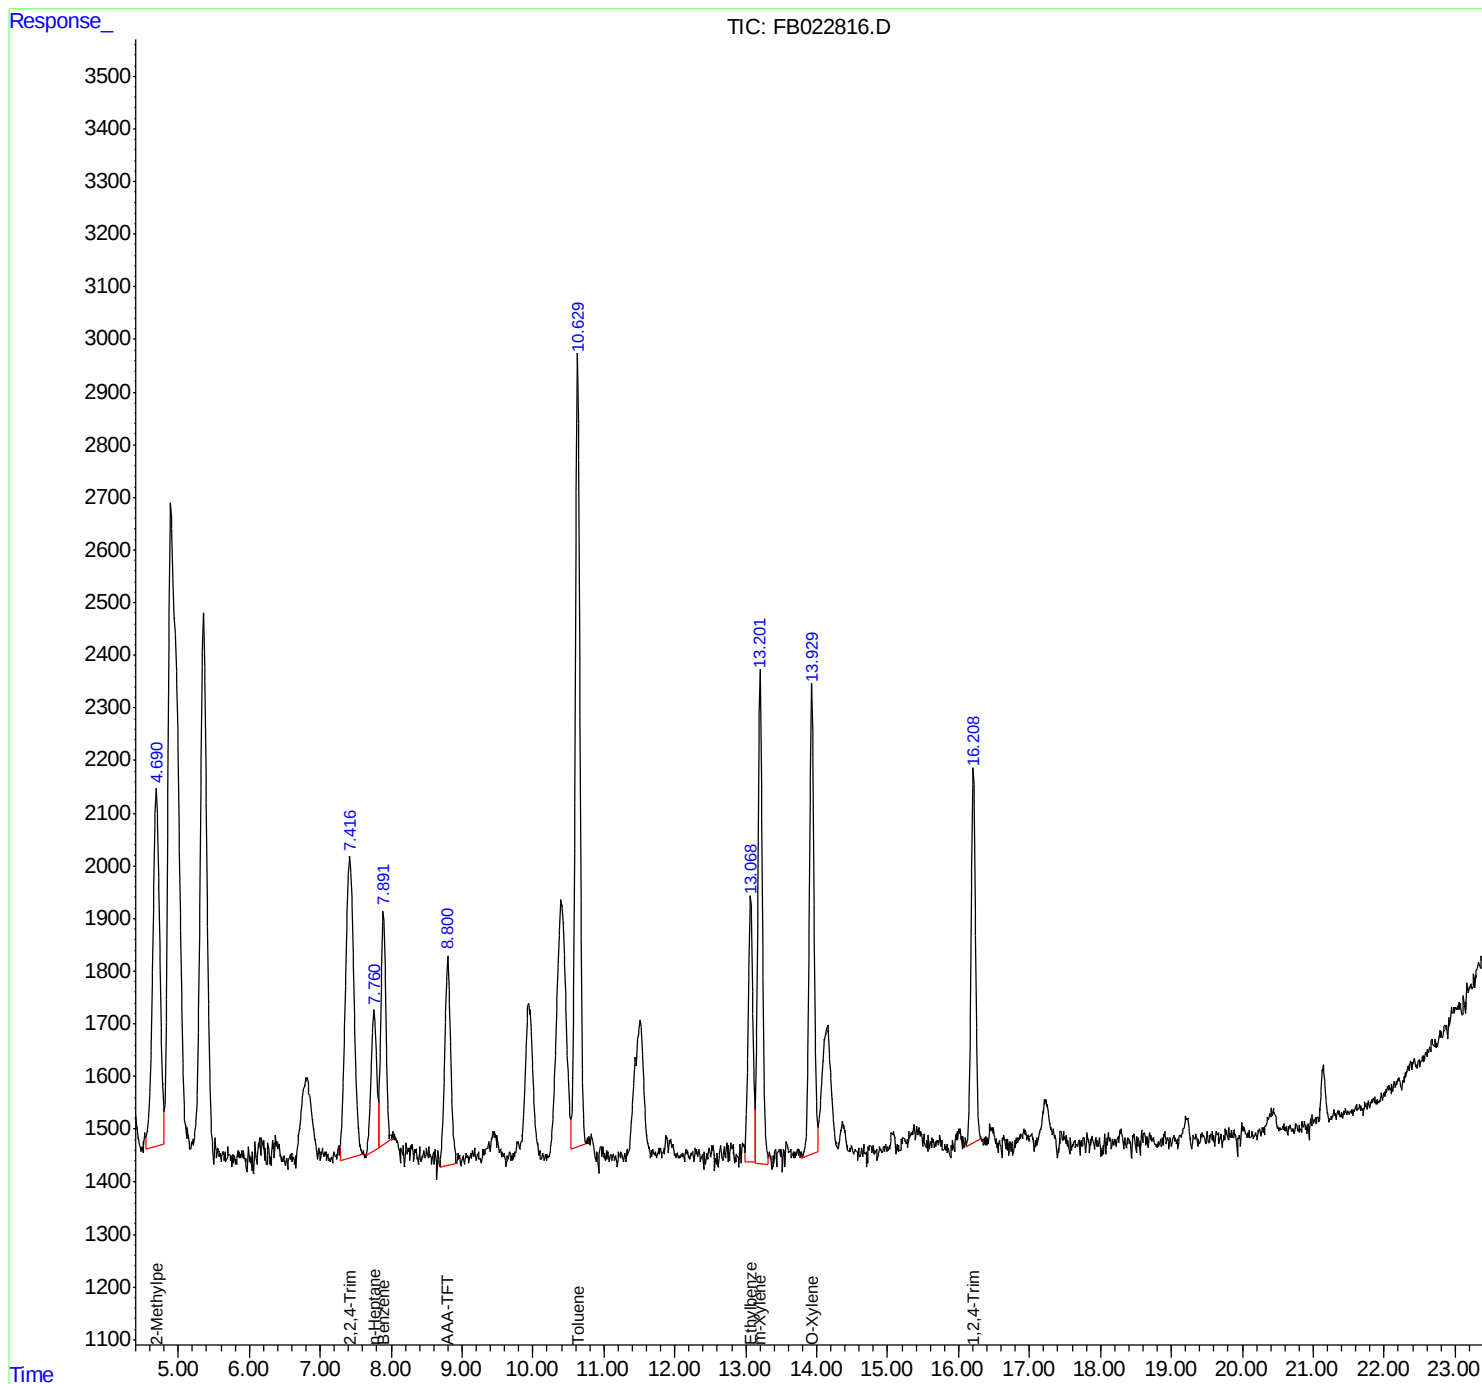

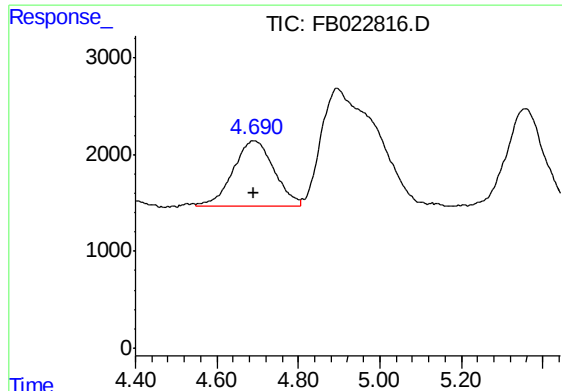


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.002 min
Response: 47137
Conc: 1.39 ng/ml

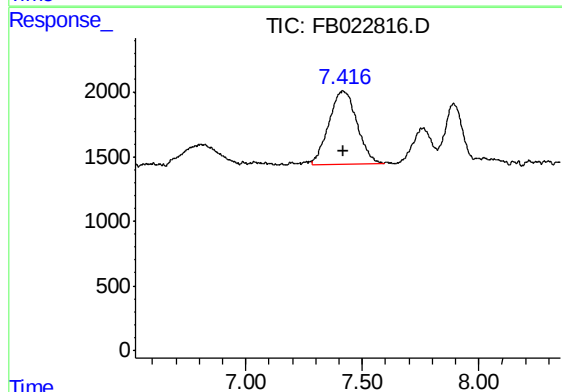


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 47222
Conc: 1.30 ng/ml

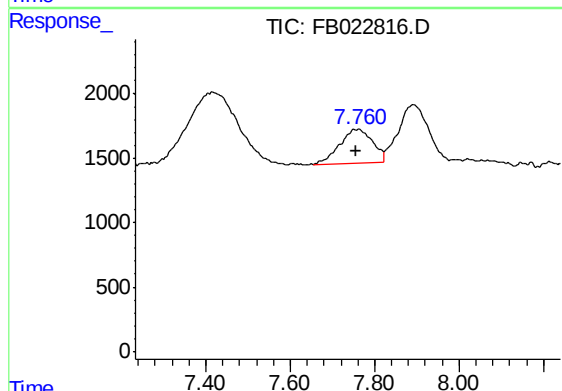


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.005 min
Response: 14309
Conc: 0.39 ng/ml

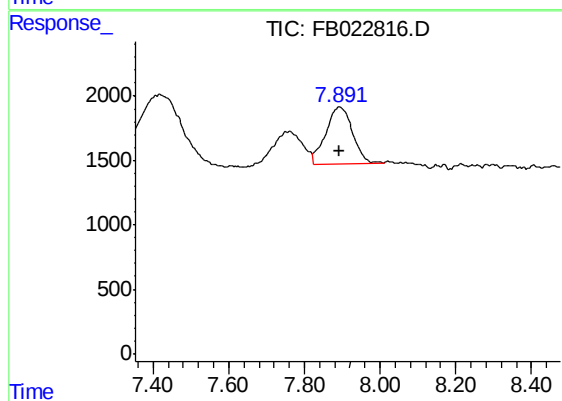


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 21926
Conc: 0.50 ng/ml

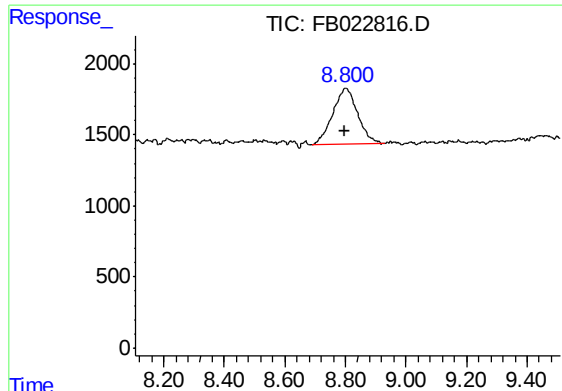


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 22839
Conc: 0.90 ng/ml

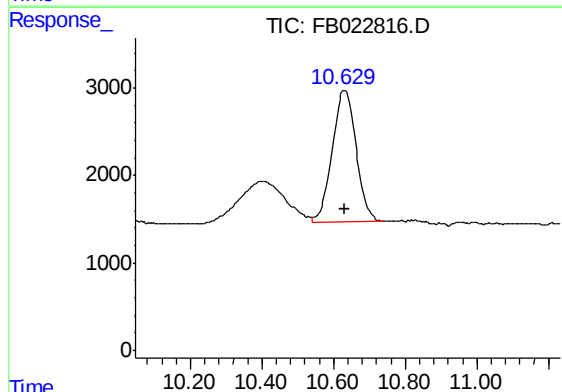


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.001 min
Response: 70158
Conc: 1.63 ng/ml

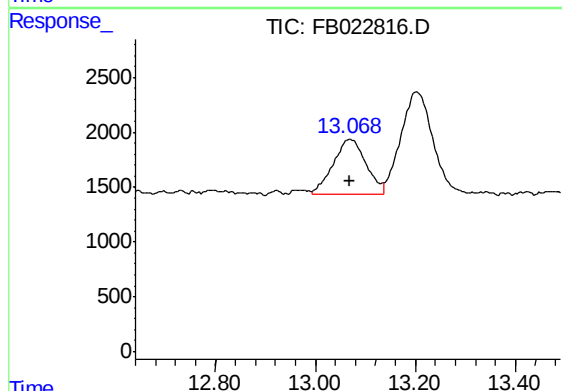


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 22633
Conc: 0.56 ng/ml

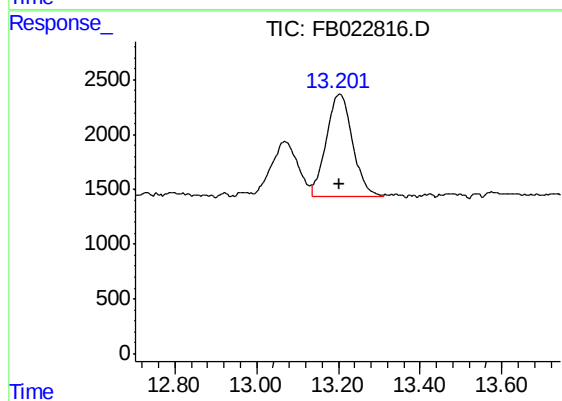


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 41855
Conc: 1.09 ng/ml

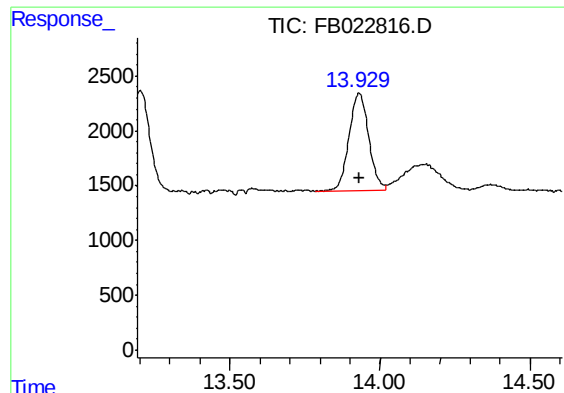

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 40802
Conc: 1.12 ng/ml

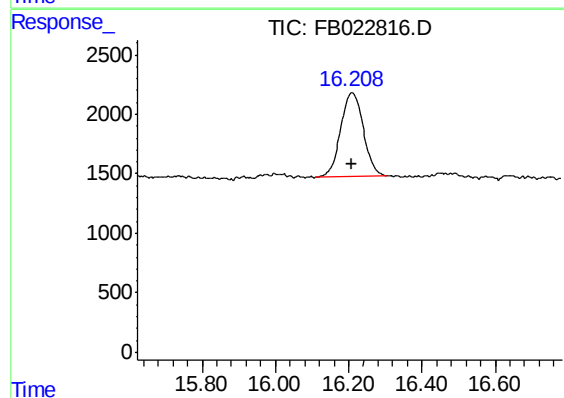

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 30435
Conc: 1.07 ng/ml