

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102320\
 Data File : FB025139.D
 Signal(s) : FID2B.CH
 Acq On : 23 Oct 2020 12:09
 Operator : DD/AJ
 Sample : L4496-02MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 24 00:56:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	497842	23.320 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	855861	28.140 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	756164	24.273 ng/ml
3) t n-Heptane	7.757	246071	8.003 ng/ml
4) t Benzene	7.893	388304	10.332 ng/ml
6) t Toluene	10.631	1069636	30.013 ng/ml
7) t Ethylbenzene	13.070	317010	9.739 ng/ml
8) t m-Xylene	13.203	628098	19.585 ng/ml
9) t O-Xylene	13.931	613910	19.915 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	485152	18.582 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102320\
Data File : FB025139.D
Signal(s) : FID2B.CH
Acq On : 23 Oct 2020 12:09
Operator : DD/AJ
Sample : L4496-02MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 24 00:56:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

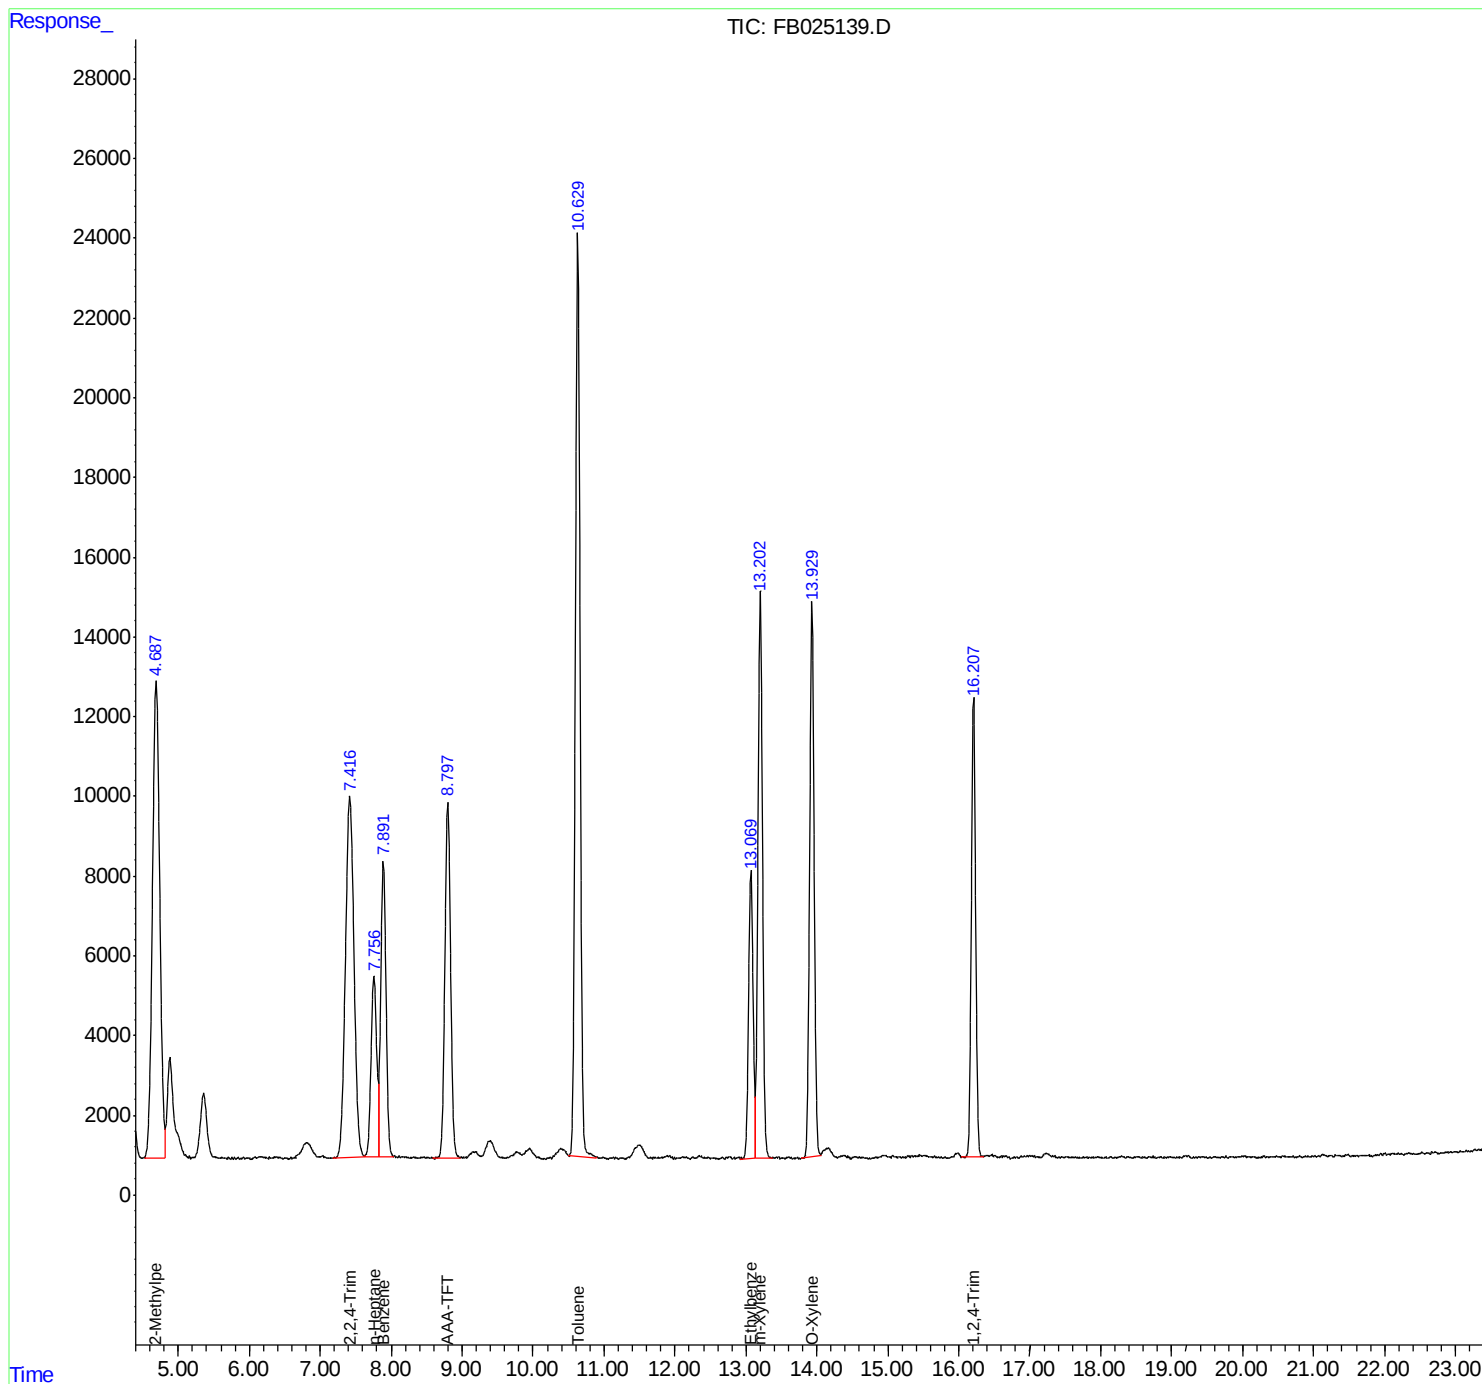

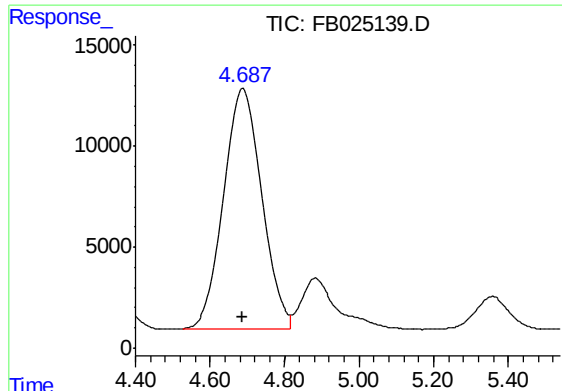


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 855861
Conc: 28.14 ng/ml

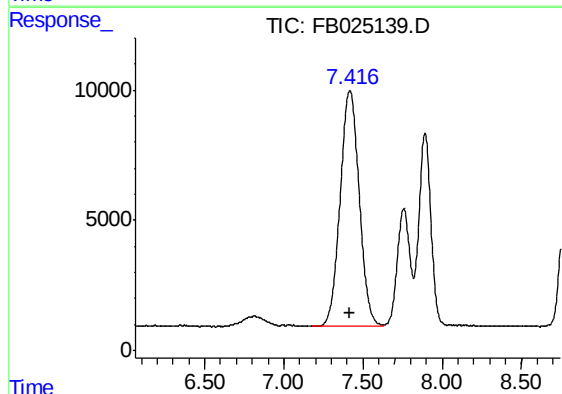


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 756164
Conc: 24.27 ng/ml

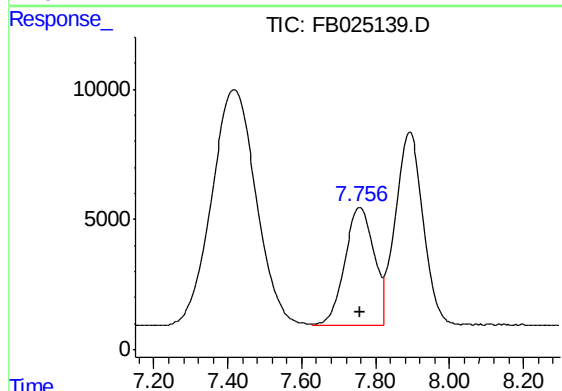


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 246071
Conc: 8.00 ng/ml

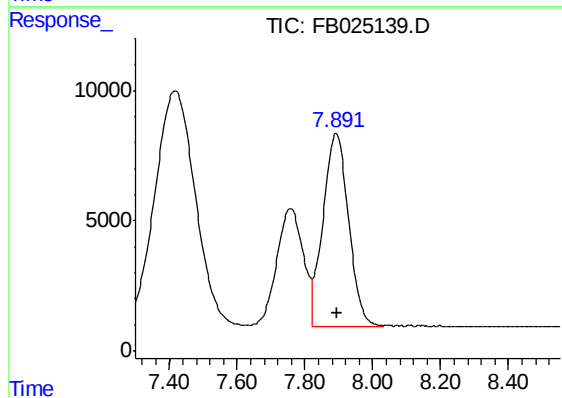


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 388304
Conc: 10.33 ng/ml

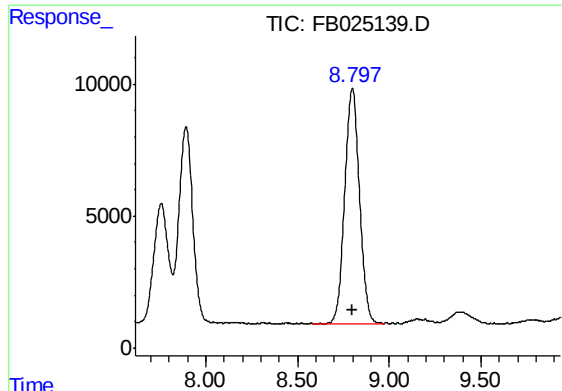


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 497842
Conc: 23.32 ng/ml

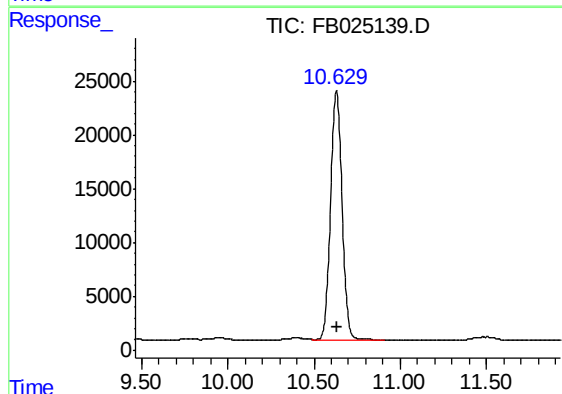


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1069636
Conc: 30.01 ng/ml

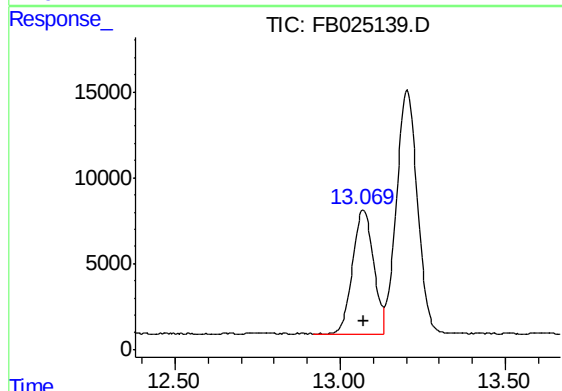


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 317010
Conc: 9.74 ng/ml

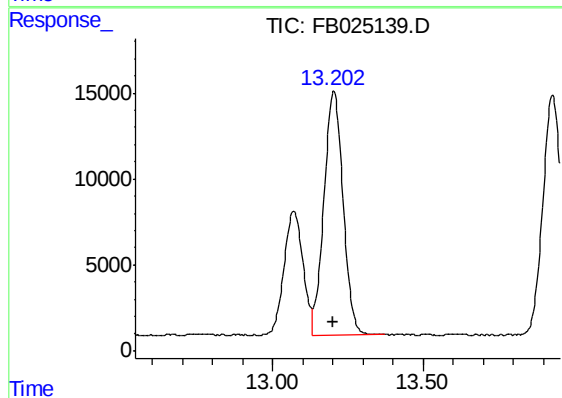


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 628098
Conc: 19.58 ng/ml

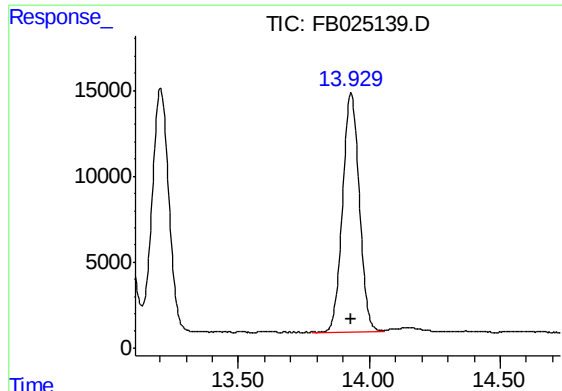

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 613910
Conc: 19.91 ng/ml

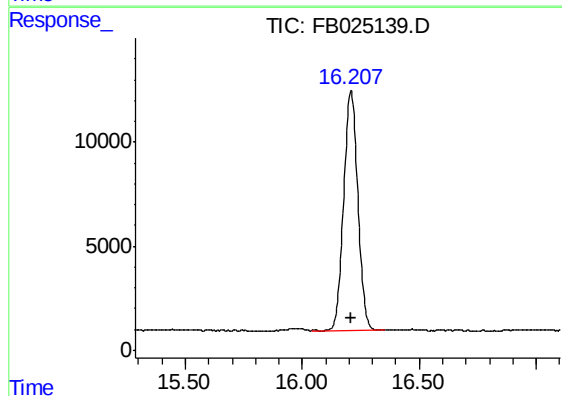

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 485152
Conc: 18.58 ng/ml