

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102418\
 Data File : FB018349.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2018 20:33
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 08:42:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	193048	22.414 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	451640	29.530 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	448543	30.355 ng/ml
3) t n-Heptane	8.068	144040	10.164 ng/ml
4) t Benzene	8.208	179711	9.647 ng/ml
6) t Toluene	10.962	462588	30.352 ng/ml
7) t Ethylbenzene	13.411	153561	9.679 ng/ml
8) t m-Xylene	13.544	317499	19.082 ng/ml
9) t O-Xylene	14.276	338414	18.980 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	492308	24.200 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102418\
Data File : FB018349.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2018 20:33
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 08:42:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

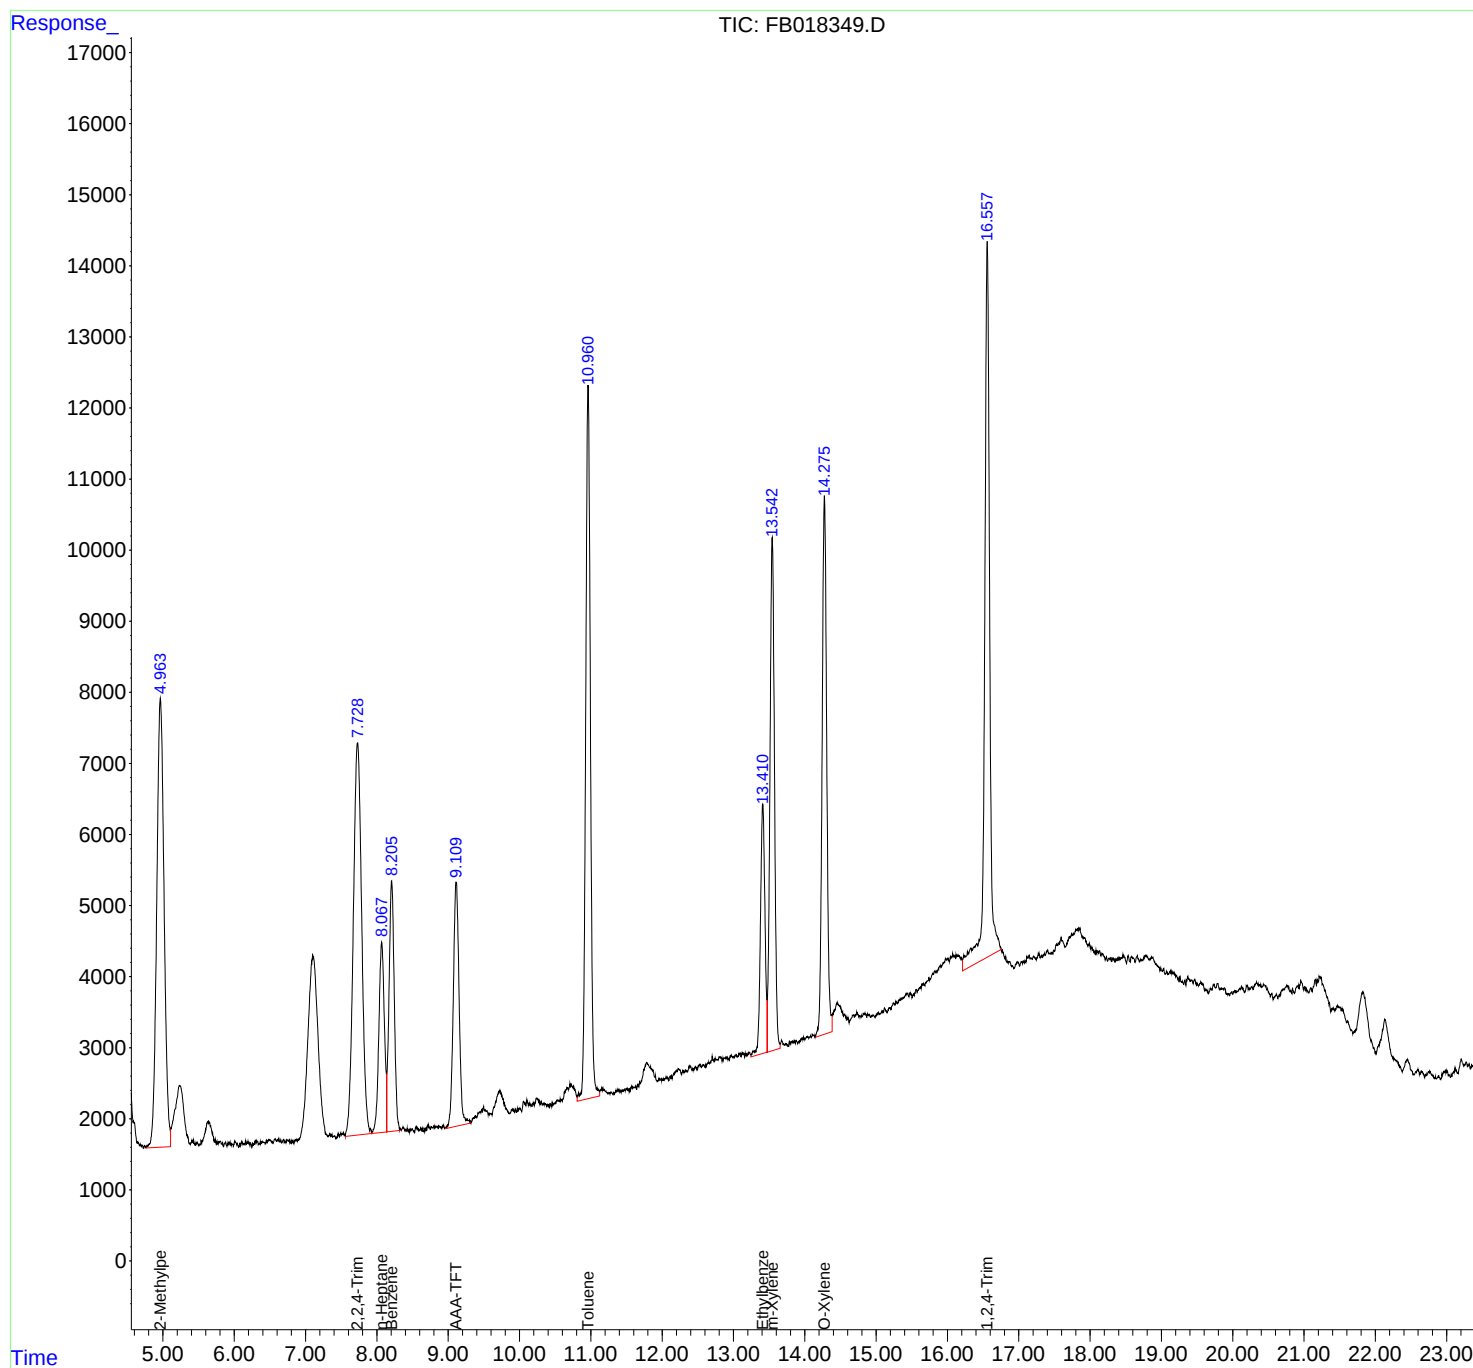

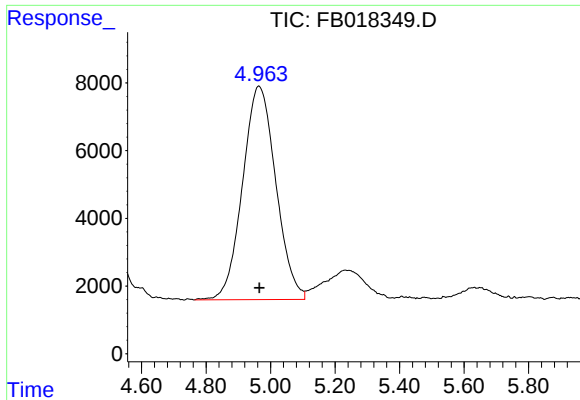


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 451640
Conc: 29.53 ng/ml

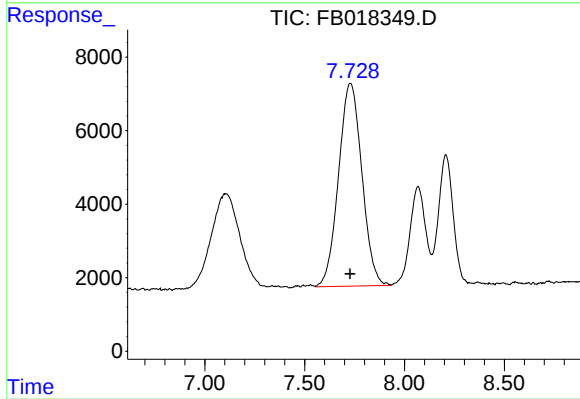


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 448543
Conc: 30.35 ng/ml

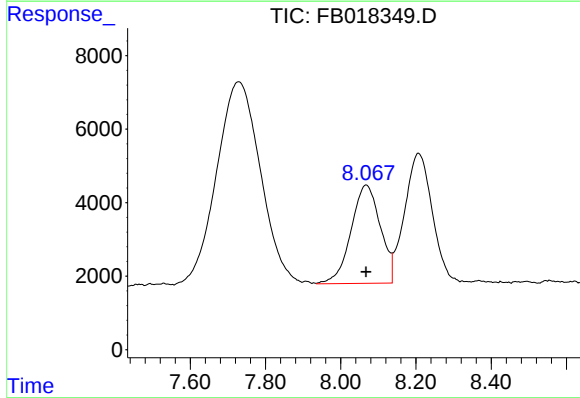


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 144040
Conc: 10.16 ng/ml

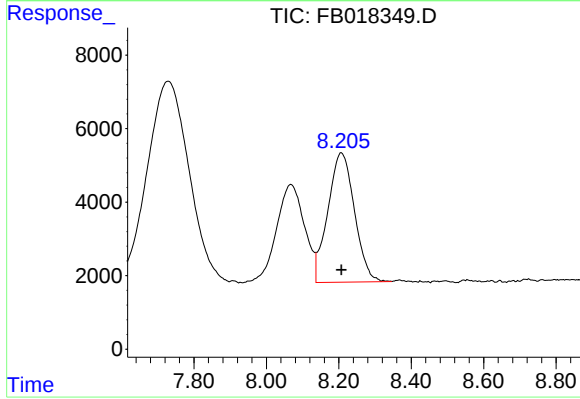


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 179711
Conc: 9.65 ng/ml

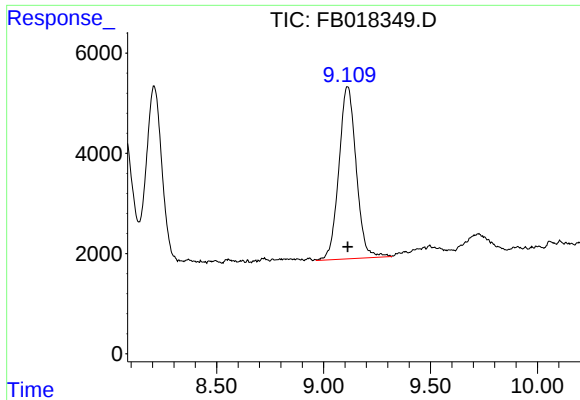


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 193048
Conc: 22.41 ng/ml

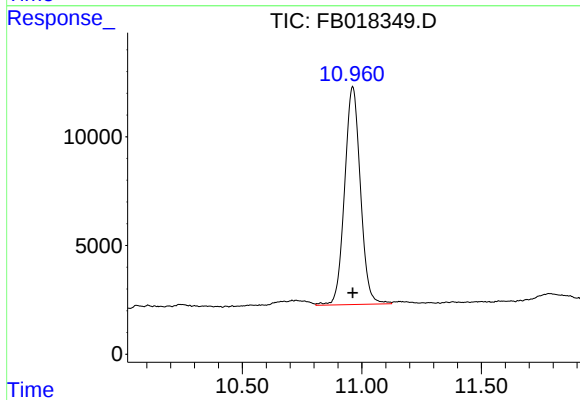


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 462588
Conc: 30.35 ng/ml

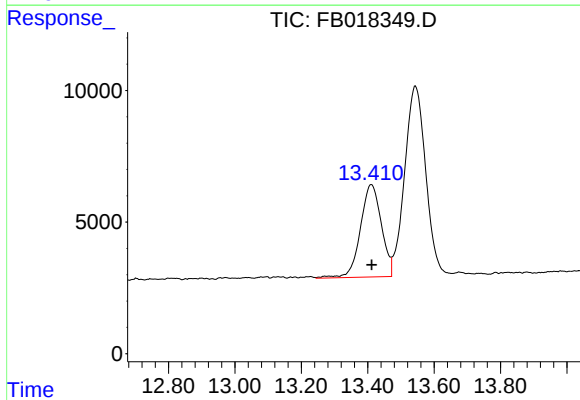


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 153561
Conc: 9.68 ng/ml

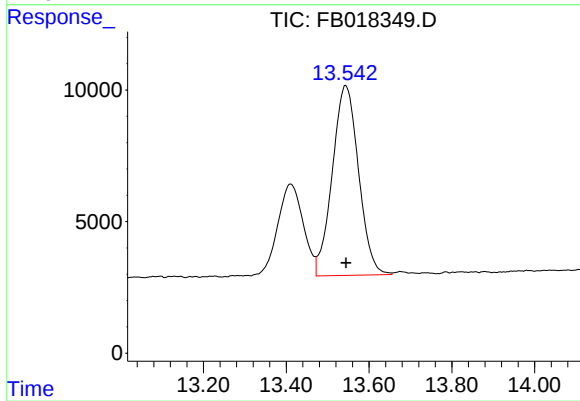

#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 317499
Conc: 19.08 ng/ml

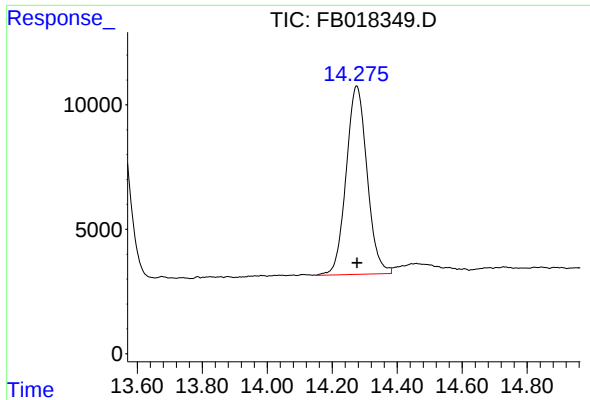


#9 O-Xylene

R.T.: 14.276 min

Delta R.T.: 0.000 min

Response: 338414

Conc: 18.98 ng/ml

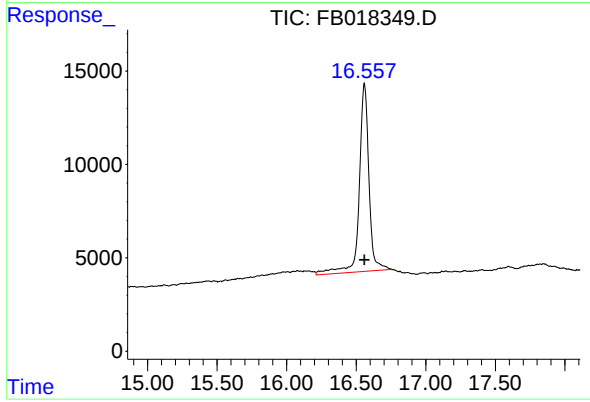

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min

Delta R.T.: 0.000 min

Response: 492308

Conc: 24.20 ng/ml