

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102418\
 Data File : FB018333.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2018 11:05
 Operator : MJ/SJ
 Sample : BSF1024S1
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 08:39:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	181659	21.092 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	480136	31.393 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	500088	33.843 ng/ml
3) t n-Heptane	8.066	164274	11.592 ng/ml
4) t Benzene	8.207	199369	10.702 ng/ml
6) t Toluene	10.960	495787	32.530 ng/ml
7) t Ethylbenzene	13.410	163661	10.315 ng/ml
8) t m-Xylene	13.542	343552	20.647 ng/ml
9) t O-Xylene	14.274	363213	20.371 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	434379	21.352 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102418\
Data File : FB018333.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2018 11:05
Operator : MJ/SJ
Sample : BSF1024S1
Misc : 5.03g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 08:39:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

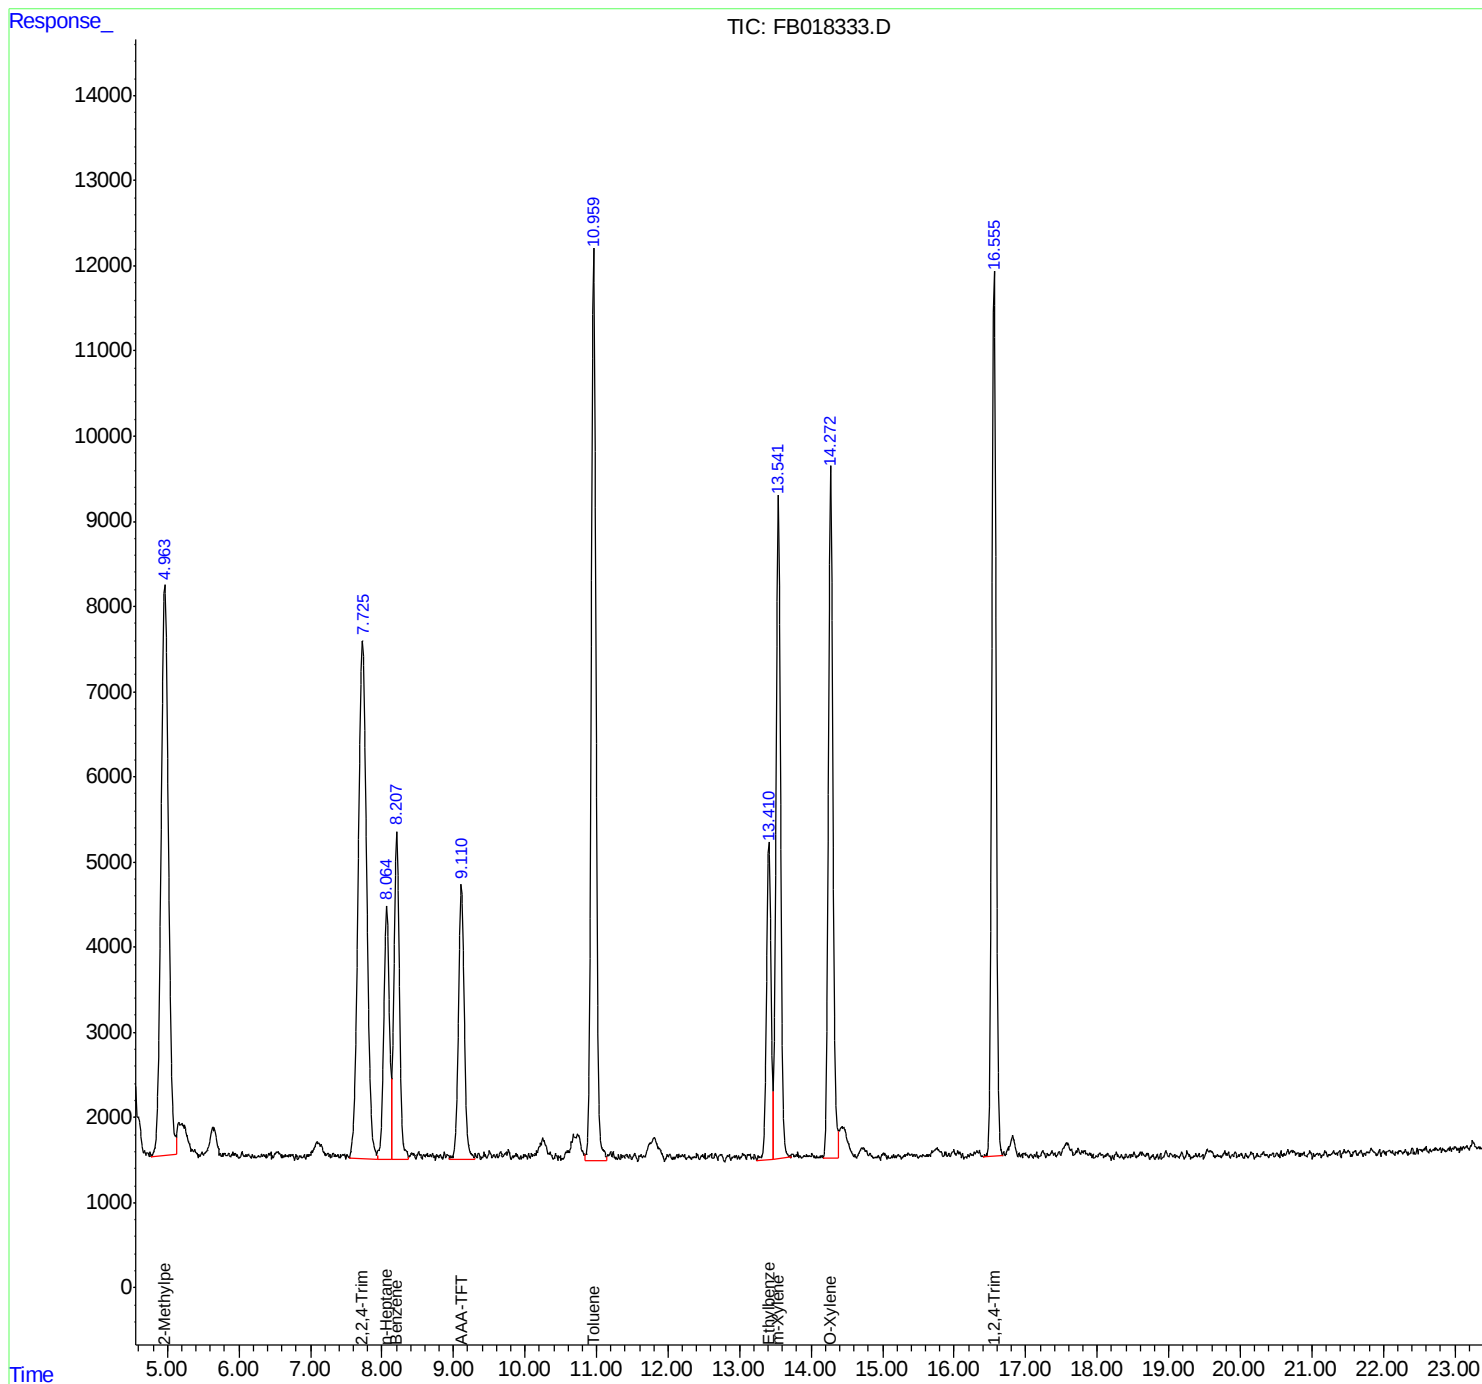

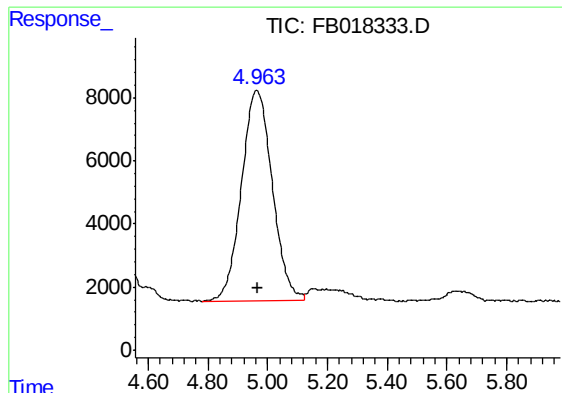


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 480136
Conc: 31.39 ng/ml

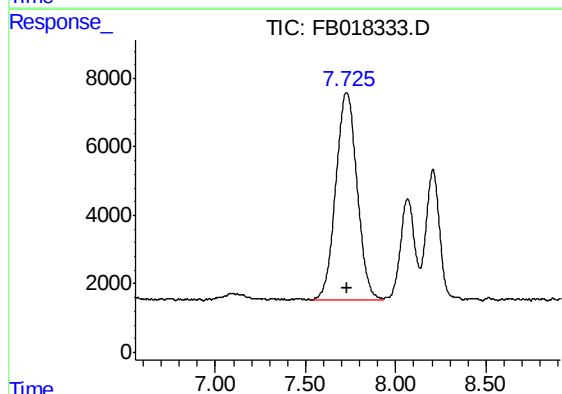


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: -0.001 min
Response: 500088
Conc: 33.84 ng/ml

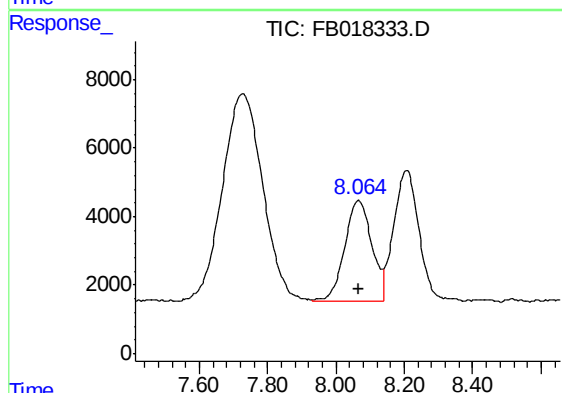


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 164274
Conc: 11.59 ng/ml

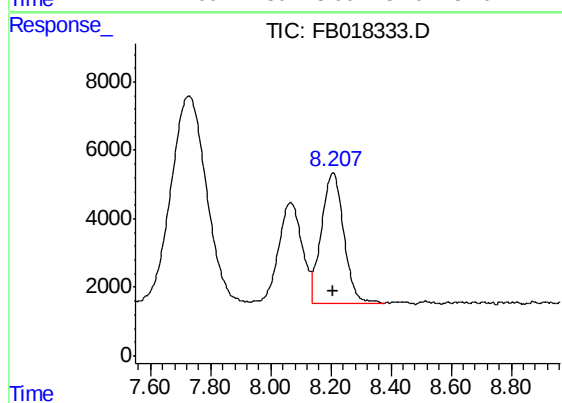


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 199369
Conc: 10.70 ng/ml

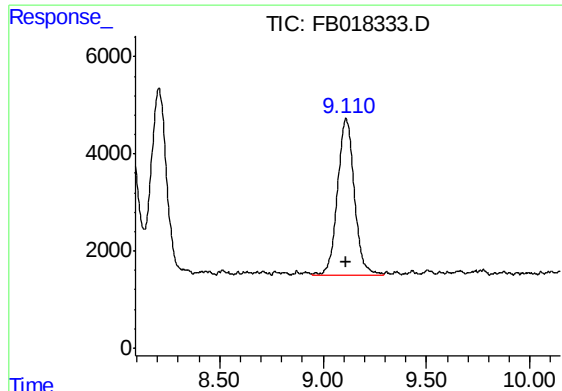


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 181659
Conc: 21.09 ng/ml

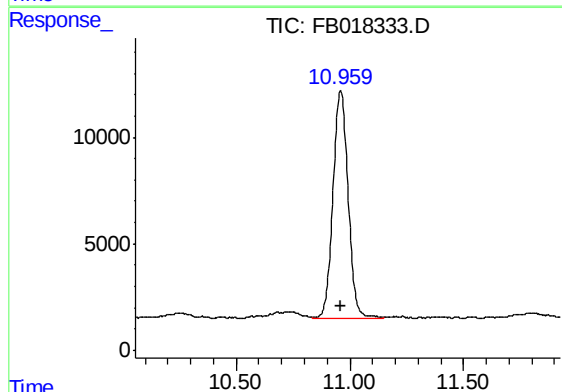


#6 Toluene

R.T.: 10.960 min
Delta R.T.: -0.002 min
Response: 495787
Conc: 32.53 ng/ml

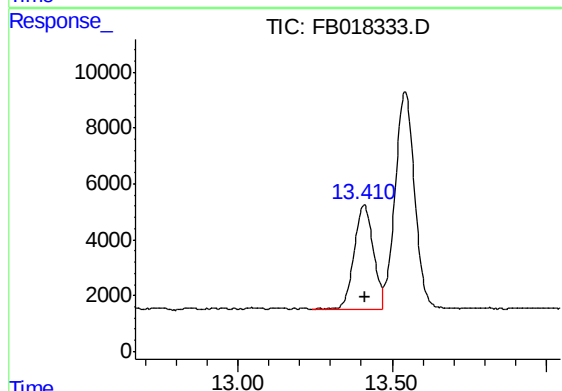


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.002 min
Response: 163661
Conc: 10.32 ng/ml

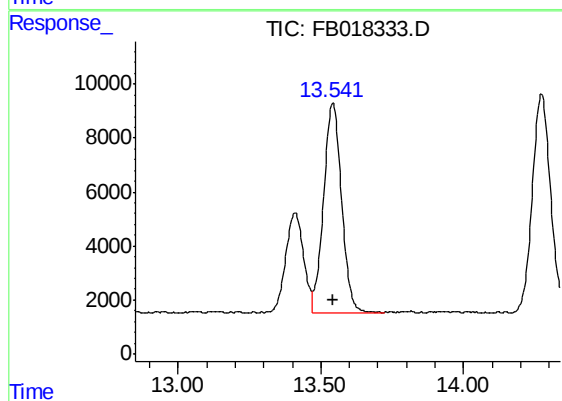


#8 m-Xylene

R.T.: 13.542 min
Delta R.T.: -0.002 min
Response: 343552
Conc: 20.65 ng/ml

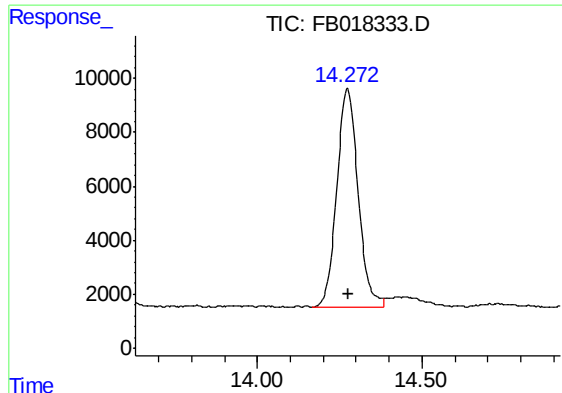

#9 O-Xylene

R.T.: 14.274 min
Delta R.T.: -0.002 min
Response: 363213
Conc: 20.37 ng/ml

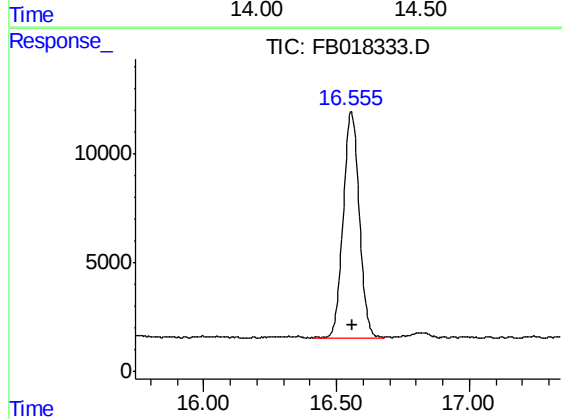

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: -0.003 min
Response: 434379
Conc: 21.35 ng/ml