

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
Data File : FB022820.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2019 11:58
Operator : DD/AJ
Sample : VBF1024S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 00:28:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	501843	19.832 ng/ml
Target Compounds				
6) t	Toluene	10.629	5031	0.117 ng/ml
8) t	m-Xylene	13.206	1657	0.043 ng/ml
9) t	O-Xylene	13.912	5273	0.145 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	5905	0.207 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
Data File : FB022820.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2019 11:58
Operator : DD/AJ
Sample : VBF1024S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 00:28:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

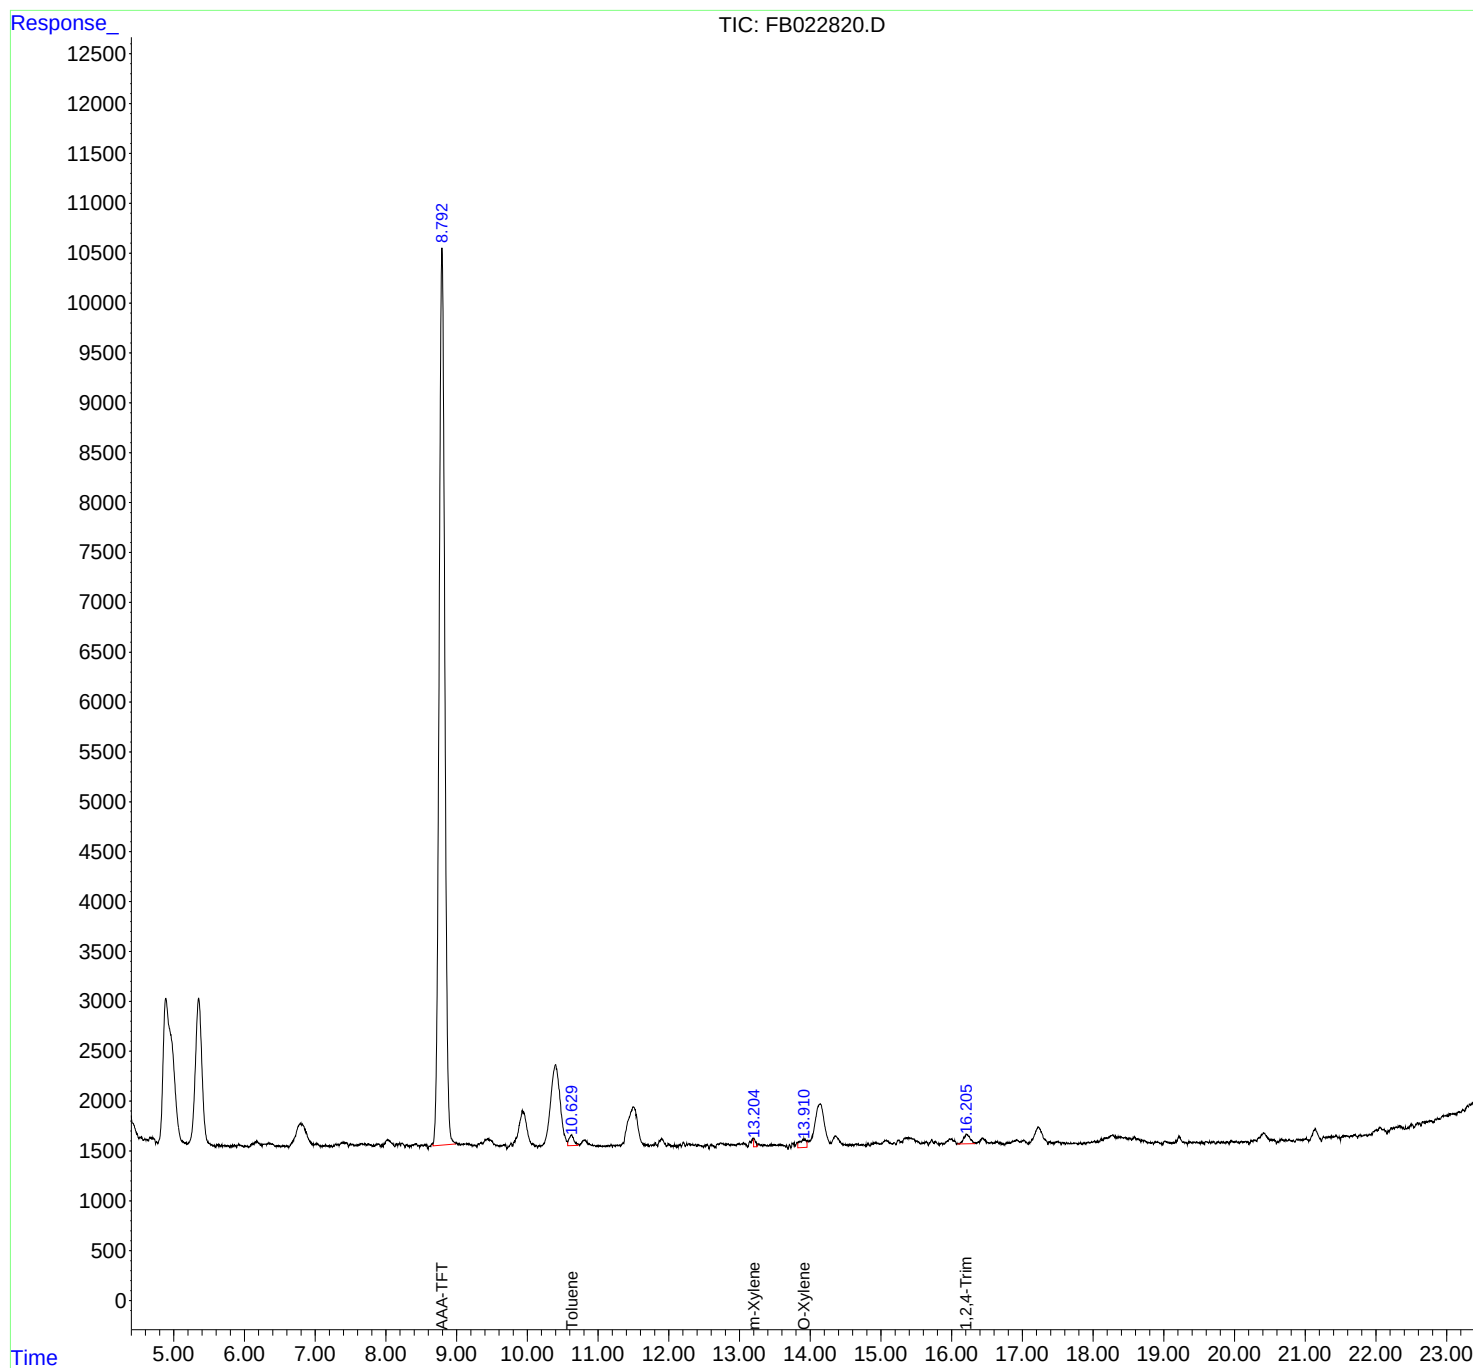

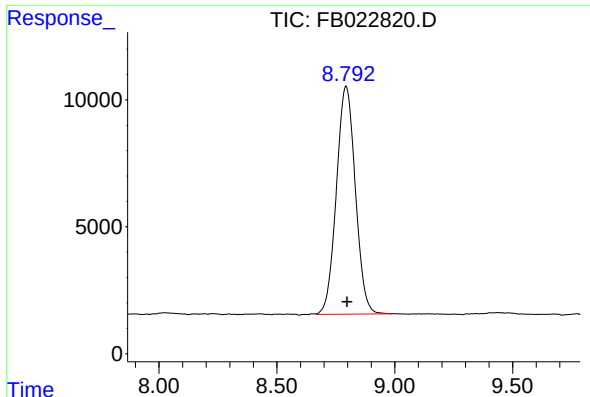


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 501843
Conc: 19.83 ng/ml

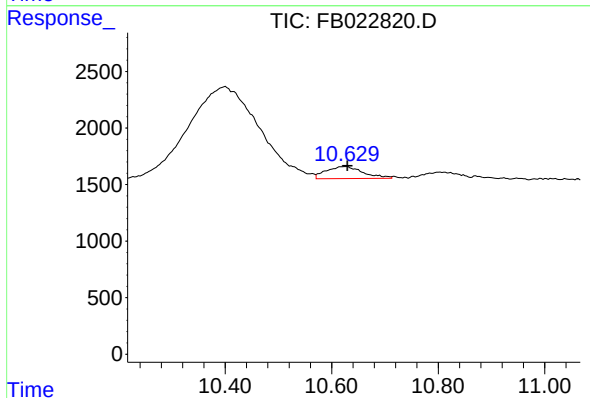


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 5031
Conc: 0.12 ng/ml

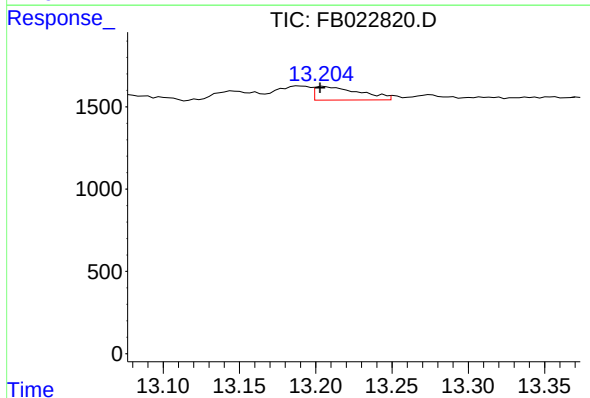


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.003 min
Response: 1657
Conc: 0.04 ng/ml

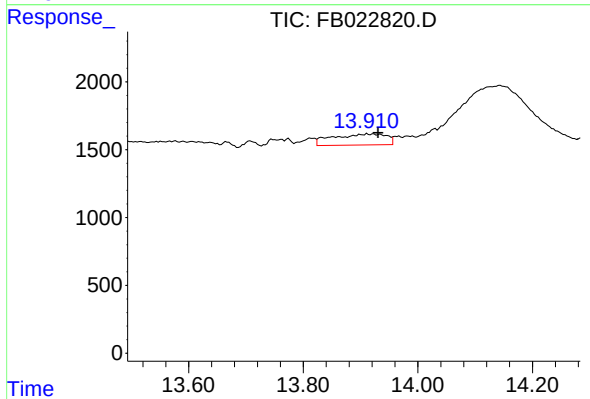

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.018 min
Response: 5273
Conc: 0.14 ng/ml

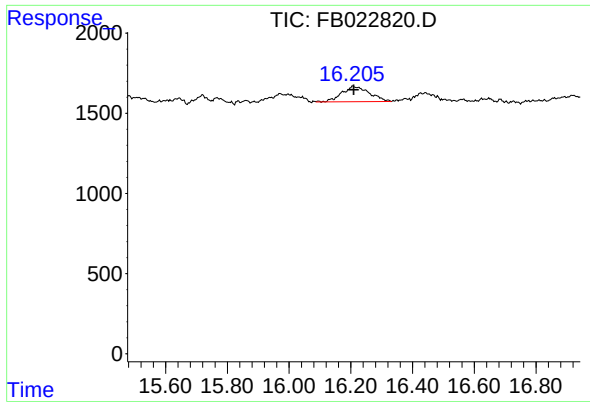

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 5905
Conc: 0.21 ng/ml